

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033920.D
 Acq On : 31 Jan 2024 14:58
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	11589	13891	1.84%	0.226%
2	1.281	68	75	88	rBV	103510	110934	14.69%	1.803%
3	1.439	113	124	130	rBV5	5680	8442	1.12%	0.137%
4	1.529	144	152	168	rVB	86884	105368	13.95%	1.712%
5	2.060	307	317	333	rVB	189784	273441	36.20%	4.444%
6	2.275	382	384	391	rBV2	142	181	0.02%	0.003%
7	2.449	430	438	447	rVB4	1115	1592	0.21%	0.026%
8	2.500	450	454	461	rVB2	230	293	0.04%	0.005%
9	2.535	461	465	468	rVB	195	174	0.02%	0.003%
10	2.587	478	481	489	rBV2	180	265	0.04%	0.004%
11	2.773	535	539	545	rVB2	219	285	0.04%	0.005%
12	2.854	561	564	569	rBV2	216	263	0.03%	0.004%
13	2.918	580	584	588	rBV	283	209	0.03%	0.003%
14	2.960	594	597	600	rVB	237	193	0.03%	0.003%
15	3.182	661	666	671	rBV2	183	179	0.02%	0.003%
16	3.252	684	688	693	rVB2	337	365	0.05%	0.006%
17	3.330	708	712	715	rBV	363	210	0.03%	0.003%
18	3.661	810	815	817	rBV2	181	181	0.02%	0.003%
19	3.783	845	853	887	rBV	46989	125953	16.67%	2.047%
20	4.059	936	939	942	rBV3	198	183	0.02%	0.003%
21	4.178	972	976	980	rBV3	249	276	0.04%	0.004%
22	4.246	981	997	1025	rBV	118140	300853	39.83%	4.889%
23	4.461	1062	1064	1068	rBV2	361	296	0.04%	0.005%
24	4.558	1091	1094	1098	rBV2	324	308	0.04%	0.005%
25	4.657	1121	1125	1127	rBV2	256	197	0.03%	0.003%
26	4.776	1159	1162	1166	rBV	253	221	0.03%	0.004%
27	4.876	1189	1193	1197	rVB2	331	365	0.05%	0.006%
28	4.899	1197	1200	1201	rBV2	316	223	0.03%	0.004%
29	4.953	1201	1217	1262	rVV2	285189	755377	100.00%	12.276%
30	5.304	1323	1326	1332	rBV2	406	380	0.05%	0.006%
31	5.362	1342	1344	1349	rVB	213	208	0.03%	0.003%
32	5.387	1349	1352	1355	rBV2	263	193	0.03%	0.003%
33	5.465	1373	1376	1380	rVV2	208	202	0.03%	0.003%
34	5.532	1385	1397	1430	rBV	282940	577316	76.43%	9.382%
35	5.828	1482	1489	1490	rBV3	1999	1847	0.24%	0.030%
36	5.985	1524	1538	1563	rBV	161868	335076	44.36%	5.446%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033920.D
 Acq On : 31 Jan 2024 14:58
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.439	1672	1679	1682	rBV2	312	494	0.07%	0.008%
38	6.538	1706	1710	1712	rBV	175	170	0.02%	0.003%
39	6.751	1773	1776	1778	rBV2	219	180	0.02%	0.003%
40	6.805	1788	1793	1799	rVB2	218	319	0.04%	0.005%
41	6.911	1816	1826	1849	rBV	94313	177288	23.47%	2.881%
42	7.185	1909	1911	1914	rBV2	282	177	0.02%	0.003%
43	7.243	1918	1929	1954	rBV	339848	606427	80.28%	9.855%
44	7.551	2016	2025	2051	rBV	65958	117061	15.50%	1.902%
45	7.773	2092	2094	2099	rBV2	147	173	0.02%	0.003%
46	7.850	2115	2118	2121	rVV2	208	179	0.02%	0.003%
47	8.021	2162	2171	2216	rBV	162474	323272	42.80%	5.254%
48	8.226	2232	2235	2238	rBV2	330	204	0.03%	0.003%
49	8.291	2251	2255	2257	rBV3	353	319	0.04%	0.005%
50	8.310	2259	2261	2264	rVB	377	194	0.03%	0.003%
51	8.355	2274	2275	2279	rVB2	362	175	0.02%	0.003%
52	8.378	2279	2282	2287	rBV2	293	226	0.03%	0.004%
53	8.519	2320	2326	2328	rBV2	166	219	0.03%	0.004%
54	8.651	2363	2367	2373	rBV	122	189	0.03%	0.003%
55	8.728	2388	2391	2397	rBV	212	272	0.04%	0.004%
56	8.783	2397	2408	2437	rBV	423187	696448	92.20%	11.318%
57	9.024	2481	2483	2489	rVB2	313	269	0.04%	0.004%
58	9.062	2489	2495	2498	rBV	248	281	0.04%	0.005%
59	9.124	2510	2514	2516	rBV	219	207	0.03%	0.003%
60	9.358	2584	2587	2590	rBV2	194	188	0.02%	0.003%
61	9.400	2594	2600	2601	rBV	229	225	0.03%	0.004%
62	9.468	2617	2621	2625	rBV2	207	221	0.03%	0.004%
63	9.741	2702	2706	2711	rVB2	216	214	0.03%	0.003%
64	9.908	2753	2758	2763	rBV2	209	271	0.04%	0.004%
65	10.008	2786	2789	2795	rVB	242	187	0.02%	0.003%
66	10.046	2797	2801	2804	rVB2	264	227	0.03%	0.004%
67	10.069	2804	2808	2811	rBV2	215	170	0.02%	0.003%
68	10.152	2823	2834	2858	rBV	208988	329111	43.57%	5.349%
69	10.406	2909	2913	2916	rBV	261	254	0.03%	0.004%
70	10.603	2969	2974	2977	rBV2	266	292	0.04%	0.005%
71	10.792	3027	3033	3035	rBV2	198	236	0.03%	0.004%
72	11.027	3100	3106	3111	rBV2	199	339	0.04%	0.006%
73	11.072	3114	3120	3122	rBV2	209	199	0.03%	0.003%
74	11.185	3144	3155	3180	rBV	450670	708585	93.81%	11.516%
75	11.416	3224	3227	3231	rBV2	203	210	0.03%	0.003%
76	11.558	3260	3271	3291	rBV	356598	565763	74.90%	9.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033920.D
 Acq On : 31 Jan 2024 14:58
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.767	3334	3336	3340	rVB2	261	189	0.03%	0.003%
78	11.860	3361	3365	3370	rBV2	206	226	0.03%	0.004%
79	12.130	3444	3449	3451	rBV2	209	203	0.03%	0.003%
80	12.278	3490	3495	3500	rBV2	188	274	0.04%	0.004%
81	12.323	3505	3509	3512	rVB	235	179	0.02%	0.003%
82	12.345	3512	3516	3521	rBV2	180	268	0.04%	0.004%
83	12.799	3649	3657	3660	rBV2	267	387	0.05%	0.006%
84	12.902	3685	3689	3692	rBV	233	207	0.03%	0.003%
85	13.281	3803	3807	3811	rBV2	175	194	0.03%	0.003%
86	13.332	3819	3823	3827	rBV2	157	181	0.02%	0.003%
87	13.538	3882	3887	3890	rBV2	160	174	0.02%	0.003%
88	13.731	3944	3947	3950	rBV	218	195	0.03%	0.003%
89	13.757	3952	3955	3964	rVB2	301	385	0.05%	0.006%
90	13.969	4019	4021	4024	rBV	268	213	0.03%	0.003%
91	13.992	4026	4028	4033	rVB2	400	315	0.04%	0.005%
92	14.043	4040	4044	4046	rBV	259	176	0.02%	0.003%
93	14.075	4050	4054	4058	rBV3	361	285	0.04%	0.005%
94	14.184	4085	4088	4092	rVB2	293	224	0.03%	0.004%
95	14.220	4096	4099	4102	rBV2	252	219	0.03%	0.004%
96	14.313	4124	4128	4132	rBV2	329	365	0.05%	0.006%
97	14.397	4152	4154	4157	rBV	247	179	0.02%	0.003%
98	14.635	4224	4228	4231	rBV2	313	277	0.04%	0.005%
99	14.683	4241	4243	4247	rBV2	289	220	0.03%	0.004%
100	15.358	4449	4453	4454	rBV	410	323	0.04%	0.005%




Sum of corrected areas: 6153233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033920.D
Acq On : 31 Jan 2024 14:58
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

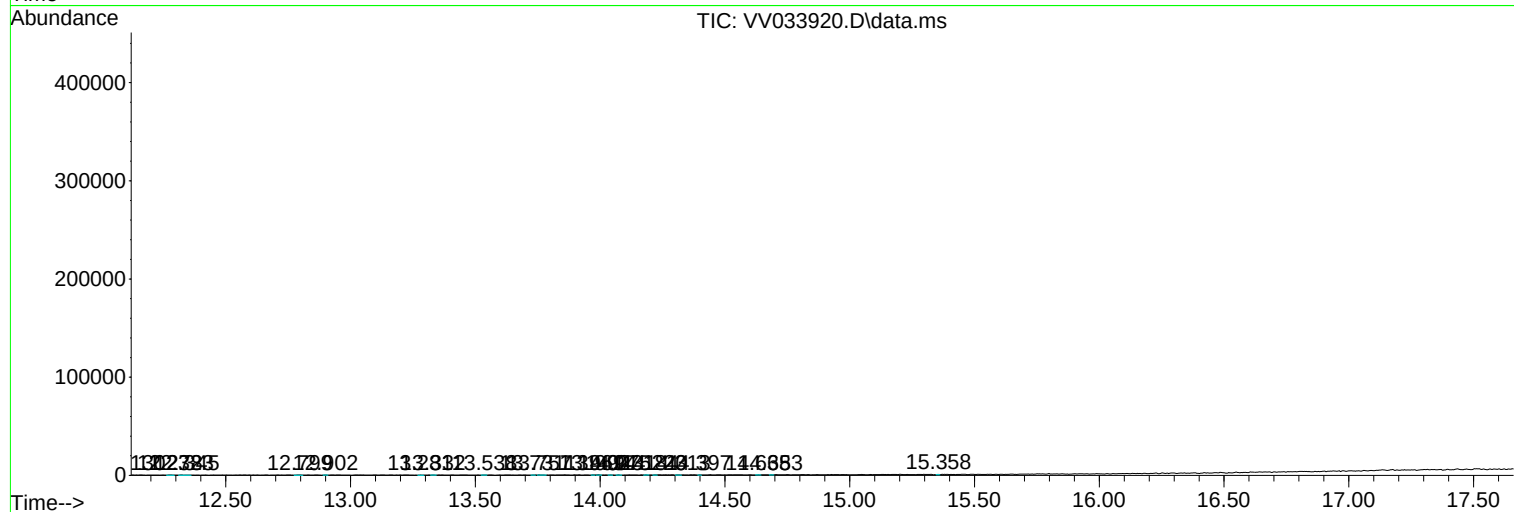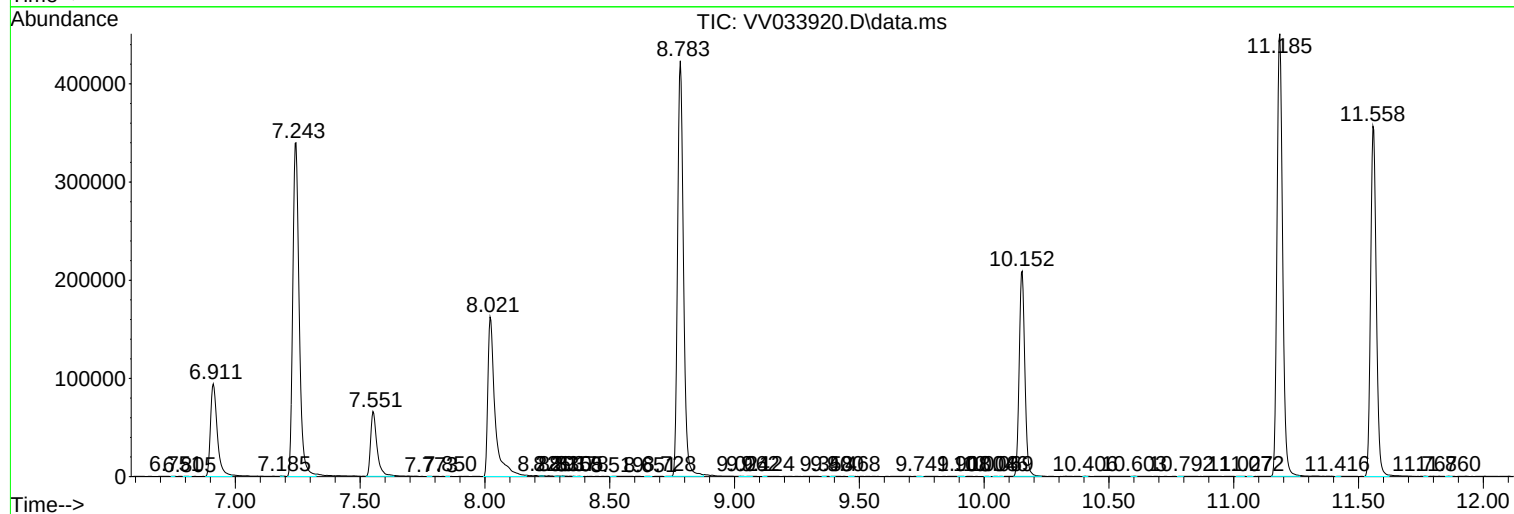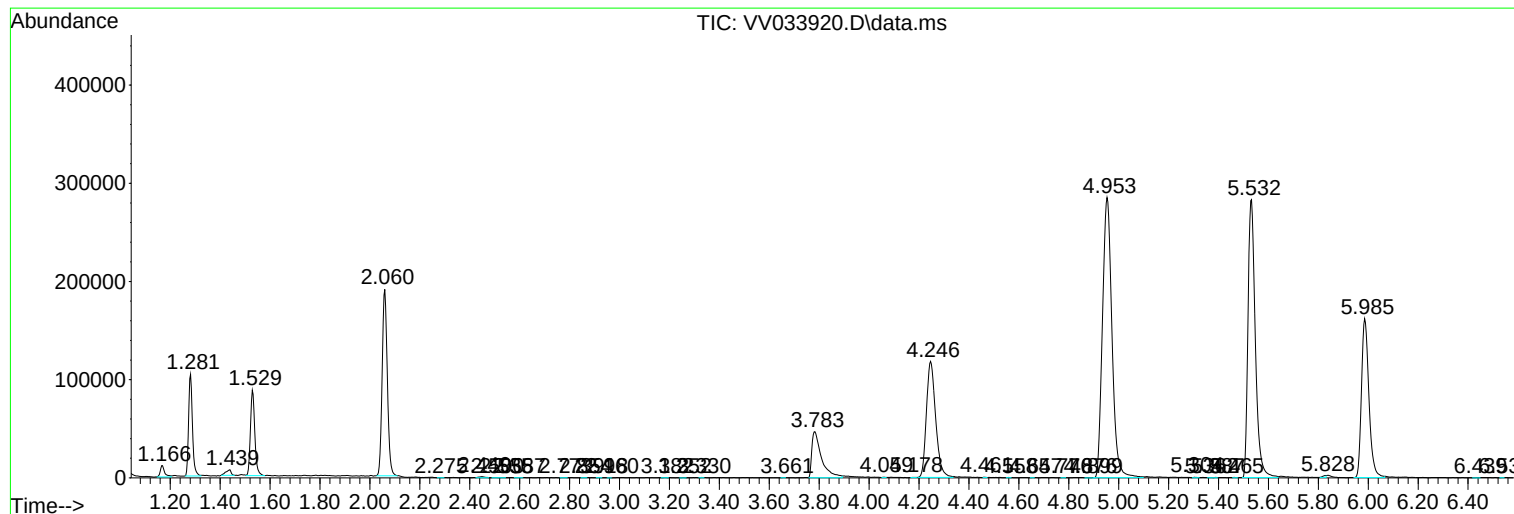

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033920.D
Acq On : 31 Jan 2024 14:58
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033920.D
Acq On : 31 Jan 2024 14:58
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc