

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033921.D
 Acq On : 31 Jan 2024 15:29
 Operator : SY/MD
 Sample : P1303-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	33	40	52	rBV	12425	15272	2.33%	0.301%
2	1.281	68	75	86	rBV	72242	75729	11.58%	1.492%
3	1.532	145	153	169	rBV	68360	81539	12.47%	1.606%
4	2.059	307	317	332	rBV	132414	195145	29.84%	3.844%
5	2.227	367	369	371	rVV	279	146	0.02%	0.003%
6	2.452	433	439	447	rVB3	1091	1743	0.27%	0.034%
7	2.561	463	473	482	rBV3	992	1958	0.30%	0.039%
8	2.748	527	531	536	rBV2	151	222	0.03%	0.004%
9	2.899	575	578	582	rBV2	184	168	0.03%	0.003%
10	2.982	600	604	608	rVB2	164	149	0.02%	0.003%
11	3.056	624	627	630	rBV	194	150	0.02%	0.003%
12	3.198	668	671	676	rVV2	176	191	0.03%	0.004%
13	3.252	684	688	693	rVB	164	187	0.03%	0.004%
14	3.317	706	708	711	rBV2	300	212	0.03%	0.004%
15	3.529	770	774	777	rBV2	146	176	0.03%	0.003%
16	3.616	797	801	802	rBV	215	169	0.03%	0.003%
17	3.635	805	807	810	rVV2	211	140	0.02%	0.003%
18	3.670	810	818	822	rVV2	203	341	0.05%	0.007%
19	3.706	825	829	834	rVB2	218	183	0.03%	0.004%
20	3.783	844	853	890	rVV	55652	151290	23.13%	2.980%
21	4.162	967	971	975	rBV2	220	253	0.04%	0.005%
22	4.249	981	998	1032	rBV	101902	260331	39.80%	5.128%
23	4.580	1096	1101	1105	rBV2	196	220	0.03%	0.004%
24	4.780	1159	1163	1166	rBV2	315	301	0.05%	0.006%
25	4.799	1166	1169	1172	rVB	180	169	0.03%	0.003%
26	4.953	1201	1217	1255	rBV2	241670	654051	100.00%	12.883%
27	5.297	1319	1324	1325	rBV	299	241	0.04%	0.005%
28	5.426	1361	1364	1367	rBV	170	170	0.03%	0.003%
29	5.532	1386	1397	1431	rBV	204584	422705	64.63%	8.326%
30	5.683	1442	1444	1447	rBV2	244	164	0.03%	0.003%
31	5.831	1483	1490	1501	rBV5	2218	4361	0.67%	0.086%
32	5.924	1516	1519	1522	rBV3	267	193	0.03%	0.004%
33	5.989	1523	1539	1573	rVV	145072	303406	46.39%	5.976%
34	6.130	1580	1583	1588	rBV4	238	251	0.04%	0.005%
35	6.317	1637	1641	1645	rVB2	356	406	0.06%	0.008%
36	6.345	1646	1650	1651	rBV	268	159	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033921.D
 Acq On : 31 Jan 2024 15:29
 Operator : SY/MD
 Sample : P1303-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.670	1747	1751	1757	rBV2	178	292	0.04%	0.006%
38	6.831	1798	1801	1805	rVB	278	245	0.04%	0.005%
39	6.854	1805	1808	1811	rBV2	324	337	0.05%	0.007%
40	6.911	1816	1826	1855	rBV	85533	160224	24.50%	3.156%
41	7.140	1894	1897	1902	rBV3	394	465	0.07%	0.009%
42	7.188	1908	1912	1914	rBV2	275	158	0.02%	0.003%
43	7.243	1918	1929	1957	rBV	272782	476973	72.93%	9.395%
44	7.551	2016	2025	2054	rBV	59186	108494	16.59%	2.137%
45	7.712	2072	2075	2077	rBV2	265	210	0.03%	0.004%
46	7.815	2103	2107	2111	rVB2	213	235	0.04%	0.005%
47	8.024	2162	2172	2212	rBV	172415	351168	53.69%	6.917%
48	8.204	2226	2228	2230	rBV2	473	161	0.02%	0.003%
49	8.268	2246	2248	2253	rVB3	439	321	0.05%	0.006%
50	8.361	2271	2277	2283	rVB3	661	912	0.14%	0.018%
51	8.394	2283	2287	2289	rBV	195	161	0.02%	0.003%
52	8.535	2327	2331	2333	rBV	268	228	0.03%	0.004%
53	8.738	2389	2394	2397	rBV2	209	254	0.04%	0.005%
54	8.783	2397	2408	2440	rBV	312946	517771	79.16%	10.199%
55	8.972	2462	2467	2470	rVB4	347	322	0.05%	0.006%
56	8.992	2470	2473	2476	rVB2	320	215	0.03%	0.004%
57	9.114	2507	2511	2515	rBV2	182	189	0.03%	0.004%
58	9.352	2581	2585	2591	rVB2	249	340	0.05%	0.007%
59	9.423	2603	2607	2610	rBV2	190	221	0.03%	0.004%
60	9.484	2623	2626	2629	rBV	178	169	0.03%	0.003%
61	10.152	2822	2834	2858	rBV	205718	327890	50.13%	6.459%
62	10.693	2998	3002	3007	rBV2	163	164	0.03%	0.003%
63	10.828	3039	3044	3047	rBV2	187	212	0.03%	0.004%
64	10.943	3076	3080	3084	rBV2	222	267	0.04%	0.005%
65	10.995	3092	3096	3101	rVB	205	191	0.03%	0.004%
66	11.101	3125	3129	3133	rVB	230	217	0.03%	0.004%
67	11.127	3133	3137	3139	rBV2	206	140	0.02%	0.003%
68	11.185	3144	3155	3181	rBV	324762	497089	76.00%	9.791%
69	11.352	3204	3207	3214	rVB3	249	305	0.05%	0.006%
70	11.561	3261	3272	3298	rBV	284804	451266	69.00%	8.889%
71	11.654	3298	3301	3304	rBV3	570	391	0.06%	0.008%
72	11.831	3353	3356	3359	rBV2	191	161	0.02%	0.003%
73	11.940	3388	3390	3396	rBV2	239	194	0.03%	0.004%
74	12.024	3411	3416	3419	rBV	236	238	0.04%	0.005%
75	12.130	3446	3449	3451	rBV2	210	140	0.02%	0.003%
76	12.172	3458	3462	3464	rBV	147	152	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033921.D
 Acq On : 31 Jan 2024 15:29
 Operator : SY/MD
 Sample : P1303-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.435	3538	3544	3546	rBV2	172	220	0.03%	0.004%
78	12.619	3598	3601	3606	rBV	153	165	0.03%	0.003%
79	12.664	3610	3615	3618	rVB2	188	183	0.03%	0.004%
80	12.689	3618	3623	3624	rBV	168	147	0.02%	0.003%
81	12.844	3669	3671	3674	rBV	230	187	0.03%	0.004%
82	12.911	3688	3692	3695	rBV2	211	190	0.03%	0.004%
83	12.985	3711	3715	3719	rBV2	183	153	0.02%	0.003%
84	13.017	3719	3725	3733	rBV	243	382	0.06%	0.008%
85	13.213	3783	3786	3789	rBV	150	157	0.02%	0.003%
86	13.281	3804	3807	3809	rBV	183	153	0.02%	0.003%
87	13.352	3825	3829	3831	rBV2	265	209	0.03%	0.004%
88	13.577	3896	3899	3902	rBV	216	181	0.03%	0.004%
89	13.676	3928	3930	3933	rVB	283	135	0.02%	0.003%
90	13.702	3933	3938	3941	rBV	220	211	0.03%	0.004%
91	13.779	3959	3962	3964	rBV2	196	136	0.02%	0.003%
92	13.934	4006	4010	4011	rBV2	241	145	0.02%	0.003%
93	14.188	4082	4089	4092	rVB2	339	349	0.05%	0.007%
94	14.210	4092	4096	4100	rBV2	276	338	0.05%	0.007%
95	14.278	4114	4117	4121	rBV3	226	226	0.03%	0.004%
96	14.377	4143	4148	4153	rVB2	253	323	0.05%	0.006%
97	14.532	4193	4196	4200	rBV2	215	162	0.02%	0.003%
98	15.139	4383	4385	4388	rBV3	265	179	0.03%	0.004%
99	15.175	4392	4396	4399	rBV3	384	336	0.05%	0.007%
100	15.368	4453	4456	4459	rBV3	511	402	0.06%	0.008%




Sum of corrected areas: 5076842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033921.D
Acq On : 31 Jan 2024 15:29
Operator : SY/MD
Sample : P1303-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

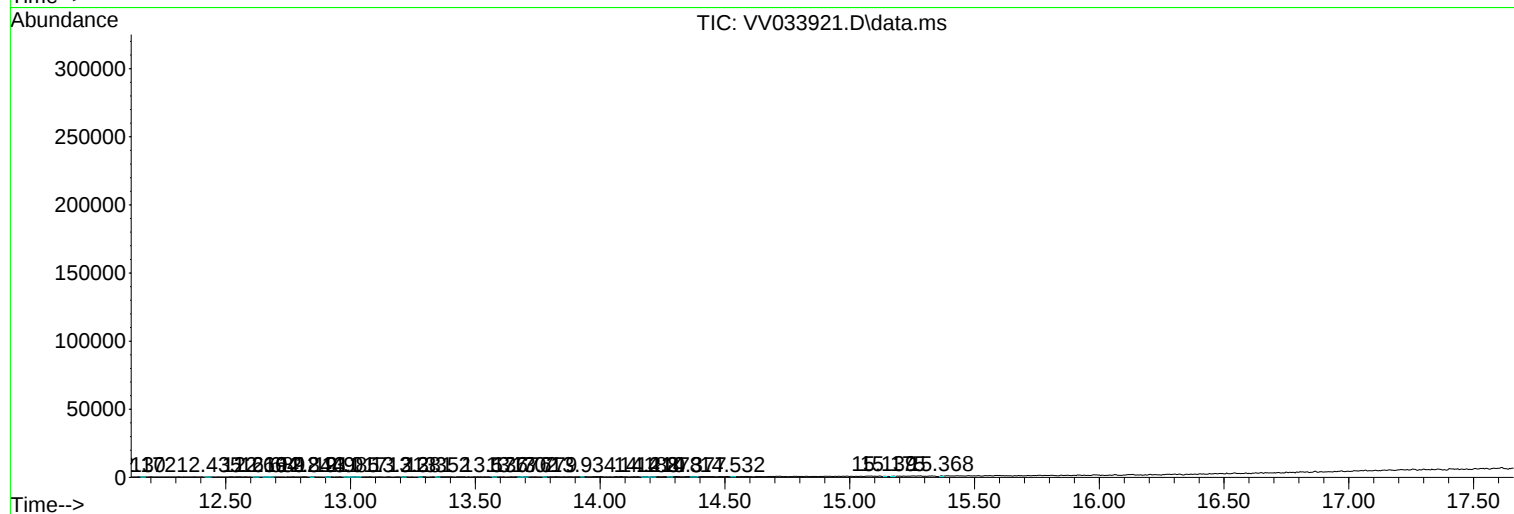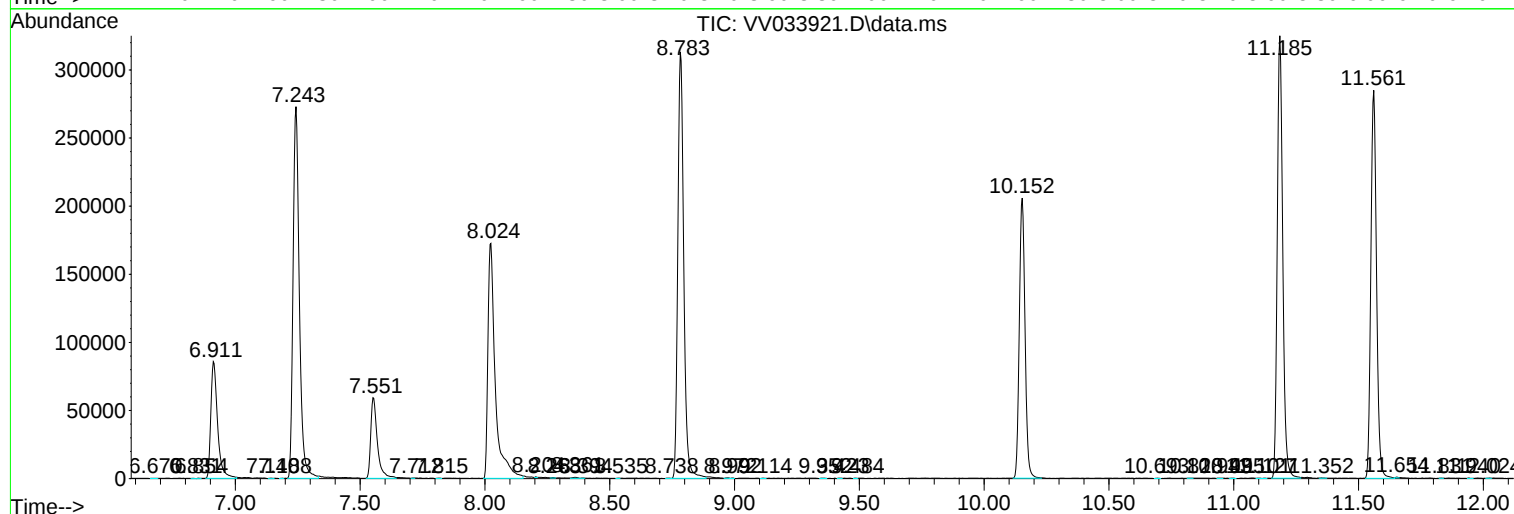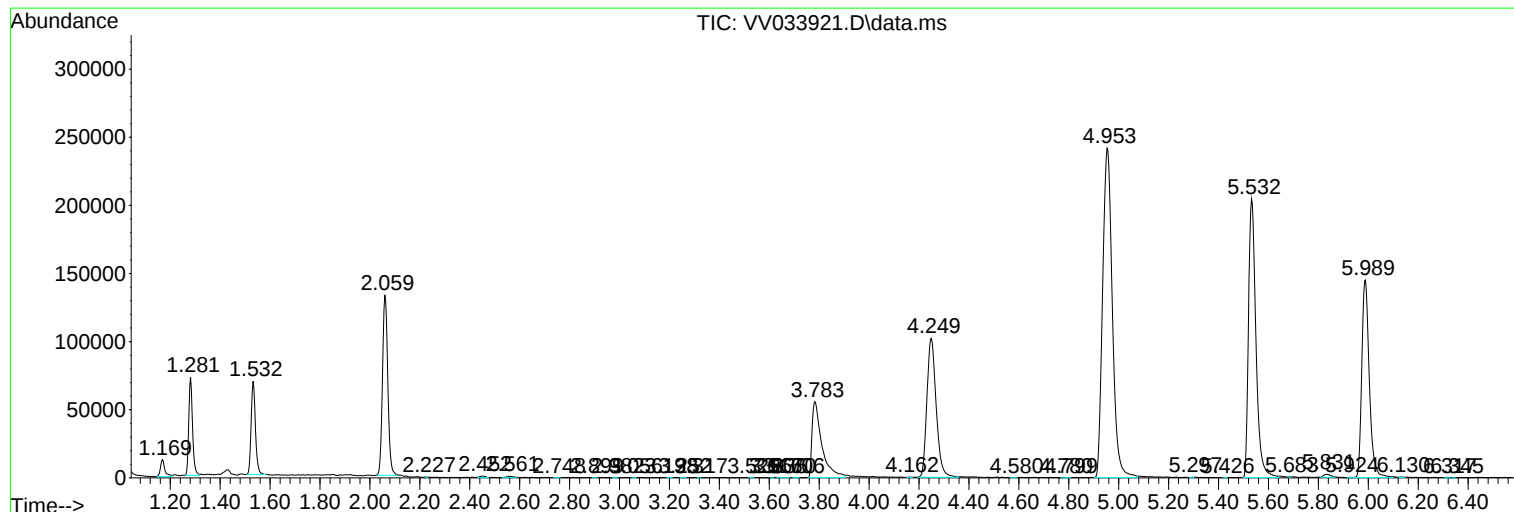

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033921.D
Acq On : 31 Jan 2024 15:29
Operator : SY/MD
Sample : P1303-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033921.D
Acq On : 31 Jan 2024 15:29
Operator : SY/MD
Sample : P1303-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------