

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033922.D
 Acq On : 31 Jan 2024 15:52
 Operator : SY/MD
 Sample : P1309-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	27	rVB	13998	14571	2.09%	0.253%
2	1.166	31	39	44	rBV	12967	14880	2.14%	0.258%
3	1.192	44	47	52	rVB	5660	4864	0.70%	0.084%
4	1.278	67	74	88	rBV	99767	111584	16.02%	1.938%
5	1.529	144	152	168	rBV	80113	98201	14.10%	1.706%
6	1.597	168	173	183	rVB3	3441	4630	0.66%	0.080%
7	2.060	306	317	329	rBV	171259	250519	35.97%	4.351%
8	2.298	384	391	396	rBV3	719	1002	0.14%	0.017%
9	2.458	436	441	442	rBV3	516	427	0.06%	0.007%
10	2.568	472	475	482	rVB	274	226	0.03%	0.004%
11	2.603	482	486	488	rBV	145	150	0.02%	0.003%
12	2.671	503	507	510	rVB2	163	170	0.02%	0.003%
13	2.690	510	513	519	rBV3	489	457	0.07%	0.008%
14	2.732	522	526	530	rBV2	216	265	0.04%	0.005%
15	2.970	594	600	605	rBV5	868	1152	0.17%	0.020%
16	3.163	656	660	662	rBV	206	174	0.02%	0.003%
17	3.233	679	682	684	rVB	291	146	0.02%	0.003%
18	3.320	705	709	714	rVB2	265	300	0.04%	0.005%
19	3.394	728	732	735	rBV	152	149	0.02%	0.003%
20	3.468	750	755	757	rBV2	155	176	0.03%	0.003%
21	3.497	760	764	766	rBV2	257	232	0.03%	0.004%
22	3.593	791	794	798	rBV	217	222	0.03%	0.004%
23	3.635	803	807	809	rBV2	224	181	0.03%	0.003%
24	3.783	845	853	889	rBV	49810	132104	18.97%	2.295%
25	4.188	977	979	982	rBV	210	169	0.02%	0.003%
26	4.249	982	998	1030	rVV	109292	280052	40.21%	4.864%
27	4.449	1057	1060	1065	rVB	283	197	0.03%	0.003%
28	4.481	1068	1070	1072	rVV	331	173	0.02%	0.003%
29	4.516	1076	1081	1082	rBV3	227	157	0.02%	0.003%
30	4.555	1090	1093	1095	rVV2	214	174	0.02%	0.003%
31	4.580	1099	1101	1103	rVV	247	163	0.02%	0.003%
32	4.593	1103	1105	1108	rVB2	323	184	0.03%	0.003%
33	4.613	1108	1111	1114	rVB2	271	166	0.02%	0.003%
34	4.642	1118	1120	1123	rVB	256	143	0.02%	0.002%
35	4.661	1123	1126	1129	rBV2	196	177	0.03%	0.003%
36	4.838	1179	1181	1184	rVB	299	151	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033922.D
Acq On : 31 Jan 2024 15:52
Operator : SY/MD
Sample : P1309-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis

37	4.957	1201	1218	1255	rBV2	263209	696539	100.00%	12.099%
38	5.365	1342	1345	1347	rBV2	285	210	0.03%	0.004%
39	5.532	1386	1397	1425	rBV	258382	525977	75.51%	9.136%
40	5.834	1484	1491	1504	rVB6	2149	4506	0.65%	0.078%
41	5.889	1504	1508	1511	rBV3	223	209	0.03%	0.004%
42	5.989	1527	1539	1573	rBV	153196	318233	45.69%	5.528%
43	6.275	1626	1628	1631	rVB2	280	173	0.02%	0.003%
44	6.381	1658	1661	1662	rBV	308	214	0.03%	0.004%
45	6.474	1687	1690	1695	rBV	161	185	0.03%	0.003%
46	6.732	1767	1770	1772	rBV2	172	136	0.02%	0.002%
47	6.818	1794	1797	1799	rBV	174	146	0.02%	0.003%
48	6.915	1816	1827	1851	rBV	89541	166353	23.88%	2.889%
49	7.156	1899	1902	1905	rBV	247	214	0.03%	0.004%
50	7.195	1912	1914	1918	rBV2	365	191	0.03%	0.003%
51	7.243	1918	1929	1952	rBV	313816	553029	79.40%	9.606%
52	7.551	2014	2025	2051	rBV	61459	111165	15.96%	1.931%
53	7.876	2119	2126	2131	rBV3	363	570	0.08%	0.010%
54	7.915	2131	2138	2146	rVB5	2356	3308	0.47%	0.057%
55	7.969	2146	2155	2158	rBV2	203	354	0.05%	0.006%
56	8.024	2163	2172	2215	rBV	168637	332881	47.79%	5.782%
57	8.400	2286	2289	2294	rVB2	216	172	0.02%	0.003%
58	8.487	2313	2316	2321	rBV	161	192	0.03%	0.003%
59	8.567	2337	2341	2342	rBV2	181	148	0.02%	0.003%
60	8.783	2397	2408	2433	rBV	388273	639358	91.79%	11.105%
61	9.088	2497	2503	2504	rBV2	354	373	0.05%	0.006%
62	9.130	2512	2516	2518	rBV2	170	169	0.02%	0.003%
63	9.233	2545	2548	2551	rBV	194	180	0.03%	0.003%
64	9.329	2574	2578	2583	rVB	256	279	0.04%	0.005%
65	9.362	2583	2588	2591	rBV2	191	173	0.02%	0.003%
66	9.654	2676	2679	2682	rBV	165	164	0.02%	0.003%
67	9.854	2736	2741	2746	rBV2	257	331	0.05%	0.006%
68	9.953	2767	2772	2774	rBV2	145	174	0.02%	0.003%
69	10.153	2823	2834	2859	rBV	206658	324843	46.64%	5.642%
70	10.313	2881	2884	2886	rBV	268	206	0.03%	0.004%
71	10.329	2886	2889	2891	rVB2	361	206	0.03%	0.004%
72	10.484	2934	2937	2943	rVB	272	236	0.03%	0.004%
73	11.075	3118	3121	3123	rBV2	216	161	0.02%	0.003%
74	11.101	3126	3129	3133	rBV2	494	482	0.07%	0.008%
75	11.185	3144	3155	3179	rVV	409095	633131	90.90%	10.997%
76	11.365	3207	3211	3214	rBV2	197	178	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033922.D
 Acq On : 31 Jan 2024 15:52
 Operator : SY/MD
 Sample : P1309-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.413	3223	3226	3232	rVB2	201	230	0.03%	0.004%
78	11.455	3236	3239	3242	rBV	209	170	0.02%	0.003%
79	11.561	3260	3272	3299	rBV	328786	515434	74.00%	8.953%
80	11.718	3318	3321	3324	rBV2	204	143	0.02%	0.002%
81	11.915	3378	3382	3385	rBV2	266	261	0.04%	0.005%
82	11.982	3398	3403	3409	rBV2	247	407	0.06%	0.007%
83	12.172	3458	3462	3465	rBV2	253	244	0.04%	0.004%
84	12.300	3496	3502	3511	rBV5	2213	3141	0.45%	0.055%
85	12.599	3592	3595	3599	rBV2	174	148	0.02%	0.003%
86	12.834	3666	3668	3674	rVB2	168	157	0.02%	0.003%
87	12.863	3674	3677	3682	rBV2	175	190	0.03%	0.003%
88	13.079	3742	3744	3750	rVB	213	163	0.02%	0.003%
89	13.136	3758	3762	3765	rBV2	143	140	0.02%	0.002%
90	13.175	3770	3774	3776	rBV2	183	175	0.03%	0.003%
91	13.210	3784	3785	3791	rVB2	228	165	0.02%	0.003%
92	13.259	3797	3800	3804	rBV	158	139	0.02%	0.002%
93	13.506	3874	3877	3880	rBV	184	173	0.02%	0.003%
94	13.789	3963	3965	3974	rBV2	194	217	0.03%	0.004%
95	13.876	3990	3992	3996	rBV2	202	158	0.02%	0.003%
96	13.947	4011	4014	4017	rBV2	225	176	0.03%	0.003%
97	14.185	4085	4088	4089	rBV2	425	203	0.03%	0.004%
98	14.297	4120	4123	4127	rBV2	237	205	0.03%	0.004%
99	14.834	4288	4290	4293	rVB	361	174	0.02%	0.003%
100	15.059	4358	4360	4364	rBV3	362	168	0.02%	0.003%




Sum of corrected areas: 5757218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033922.D
Acq On : 31 Jan 2024 15:52
Operator : SY/MD
Sample : P1309-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

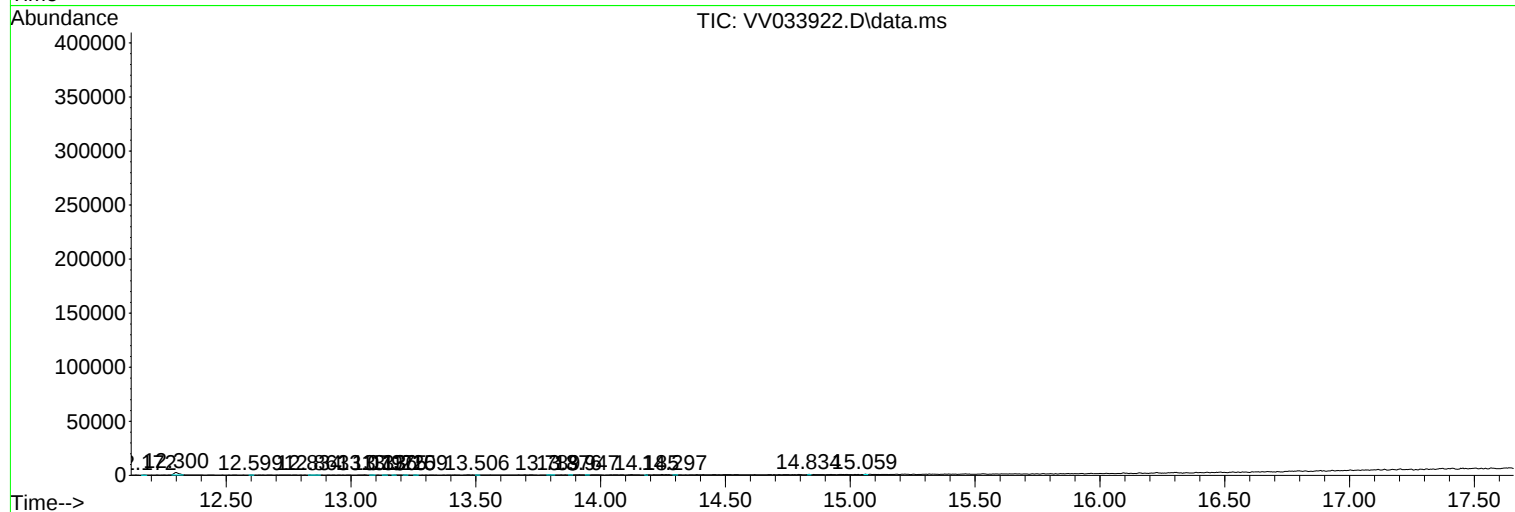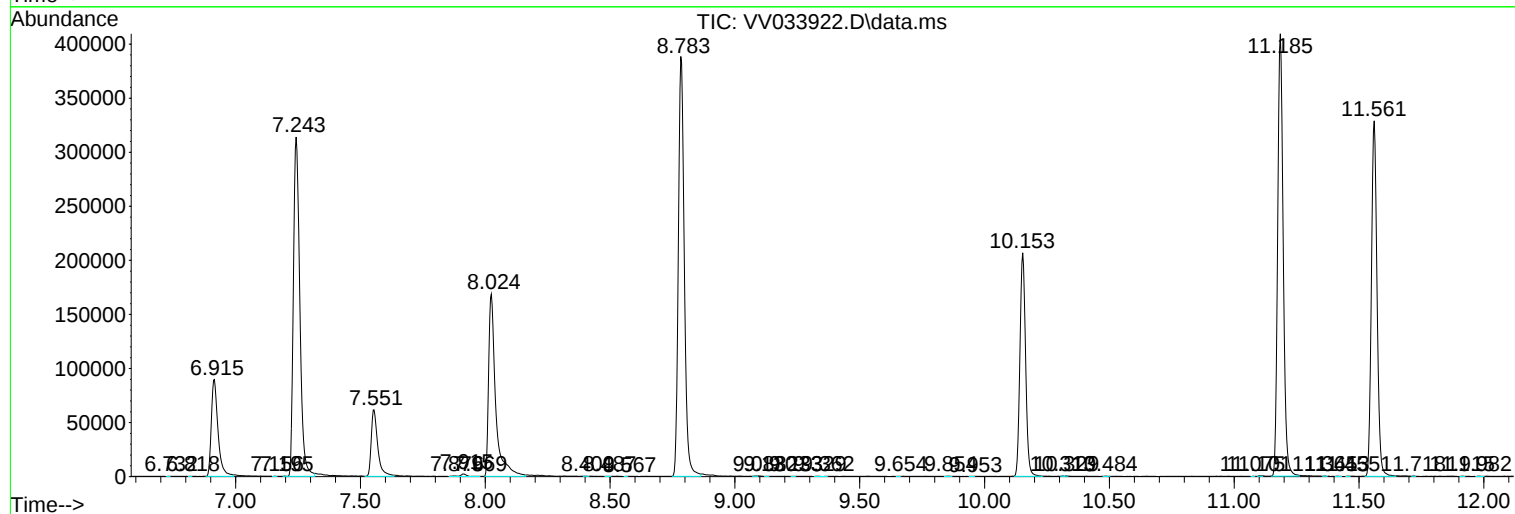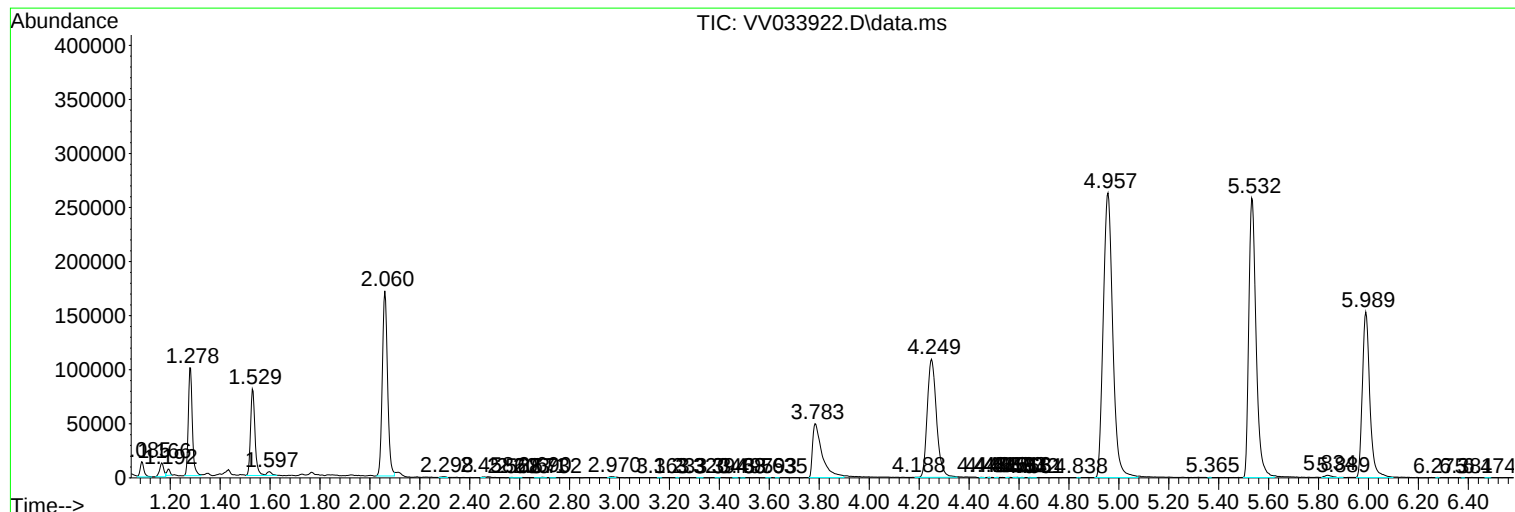

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033922.D
Acq On : 31 Jan 2024 15:52
Operator : SY/MD
Sample : P1309-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033922.D
Acq On : 31 Jan 2024 15:52
Operator : SY/MD
Sample : P1309-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------