

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033923.D
 Acq On : 31 Jan 2024 16:16
 Operator : SY/MD
 Sample : P1309-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH902

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	22	rVB2	5551	5718	0.81%	0.100%
2	1.166	32	39	44	rBV	11750	12874	1.83%	0.224%
3	1.278	68	74	88	rBV	96227	105028	14.89%	1.828%
4	1.529	144	152	165	rVB	79173	97116	13.77%	1.690%
5	1.835	242	247	259	rVB4	2080	3783	0.54%	0.066%
6	2.060	307	317	339	rBV	174956	256547	36.37%	4.464%
7	2.224	364	368	369	rBV	278	190	0.03%	0.003%
8	2.233	369	371	374	rVB2	292	159	0.02%	0.003%
9	2.429	429	432	435	rBV2	174	157	0.02%	0.003%
10	2.452	436	439	442	rVV	367	270	0.04%	0.005%
11	2.478	442	447	454	rVB2	391	534	0.08%	0.009%
12	2.950	589	594	598	rVV	149	206	0.03%	0.004%
13	2.979	598	603	608	rVV2	253	300	0.04%	0.005%
14	3.085	630	636	641	rBV2	206	295	0.04%	0.005%
15	3.182	663	666	669	rVB2	226	162	0.02%	0.003%
16	3.220	674	678	681	rBV	183	176	0.02%	0.003%
17	3.291	697	700	704	rBV	254	250	0.04%	0.004%
18	3.336	711	714	719	rBV2	190	187	0.03%	0.003%
19	3.362	719	722	726	rBV	170	178	0.03%	0.003%
20	3.426	739	742	747	rVB2	185	161	0.02%	0.003%
21	3.635	804	807	811	rBV2	230	214	0.03%	0.004%
22	3.677	811	820	823	rBV2	224	344	0.05%	0.006%
23	3.754	838	844	845	rBV	312	278	0.04%	0.005%
24	3.783	845	853	890	rVV	49724	132483	18.78%	2.305%
25	4.249	982	998	1030	rBV	109907	282330	40.03%	4.913%
26	4.407	1044	1047	1051	rBV3	205	176	0.02%	0.003%
27	4.478	1064	1069	1072	rVB2	334	327	0.05%	0.006%
28	4.510	1072	1079	1081	rBV2	262	258	0.04%	0.004%
29	4.542	1085	1089	1095	rVB3	272	353	0.05%	0.006%
30	4.619	1110	1113	1116	rBV	245	162	0.02%	0.003%
31	4.770	1156	1160	1165	rBV	201	287	0.04%	0.005%
32	4.957	1201	1218	1252	rBV2	265193	705383	100.00%	12.275%
33	5.288	1319	1321	1325	rVB2	306	185	0.03%	0.003%
34	5.314	1325	1329	1332	rVB2	356	300	0.04%	0.005%
35	5.339	1332	1337	1341	rBV2	335	357	0.05%	0.006%
36	5.407	1355	1358	1363	rBV	189	187	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW013124\
 Data File : VW033923.D
 Acq On : 31 Jan 2024 16:16
 Operator : SY/MD
 Sample : P1309-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH902

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1431	rBV	255565	522350	74.05%	9.090%
38	5.838	1484	1492	1500	rBV5	1808	3613	0.51%	0.063%
39	5.989	1526	1539	1567	rVV	152052	317054	44.95%	5.517%
40	6.217	1607	1610	1613	rVB2	272	172	0.02%	0.003%
41	6.262	1619	1624	1627	rBV3	364	319	0.05%	0.006%
42	6.307	1636	1638	1642	rVB	295	236	0.03%	0.004%
43	6.339	1642	1648	1649	rBV2	190	221	0.03%	0.004%
44	6.751	1770	1776	1778	rBV	160	215	0.03%	0.004%
45	6.812	1791	1795	1799	rBV2	205	214	0.03%	0.004%
46	6.915	1816	1827	1851	rBV	90564	168205	23.85%	2.927%
47	7.140	1892	1897	1902	rVB2	337	388	0.06%	0.007%
48	7.243	1918	1929	1962	rBV	322032	564239	79.99%	9.819%
49	7.555	2016	2026	2065	rVV2	60942	112904	16.01%	1.965%
50	7.876	2122	2126	2133	rVB2	581	861	0.12%	0.015%
51	8.024	2163	2172	2218	rBV	170088	339653	48.15%	5.910%
52	8.722	2385	2389	2395	rBV2	177	240	0.03%	0.004%
53	8.783	2397	2408	2441	rBV	384034	630195	89.34%	10.966%
54	8.969	2463	2466	2471	rVB4	342	302	0.04%	0.005%
55	9.030	2480	2485	2489	rBV2	234	339	0.05%	0.006%
56	9.461	2615	2619	2620	rBV2	447	265	0.04%	0.005%
57	9.493	2625	2629	2633	rVV4	170	182	0.03%	0.003%
58	9.731	2698	2703	2706	rBV2	234	250	0.04%	0.004%
59	10.024	2790	2794	2798	rBV	162	175	0.02%	0.003%
60	10.059	2800	2805	2807	rBV2	164	178	0.03%	0.003%
61	10.153	2822	2834	2859	rBV	209887	327186	46.38%	5.693%
62	10.243	2860	2862	2866	rVV2	348	217	0.03%	0.004%
63	10.320	2881	2886	2887	rBV2	452	382	0.05%	0.007%
64	10.407	2907	2913	2915	rBV2	167	191	0.03%	0.003%
65	10.439	2919	2923	2925	rBV	152	153	0.02%	0.003%
66	10.535	2949	2953	2955	rBV2	196	152	0.02%	0.003%
67	10.564	2959	2962	2966	rBV2	188	163	0.02%	0.003%
68	10.587	2966	2969	2972	rVB	248	190	0.03%	0.003%
69	10.902	3061	3067	3069	rBV2	164	188	0.03%	0.003%
70	10.940	3074	3079	3081	rBV	181	181	0.03%	0.003%
71	11.185	3144	3155	3185	rVV	403407	621831	88.16%	10.821%
72	11.313	3192	3195	3198	rBV3	289	182	0.03%	0.003%
73	11.561	3258	3272	3295	rBV	328711	518962	73.57%	9.031%
74	11.770	3331	3337	3340	rBV2	241	257	0.04%	0.004%
75	11.905	3376	3379	3382	rBV2	167	150	0.02%	0.003%
76	12.005	3407	3410	3411	rBV	244	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033923.D
 Acq On : 31 Jan 2024 16:16
 Operator : SY/MD
 Sample : P1309-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH902

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.062	3425	3428	3430	rBV2	191	150	0.02%	0.003%
78	12.107	3438	3442	3445	rBV2	190	163	0.02%	0.003%
79	12.210	3470	3474	3478	rBV2	237	286	0.04%	0.005%
80	12.284	3492	3497	3501	rBV2	191	205	0.03%	0.004%
81	12.323	3501	3509	3513	rBV2	493	557	0.08%	0.010%
82	12.583	3582	3590	3592	rBV2	215	284	0.04%	0.005%
83	12.776	3648	3650	3655	rVB2	187	153	0.02%	0.003%
84	12.802	3655	3658	3662	rBV2	208	224	0.03%	0.004%
85	12.914	3690	3693	3698	rVB2	289	236	0.03%	0.004%
86	12.940	3698	3701	3703	rBV2	187	157	0.02%	0.003%
87	12.985	3712	3715	3717	rBV	217	156	0.02%	0.003%
88	13.066	3735	3740	3741	rBV	179	170	0.02%	0.003%
89	13.307	3812	3815	3821	rVB2	273	305	0.04%	0.005%
90	13.384	3837	3839	3843	rBV2	175	170	0.02%	0.003%
91	13.496	3871	3874	3877	rBB2	281	190	0.03%	0.003%
92	13.857	3983	3986	3989	rBV2	251	170	0.02%	0.003%
93	14.123	4066	4069	4071	rBV2	322	227	0.03%	0.004%
94	14.471	4172	4177	4179	rBV2	197	236	0.03%	0.004%
95	14.519	4188	4192	4195	rVB2	225	194	0.03%	0.003%
96	14.538	4195	4198	4200	rBV3	238	176	0.02%	0.003%
97	14.873	4299	4302	4308	rBV2	346	315	0.04%	0.005%
98	14.902	4308	4311	4312	rBV2	282	181	0.03%	0.003%
99	14.930	4318	4320	4322	rBV	363	182	0.03%	0.003%
100	15.406	4465	4468	4471	rBV2	378	337	0.05%	0.006%




Sum of corrected areas: 5746664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033923.D
Acq On : 31 Jan 2024 16:16
Operator : SY/MD
Sample : P1309-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH902

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

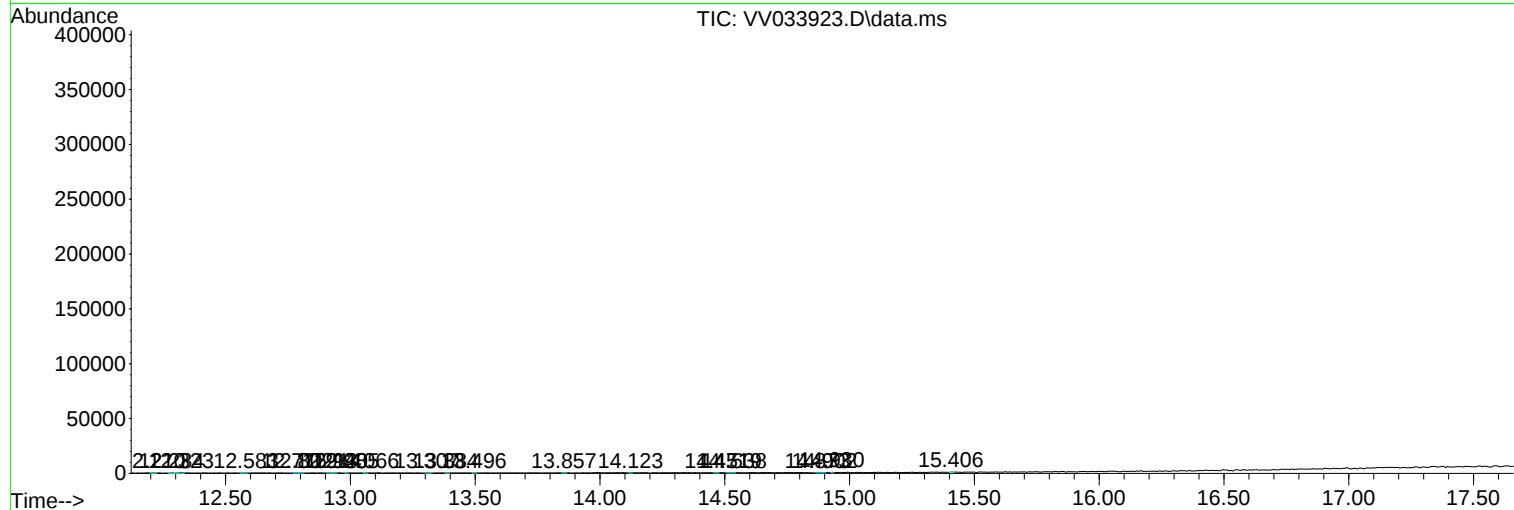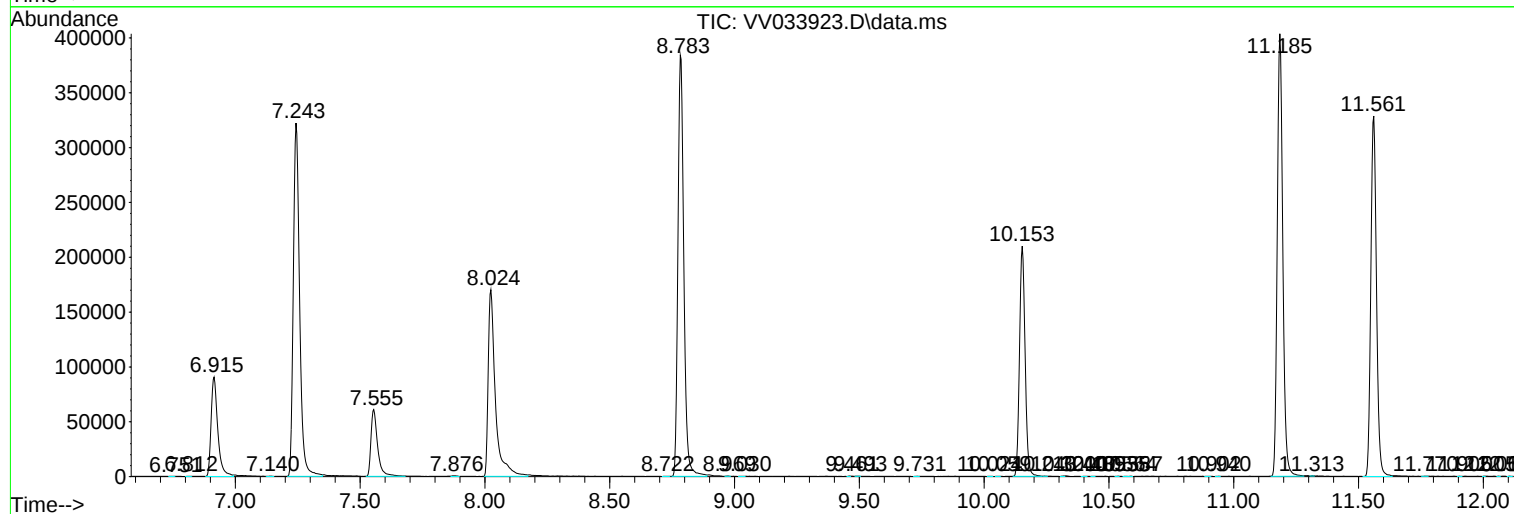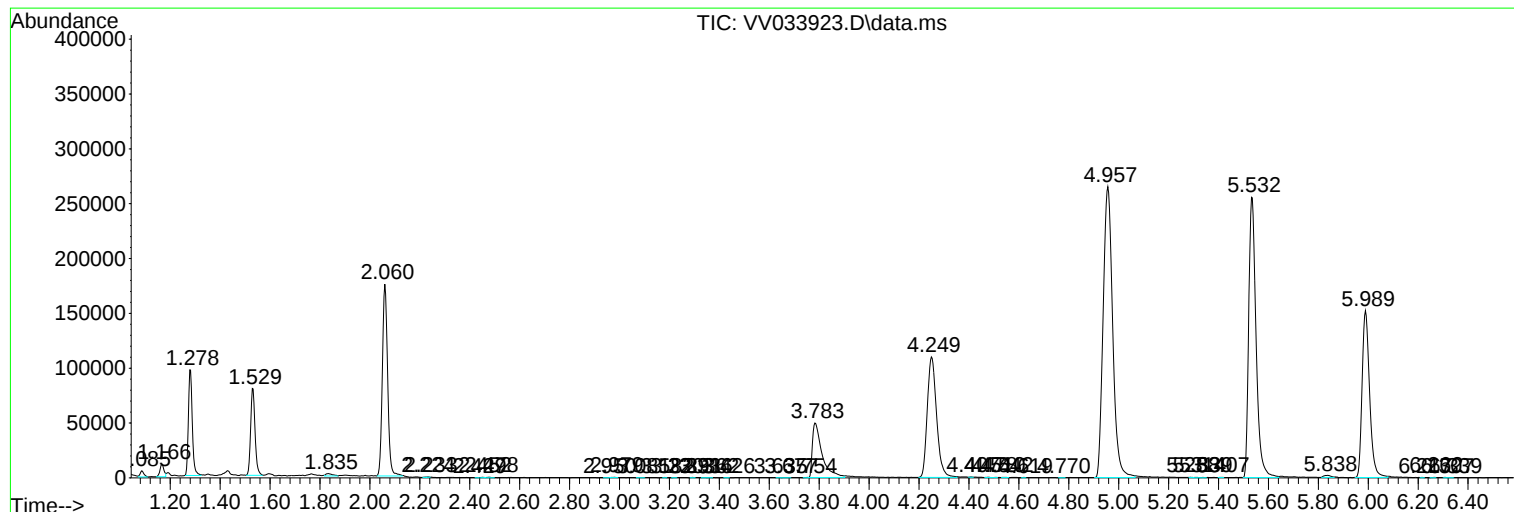

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033923.D
Acq On : 31 Jan 2024 16:16
Operator : SY/MD
Sample : P1309-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH902

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033923.D
Acq On : 31 Jan 2024 16:16
Operator : SY/MD
Sample : P1309-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH902

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc