

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033924.D
 Acq On : 31 Jan 2024 16:40
 Operator : SY/MD
 Sample : P1309-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	8	14	27	rVB	18454	19222	2.73%	0.334%
2	1.166	33	39	44	rBV	10976	11804	1.67%	0.205%
3	1.282	66	75	88	rBV	102693	115374	16.37%	2.008%
4	1.429	112	121	127	rBV7	4116	6460	0.92%	0.112%
5	1.529	144	152	167	rVB	81137	98541	13.98%	1.715%
6	2.060	306	317	329	rBV	170231	248675	35.28%	4.327%
7	2.224	363	368	369	rBV2	285	216	0.03%	0.004%
8	2.391	415	420	423	rVV2	232	217	0.03%	0.004%
9	2.407	423	425	430	rVB2	236	207	0.03%	0.004%
10	2.442	434	436	439	rVV2	401	293	0.04%	0.005%
11	2.773	536	539	541	rBV	192	153	0.02%	0.003%
12	2.812	547	551	556	rVB2	201	188	0.03%	0.003%
13	2.844	556	561	563	rBV2	156	175	0.02%	0.003%
14	2.880	568	572	574	rBV2	418	302	0.04%	0.005%
15	2.928	584	587	591	rVB2	186	162	0.02%	0.003%
16	2.986	602	605	611	rVB2	299	288	0.04%	0.005%
17	3.018	611	615	619	rBV	223	247	0.04%	0.004%
18	3.224	676	679	683	rVB2	173	157	0.02%	0.003%
19	3.288	695	699	704	rBV2	336	435	0.06%	0.008%
20	3.648	807	811	813	rBV	223	199	0.03%	0.003%
21	3.751	840	843	845	rBV	201	169	0.02%	0.003%
22	3.783	845	853	886	rBV	48521	129165	18.33%	2.248%
23	4.060	936	939	945	rBV3	343	317	0.04%	0.006%
24	4.249	982	998	1025	rBV	109457	283331	40.20%	4.930%
25	4.497	1072	1075	1079	rVB2	312	248	0.04%	0.004%
26	4.632	1114	1117	1120	rBV	201	173	0.02%	0.003%
27	4.664	1123	1127	1129	rBV	334	174	0.02%	0.003%
28	4.957	1202	1218	1252	rBV2	264890	704852	100.00%	12.265%
29	5.162	1280	1282	1288	rBV3	282	213	0.03%	0.004%
30	5.436	1364	1367	1371	rBV2	199	198	0.03%	0.003%
31	5.494	1381	1385	1386	rBV2	257	179	0.03%	0.003%
32	5.532	1386	1397	1434	rBV	254494	520912	73.90%	9.064%
33	5.834	1484	1491	1504	rVB6	1909	3614	0.51%	0.063%
34	5.989	1526	1539	1572	rBV	153161	315839	44.81%	5.496%
35	6.127	1579	1582	1585	rBV2	275	195	0.03%	0.003%
36	6.240	1608	1617	1620	rBV	240	404	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033924.D
 Acq On : 31 Jan 2024 16:40
 Operator : SY/MD
 Sample : P1309-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.616	1728	1734	1737	rBV2	335	309	0.04%	0.005%
38	6.635	1737	1740	1745	rVV2	129	157	0.02%	0.003%
39	6.847	1802	1806	1809	rBV2	287	266	0.04%	0.005%
40	6.915	1816	1827	1860	rBV	88864	168352	23.88%	2.929%
41	7.104	1883	1886	1891	rVB3	367	323	0.05%	0.006%
42	7.172	1903	1907	1911	rVB2	395	270	0.04%	0.005%
43	7.243	1917	1929	1952	rBV	316385	559361	79.36%	9.733%
44	7.555	2017	2026	2051	rVV	60204	110390	15.66%	1.921%
45	7.866	2120	2123	2125	rBV2	279	213	0.03%	0.004%
46	8.024	2163	2172	2210	rBV	170179	331675	47.06%	5.771%
47	8.281	2249	2252	2254	rBV3	299	197	0.03%	0.003%
48	8.375	2278	2281	2286	rBV2	222	194	0.03%	0.003%
49	8.400	2286	2289	2293	rVB2	291	225	0.03%	0.004%
50	8.432	2293	2299	2300	rBV2	181	202	0.03%	0.004%
51	8.555	2333	2337	2339	rBV2	263	178	0.03%	0.003%
52	8.632	2355	2361	2363	rBV	176	202	0.03%	0.004%
53	8.783	2397	2408	2442	rBV	388015	631672	89.62%	10.991%
54	8.969	2462	2466	2475	rVB4	494	644	0.09%	0.011%
55	9.133	2513	2517	2521	rVB2	200	205	0.03%	0.004%
56	9.352	2578	2585	2588	rBV2	213	280	0.04%	0.005%
57	9.400	2596	2600	2605	rVB2	173	188	0.03%	0.003%
58	9.429	2605	2609	2612	rBV	183	213	0.03%	0.004%
59	9.497	2627	2630	2633	rVB	306	226	0.03%	0.004%
60	9.651	2673	2678	2681	rBV2	144	176	0.02%	0.003%
61	9.751	2705	2709	2712	rBV2	206	205	0.03%	0.004%
62	10.153	2822	2834	2856	rBV	206318	328728	46.64%	5.720%
63	10.262	2863	2868	2869	rBV	213	194	0.03%	0.003%
64	10.300	2873	2880	2883	rBV3	319	436	0.06%	0.008%
65	10.326	2883	2888	2892	rVB3	407	398	0.06%	0.007%
66	10.391	2903	2908	2914	rBV	208	294	0.04%	0.005%
67	10.487	2935	2938	2941	rVB2	214	145	0.02%	0.003%
68	10.767	3021	3025	3028	rBV2	161	145	0.02%	0.003%
69	10.863	3051	3055	3059	rVB3	369	247	0.04%	0.004%
70	10.924	3069	3074	3076	rBV	218	204	0.03%	0.004%
71	11.001	3093	3098	3105	rBV2	213	392	0.06%	0.007%
72	11.034	3105	3108	3112	rBV3	213	172	0.02%	0.003%
73	11.079	3119	3122	3125	rBV	282	240	0.03%	0.004%
74	11.185	3144	3155	3186	rBV	400361	618615	87.77%	10.764%
75	11.561	3261	3272	3295	rBV	334055	520183	73.80%	9.051%
76	11.722	3319	3322	3327	rVB2	314	201	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033924.D
 Acq On : 31 Jan 2024 16:40
 Operator : SY/MD
 Sample : P1309-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.763	3331	3335	3338	rBV2	165	173	0.02%	0.003%
78	11.915	3379	3382	3386	rBV	194	200	0.03%	0.003%
79	12.030	3413	3418	3419	rBV2	251	236	0.03%	0.004%
80	12.181	3461	3465	3467	rBV	201	160	0.02%	0.003%
81	12.255	3484	3488	3493	rBV2	165	212	0.03%	0.004%
82	12.297	3495	3501	3502	rBV2	893	712	0.10%	0.012%
83	12.477	3553	3557	3561	rBV2	220	277	0.04%	0.005%
84	12.619	3597	3601	3608	rBV2	263	331	0.05%	0.006%
85	12.696	3623	3625	3628	rBV	176	145	0.02%	0.003%
86	12.821	3661	3664	3668	rBV3	318	265	0.04%	0.005%
87	13.152	3760	3767	3769	rBV2	254	290	0.04%	0.005%
88	13.416	3845	3849	3851	rBV2	193	200	0.03%	0.003%
89	13.763	3955	3957	3965	rBV2	171	151	0.02%	0.003%
90	13.985	4021	4026	4029	rBV4	374	392	0.06%	0.007%
91	14.175	4083	4085	4090	rVV2	191	151	0.02%	0.003%
92	14.223	4096	4100	4103	rBV	245	204	0.03%	0.004%
93	14.339	4132	4136	4143	rBV2	279	376	0.05%	0.007%
94	14.477	4176	4179	4181	rBV	232	176	0.02%	0.003%
95	15.133	4380	4383	4385	rVB4	355	195	0.03%	0.003%
96	15.291	4430	4432	4434	rVB	396	194	0.03%	0.003%
97	15.310	4434	4438	4439	rBV	401	314	0.04%	0.005%
98	15.352	4447	4451	4455	rBV2	778	842	0.12%	0.015%
99	15.500	4494	4497	4501	rBV3	540	452	0.06%	0.008%
100	15.625	4534	4536	4537	rBV	427	159	0.02%	0.003%


Sum of corrected areas: 5747022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033924\
Data File : VV033924.D
Acq On : 31 Jan 2024 16:40
Operator : SY/MD
Sample : P1309-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH903

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

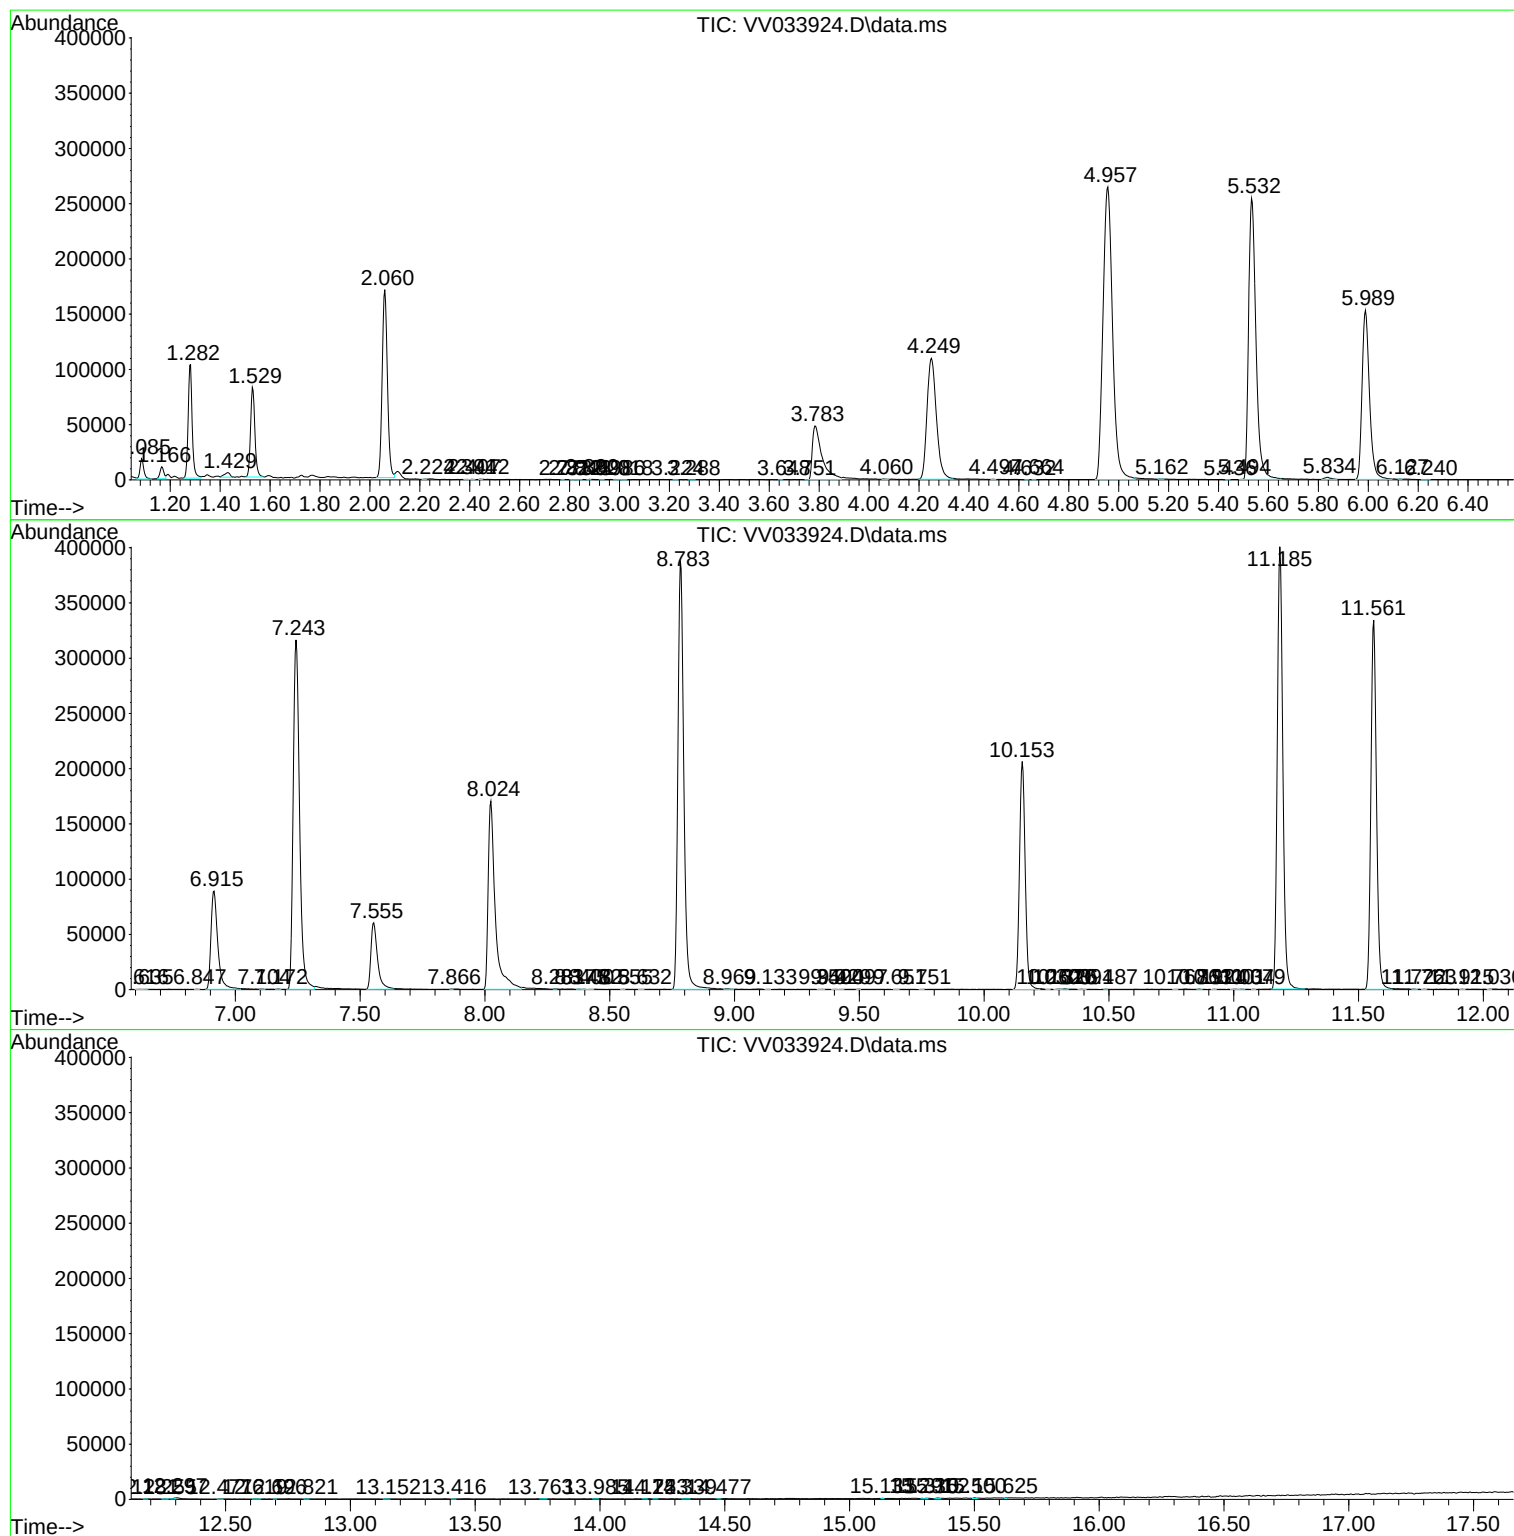

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033924.D
Acq On : 31 Jan 2024 16:40
Operator : SY/MD
Sample : P1309-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH903

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033924.D
Acq On : 31 Jan 2024 16:40
Operator : SY/MD
Sample : P1309-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH903

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------