

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033925.D
 Acq On : 31 Jan 2024 17:04
 Operator : SY/MD
 Sample : P1309-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH904

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	11	15	32	rVB3	2065	2768	0.39%	0.050%
2	1.166	32	39	44	rBV	10712	11614	1.64%	0.210%
3	1.217	51	55	63	rVB2	1764	1538	0.22%	0.028%
4	1.282	67	75	88	rBV	97975	103657	14.66%	1.871%
5	1.532	145	153	166	rVB	84356	100066	14.15%	1.806%
6	2.060	306	317	333	rBV	173828	254754	36.02%	4.598%
7	2.214	363	365	368	rBV	298	199	0.03%	0.004%
8	2.272	380	383	390	rBV2	168	181	0.03%	0.003%
9	2.455	437	440	444	rVB2	268	200	0.03%	0.004%
10	2.796	542	546	550	rVB2	193	188	0.03%	0.003%
11	2.825	552	555	558	rBV	236	209	0.03%	0.004%
12	2.867	562	568	573	rBV2	192	284	0.04%	0.005%
13	2.889	573	575	577	rVB	235	120	0.02%	0.002%
14	2.908	577	581	582	rBV2	211	154	0.02%	0.003%
15	3.124	643	648	652	rBV2	183	269	0.04%	0.005%
16	3.214	673	676	680	rVB2	206	169	0.02%	0.003%
17	3.465	751	754	758	rBV	153	180	0.03%	0.003%
18	3.503	764	766	769	rBV	273	190	0.03%	0.003%
19	3.661	811	815	818	rVB2	306	282	0.04%	0.005%
20	3.680	818	821	825	rBV2	330	398	0.06%	0.007%
21	3.783	845	853	885	rBV	51562	136037	19.24%	2.455%
22	4.249	982	998	1025	rBV2	111837	293794	41.55%	5.303%
23	4.384	1038	1040	1047	rVB2	438	341	0.05%	0.006%
24	4.625	1112	1115	1120	rVB2	206	195	0.03%	0.004%
25	4.773	1156	1161	1163	rBV	209	211	0.03%	0.004%
26	4.854	1181	1186	1190	rBV2	239	278	0.04%	0.005%
27	4.896	1197	1199	1201	rBV	216	119	0.02%	0.002%
28	4.957	1202	1218	1264	rVV2	266257	707169	100.00%	12.763%
29	5.185	1284	1289	1290	rBV3	282	245	0.03%	0.004%
30	5.246	1305	1308	1310	rBV2	217	124	0.02%	0.002%
31	5.535	1386	1398	1432	rBV	221443	459432	64.97%	8.292%
32	5.838	1484	1492	1504	rVB6	2132	4526	0.64%	0.082%
33	5.899	1509	1511	1514	rVB	215	154	0.02%	0.003%
34	5.989	1526	1539	1572	rBV	153668	319407	45.17%	5.765%
35	6.140	1584	1586	1588	rBV2	239	134	0.02%	0.002%
36	6.220	1609	1611	1615	rBV	175	150	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033925.D
 Acq On : 31 Jan 2024 17:04
 Operator : SY/MD
 Sample : P1309-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH904

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.506	1696	1700	1704	rVB2	240	221	0.03%	0.004%
38	6.712	1759	1764	1766	rVB2	185	184	0.03%	0.003%
39	6.744	1770	1774	1776	rBV	148	156	0.02%	0.003%
40	6.915	1816	1827	1861	rBV	88403	167866	23.74%	3.030%
41	7.066	1872	1874	1879	rVB3	273	208	0.03%	0.004%
42	7.243	1917	1929	1954	rBV	319092	556346	78.67%	10.041%
43	7.493	2005	2007	2011	rVB2	327	183	0.03%	0.003%
44	7.519	2013	2015	2017	rBV	173	125	0.02%	0.002%
45	7.555	2017	2026	2060	rBV	62133	111629	15.79%	2.015%
46	7.731	2079	2081	2085	rBV2	352	308	0.04%	0.006%
47	7.767	2088	2092	2096	rVB3	220	246	0.03%	0.004%
48	7.879	2119	2127	2130	rBV	467	628	0.09%	0.011%
49	7.915	2130	2138	2148	rVB6	3717	6283	0.89%	0.113%
50	8.024	2163	2172	2211	rBV	180525	346736	49.03%	6.258%
51	8.352	2271	2274	2275	rBV2	208	116	0.02%	0.002%
52	8.667	2370	2372	2376	rBV2	161	143	0.02%	0.003%
53	8.786	2397	2409	2436	rBV	332441	550320	77.82%	9.932%
54	9.037	2482	2487	2491	rBV2	128	146	0.02%	0.003%
55	9.066	2491	2496	2499	rBV2	135	157	0.02%	0.003%
56	9.461	2616	2619	2623	rBV2	165	127	0.02%	0.002%
57	9.632	2668	2672	2673	rBV	155	133	0.02%	0.002%
58	9.702	2691	2694	2697	rVB2	198	131	0.02%	0.002%
59	9.783	2714	2719	2721	rBV2	226	205	0.03%	0.004%
60	9.805	2721	2726	2729	rBV2	171	194	0.03%	0.004%
61	9.956	2769	2773	2776	rBV	166	180	0.03%	0.003%
62	10.011	2786	2790	2793	rBV2	196	202	0.03%	0.004%
63	10.153	2822	2834	2855	rBV	211337	329857	46.64%	5.953%
64	10.323	2882	2887	2897	rVB3	948	1268	0.18%	0.023%
65	10.368	2898	2901	2905	rBV	203	170	0.02%	0.003%
66	10.394	2905	2909	2912	rBV2	267	287	0.04%	0.005%
67	10.445	2920	2925	2930	rBV2	238	286	0.04%	0.005%
68	10.587	2963	2969	2973	rBV2	213	308	0.04%	0.006%
69	10.648	2984	2988	2990	rBV	170	161	0.02%	0.003%
70	10.821	3040	3042	3047	rBV2	178	177	0.03%	0.003%
71	10.898	3063	3066	3073	rVB2	256	344	0.05%	0.006%
72	10.934	3074	3077	3079	rBV2	201	147	0.02%	0.003%
73	11.185	3145	3155	3178	rBV	340888	539278	76.26%	9.733%
74	11.304	3190	3192	3197	rVB	402	230	0.03%	0.004%
75	11.368	3210	3212	3216	rBV2	156	125	0.02%	0.002%
76	11.561	3261	3272	3298	rVV	325205	517639	73.20%	9.343%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033925.D
 Acq On : 31 Jan 2024 17:04
 Operator : SY/MD
 Sample : P1309-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH904

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.728	3319	3324	3327	rBV3	509	361	0.05%	0.007%
78	11.895	3371	3376	3382	rBV	193	256	0.04%	0.005%
79	11.953	3388	3394	3399	rVB2	249	297	0.04%	0.005%
80	11.979	3399	3402	3406	rBV2	205	204	0.03%	0.004%
81	12.024	3409	3416	3418	rBV3	278	340	0.05%	0.006%
82	12.046	3420	3423	3426	rBV	353	222	0.03%	0.004%
83	12.133	3445	3450	3452	rBV2	239	200	0.03%	0.004%
84	12.149	3452	3455	3457	rBV	201	155	0.02%	0.003%
85	12.236	3479	3482	3485	rBV	224	185	0.03%	0.003%
86	12.307	3497	3504	3511	rBV4	1448	2177	0.31%	0.039%
87	12.686	3619	3622	3625	rBV2	181	148	0.02%	0.003%
88	12.731	3633	3636	3638	rBV	176	150	0.02%	0.003%
89	12.947	3699	3703	3704	rBV2	193	136	0.02%	0.002%
90	13.149	3762	3766	3768	rBV	137	120	0.02%	0.002%
91	13.622	3911	3913	3918	rBV2	191	199	0.03%	0.004%
92	13.648	3918	3921	3923	rVV	256	151	0.02%	0.003%
93	13.795	3964	3967	3972	rVB	221	155	0.02%	0.003%
94	13.869	3987	3990	3996	rBV2	271	381	0.05%	0.007%
95	14.024	4032	4038	4042	rVB3	302	358	0.05%	0.006%
96	14.075	4050	4054	4057	rBV3	227	231	0.03%	0.004%
97	14.130	4067	4071	4077	rVB2	194	216	0.03%	0.004%
98	14.252	4106	4109	4114	rVB2	399	233	0.03%	0.004%
99	14.439	4165	4167	4171	rBV2	239	183	0.03%	0.003%
100	14.963	4327	4330	4334	rBV2	396	377	0.05%	0.007%




Sum of corrected areas: 5540621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033925.D
Acq On : 31 Jan 2024 17:04
Operator : SY/MD
Sample : P1309-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH904

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

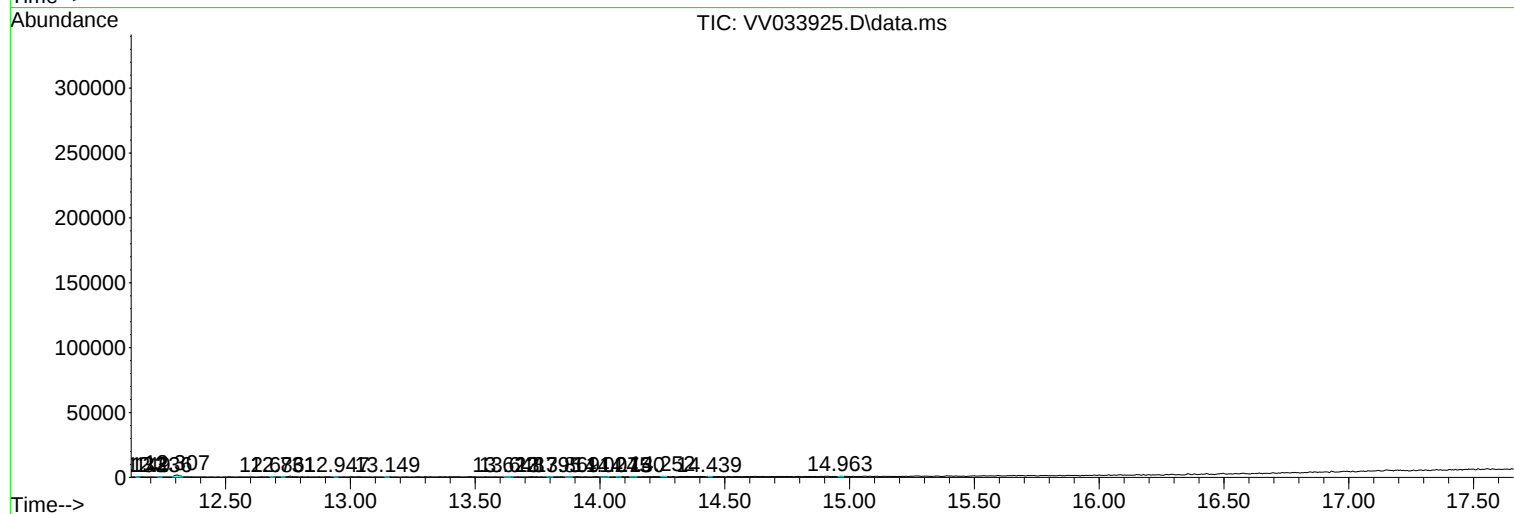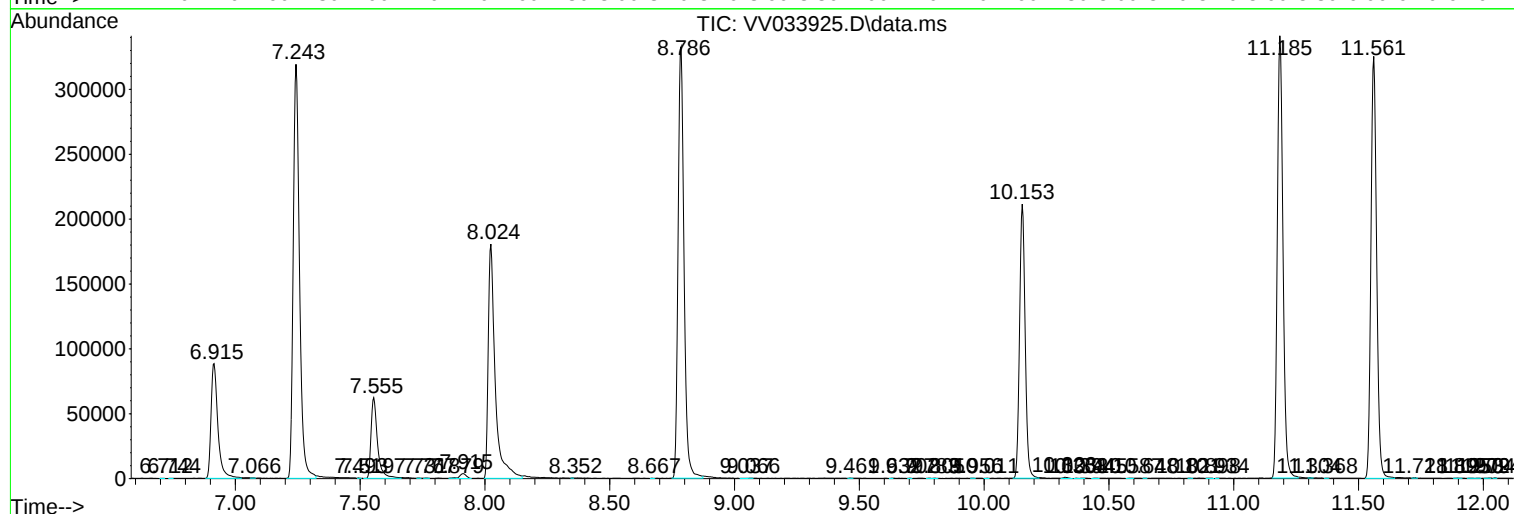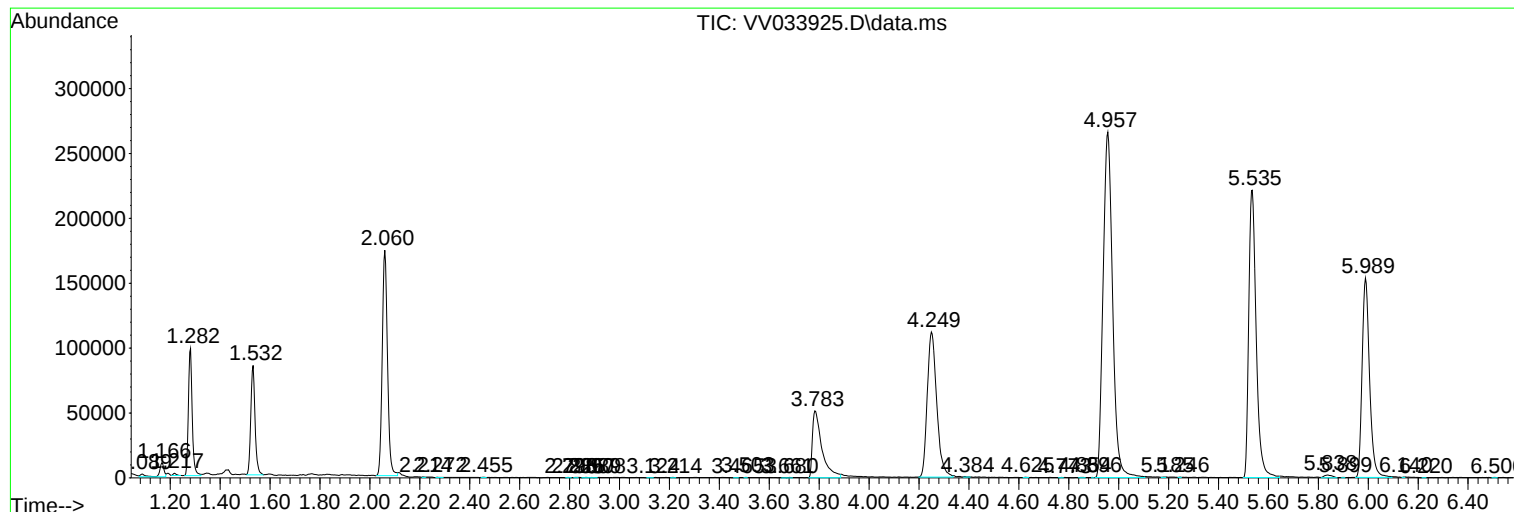

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033925.D
Acq On : 31 Jan 2024 17:04
Operator : SY/MD
Sample : P1309-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH904

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033925.D
Acq On : 31 Jan 2024 17:04
Operator : SY/MD
Sample : P1309-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH904

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc