

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033926.D
 Acq On : 31 Jan 2024 17:28
 Operator : SY/MD
 Sample : P1309-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	24	rVB2	8216	8265	1.14%	0.141%
2	1.166	32	39	44	rBV	11390	11852	1.64%	0.202%
3	1.217	52	55	62	rVB3	1616	1490	0.21%	0.025%
4	1.278	66	74	90	rBV	100988	112279	15.54%	1.916%
5	1.529	144	152	166	rVB	82205	99732	13.80%	1.701%
6	2.060	306	317	330	rBV	179205	260996	36.12%	4.453%
7	2.288	383	388	389	rBV	548	352	0.05%	0.006%
8	2.449	432	438	445	rBV3	999	1352	0.19%	0.023%
9	2.703	505	517	528	rBV6	1322	2726	0.38%	0.047%
10	2.915	577	583	587	rBV2	265	353	0.05%	0.006%
11	3.076	628	633	637	rBV2	189	249	0.03%	0.004%
12	3.201	670	672	675	rBV2	173	151	0.02%	0.003%
13	3.384	723	729	730	rBV	284	262	0.04%	0.004%
14	3.471	753	756	760	rBV2	245	268	0.04%	0.005%
15	3.622	800	803	807	rBV2	182	190	0.03%	0.003%
16	3.783	845	853	889	rBV	53911	143657	19.88%	2.451%
17	4.249	983	998	1027	rBV	114627	295348	40.87%	5.039%
18	4.429	1050	1054	1059	rVB4	340	367	0.05%	0.006%
19	4.574	1096	1099	1100	rBV3	439	234	0.03%	0.004%
20	4.748	1149	1153	1156	rVB3	431	411	0.06%	0.007%
21	4.777	1156	1162	1165	rBV2	192	266	0.04%	0.005%
22	4.863	1181	1189	1191	rBV	240	360	0.05%	0.006%
23	4.957	1202	1218	1245	rBV2	273464	722646	100.00%	12.329%
24	5.198	1291	1293	1300	rVB2	318	276	0.04%	0.005%
25	5.346	1337	1339	1344	rVB2	336	292	0.04%	0.005%
26	5.381	1346	1350	1351	rBV	329	256	0.04%	0.004%
27	5.490	1379	1384	1386	rBV	188	189	0.03%	0.003%
28	5.532	1386	1397	1429	rBV	245773	505587	69.96%	8.626%
29	5.841	1483	1493	1502	rVB8	1945	4383	0.61%	0.075%
30	5.989	1527	1539	1568	rBV	157900	328687	45.48%	5.608%
31	6.140	1582	1586	1589	rBV4	443	358	0.05%	0.006%
32	6.307	1632	1638	1641	rBV2	187	220	0.03%	0.004%
33	6.445	1677	1681	1685	rBV2	222	238	0.03%	0.004%
34	6.574	1717	1721	1723	rBV	190	175	0.02%	0.003%
35	6.815	1793	1796	1798	rBV	198	165	0.02%	0.003%
36	6.912	1816	1826	1852	rVV	93967	176435	24.42%	3.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033926.D
 Acq On : 31 Jan 2024 17:28
 Operator : SY/MD
 Sample : P1309-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	7.198	1911	1915	1918	rBV3	263	203	0.03%	0.003%
38	7.243	1918	1929	1952	rBV	326007	573145	79.31%	9.778%
39	7.490	2004	2006	2011	rVB	338	224	0.03%	0.004%
40	7.555	2016	2026	2049	rBV	63580	115006	15.91%	1.962%
41	7.677	2062	2064	2068	rVB3	299	214	0.03%	0.004%
42	7.715	2073	2076	2079	rVB3	305	202	0.03%	0.003%
43	7.735	2079	2082	2083	rBV	237	156	0.02%	0.003%
44	7.912	2136	2137	2142	rVB	569	385	0.05%	0.007%
45	8.024	2163	2172	2217	rBV	191586	366887	50.77%	6.259%
46	8.175	2217	2219	2222	rVV2	453	209	0.03%	0.004%
47	8.252	2241	2243	2248	rVB5	406	319	0.04%	0.005%
48	8.358	2271	2276	2279	rBV2	181	204	0.03%	0.003%
49	8.526	2324	2328	2331	rBV2	214	229	0.03%	0.004%
50	8.744	2392	2396	2398	rBV	239	225	0.03%	0.004%
51	8.783	2398	2408	2444	rBV	368458	614562	85.04%	10.485%
52	8.992	2471	2473	2478	rVB2	361	228	0.03%	0.004%
53	9.085	2496	2502	2504	rBV2	723	652	0.09%	0.011%
54	9.188	2528	2534	2538	rBV	140	218	0.03%	0.004%
55	9.275	2558	2561	2568	rBV2	204	272	0.04%	0.005%
56	9.484	2622	2626	2628	rBV2	965	822	0.11%	0.014%
57	9.612	2662	2666	2669	rBV	147	154	0.02%	0.003%
58	9.719	2695	2699	2701	rBV2	218	203	0.03%	0.003%
59	9.873	2742	2747	2754	rVV4	1140	1567	0.22%	0.027%
60	10.153	2823	2834	2863	rVB	220514	346180	47.90%	5.906%
61	10.487	2930	2938	2946	rBV3	1252	2018	0.28%	0.034%
62	10.648	2985	2988	2994	rBV2	162	232	0.03%	0.004%
63	10.863	3049	3055	3064	rVB2	765	1236	0.17%	0.021%
64	11.072	3117	3120	3127	rBV2	240	307	0.04%	0.005%
65	11.130	3133	3138	3142	rBV2	823	895	0.12%	0.015%
66	11.185	3144	3155	3184	rVV	388574	602559	83.38%	10.280%
67	11.320	3195	3197	3201	rBV2	290	237	0.03%	0.004%
68	11.368	3210	3212	3215	rBV2	283	177	0.02%	0.003%
69	11.394	3215	3220	3226	rVB	176	270	0.04%	0.005%
70	11.490	3246	3250	3261	rBV2	153	336	0.05%	0.006%
71	11.561	3261	3272	3291	rBV	340402	540575	74.80%	9.223%
72	11.699	3312	3315	3321	rVB3	230	188	0.03%	0.003%
73	11.728	3321	3324	3328	rBV2	274	232	0.03%	0.004%
74	11.783	3336	3341	3343	rBV2	173	175	0.02%	0.003%
75	11.982	3399	3403	3406	rBV	215	233	0.03%	0.004%
76	12.214	3471	3475	3477	rBV	228	208	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033926.D
Acq On : 31 Jan 2024 17:28
Operator : SY/MD
Sample : P1309-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis

77	12.300	3497	3502	3507	rBV5	1154	1410	0.20%	0.024%
78	12.590	3579	3592	3598	rBV4	616	1226	0.17%	0.021%
79	12.641	3605	3608	3611	rBV	200	189	0.03%	0.003%
80	12.789	3651	3654	3659	rBV2	156	168	0.02%	0.003%
81	12.969	3707	3710	3715	rBV2	190	242	0.03%	0.004%
82	13.207	3782	3784	3785	rBV	404	194	0.03%	0.003%
83	13.439	3853	3856	3857	rBV2	296	154	0.02%	0.003%
84	13.503	3870	3876	3878	rBV	160	191	0.03%	0.003%
85	13.632	3913	3916	3921	rVB3	274	224	0.03%	0.004%
86	13.686	3930	3933	3934	rBV	231	159	0.02%	0.003%
87	13.722	3941	3944	3946	rBV2	282	188	0.03%	0.003%
88	13.937	4008	4011	4016	rVB3	345	299	0.04%	0.005%
89	13.985	4021	4026	4027	rBV	533	454	0.06%	0.008%
90	14.024	4036	4038	4040	rBV2	275	178	0.02%	0.003%
91	14.040	4040	4043	4047	rVB2	365	305	0.04%	0.005%
92	14.066	4047	4051	4053	rBV2	250	239	0.03%	0.004%
93	14.136	4069	4073	4076	rBV2	288	249	0.03%	0.004%
94	14.345	4132	4138	4141	rBV3	386	507	0.07%	0.009%
95	14.442	4164	4168	4173	rBV2	354	393	0.05%	0.007%
96	14.471	4173	4177	4179	rBV2	263	206	0.03%	0.004%
97	14.757	4264	4266	4269	rBV2	299	167	0.02%	0.003%
98	15.033	4349	4352	4354	rBV2	341	229	0.03%	0.004%
99	15.194	4400	4402	4406	rBV2	366	191	0.03%	0.003%
100	15.468	4484	4487	4488	rBV	387	250	0.03%	0.004%




Sum of corrected areas: 5861423

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033926.D
Acq On : 31 Jan 2024 17:28
Operator : SY/MD
Sample : P1309-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH905

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

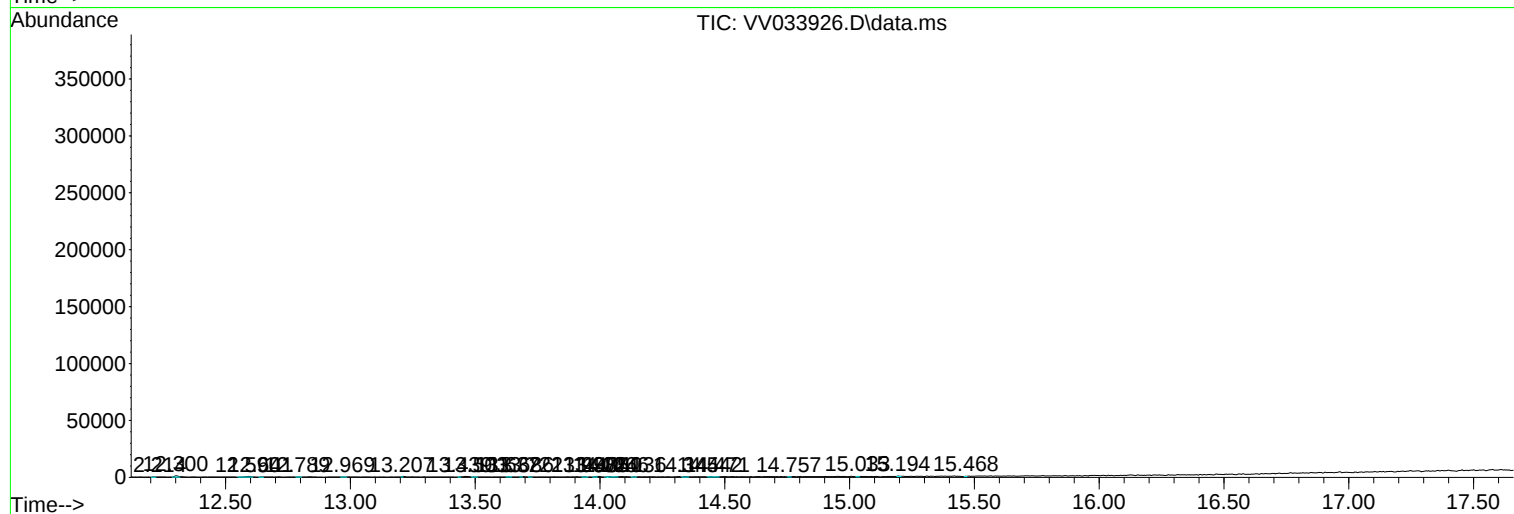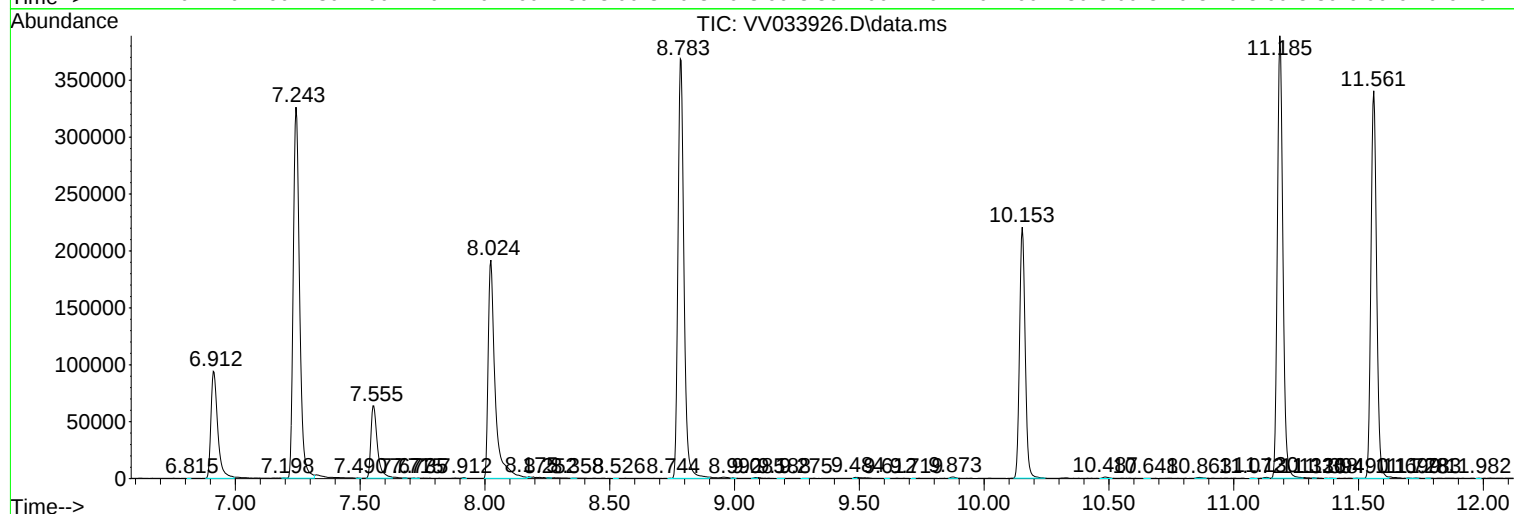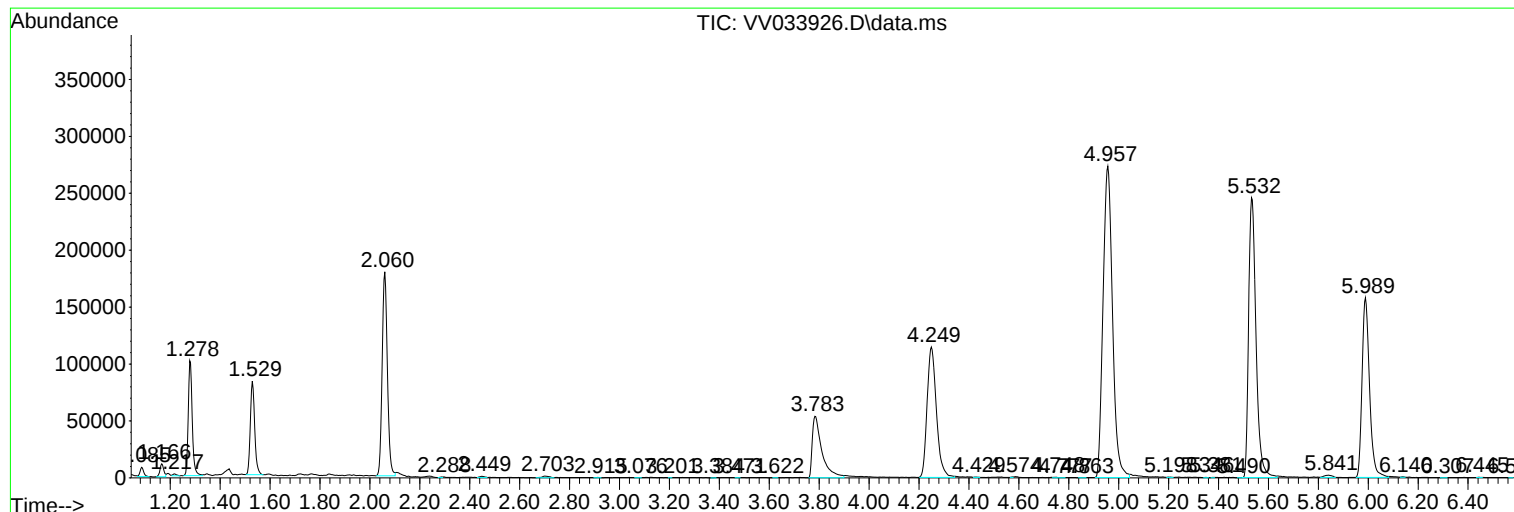

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033926.D
Acq On : 31 Jan 2024 17:28
Operator : SY/MD
Sample : P1309-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH905

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033926.D
Acq On : 31 Jan 2024 17:28
Operator : SY/MD
Sample : P1309-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH905

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------