

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033927.D
 Acq On : 31 Jan 2024 17:52
 Operator : SY/MD
 Sample : P1309-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	23	rVB	11600	11219	1.61%	0.197%
2	1.166	32	39	44	rBV	9401	10562	1.51%	0.185%
3	1.278	67	74	88	rBV	97452	106327	15.25%	1.864%
4	1.529	144	152	165	rVB	80580	97778	14.02%	1.714%
5	2.060	307	317	331	rBV	171573	249621	35.79%	4.376%
6	2.182	352	355	363	rVB3	626	603	0.09%	0.011%
7	2.220	363	367	368	rBV	365	245	0.04%	0.004%
8	2.394	419	421	424	rBV	248	159	0.02%	0.003%
9	2.600	481	485	486	rBV	242	189	0.03%	0.003%
10	2.648	495	500	502	rBV2	185	212	0.03%	0.004%
11	2.706	512	518	521	rBV2	235	317	0.05%	0.006%
12	2.851	560	563	566	rBV2	198	169	0.02%	0.003%
13	2.883	571	573	578	rVB3	428	309	0.04%	0.005%
14	2.947	590	593	595	rBV	150	133	0.02%	0.002%
15	3.034	617	620	625	rBV2	191	149	0.02%	0.003%
16	3.092	636	638	640	rBV	269	193	0.03%	0.003%
17	3.227	676	680	682	rBV2	179	182	0.03%	0.003%
18	3.314	701	707	709	rBV	158	207	0.03%	0.004%
19	3.458	750	752	754	rBV	185	127	0.02%	0.002%
20	3.474	754	757	760	rVV	188	180	0.03%	0.003%
21	3.500	763	765	768	rBV2	156	135	0.02%	0.002%
22	3.590	789	793	797	rBV	159	172	0.02%	0.003%
23	3.638	805	808	813	rVB2	161	124	0.02%	0.002%
24	3.683	819	822	826	rVB2	212	194	0.03%	0.003%
25	3.728	831	836	841	rBV2	255	322	0.05%	0.006%
26	3.783	845	853	883	rBV	53046	138842	19.91%	2.434%
27	4.137	960	963	967	rBV2	180	189	0.03%	0.003%
28	4.249	982	998	1029	rBV2	111208	289966	41.58%	5.084%
29	4.703	1138	1139	1143	rVB2	261	123	0.02%	0.002%
30	4.732	1143	1148	1154	rBV2	218	306	0.04%	0.005%
31	4.806	1167	1171	1173	rBV	226	194	0.03%	0.003%
32	4.860	1183	1188	1190	rBV2	158	192	0.03%	0.003%
33	4.957	1202	1218	1254	rBV2	262702	697391	100.00%	12.226%
34	5.349	1337	1340	1345	rBV2	197	168	0.02%	0.003%
35	5.416	1357	1361	1363	rBV2	188	170	0.02%	0.003%
36	5.532	1386	1397	1431	rBV	251014	510565	73.21%	8.951%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033927.D
 Acq On : 31 Jan 2024 17:52
 Operator : SY/MD
 Sample : P1309-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.834	1483	1491	1504	rBV5	1986	4376	0.63%	0.077%
38	5.989	1526	1539	1573	rBV	154132	317330	45.50%	5.563%
39	6.323	1639	1643	1645	rBV	199	189	0.03%	0.003%
40	6.535	1703	1709	1713	rBV	237	340	0.05%	0.006%
41	6.580	1719	1723	1727	rBV2	217	255	0.04%	0.004%
42	6.625	1734	1737	1741	rBV2	288	234	0.03%	0.004%
43	6.854	1804	1808	1811	rBV2	193	235	0.03%	0.004%
44	6.915	1816	1827	1855	rBV	88997	167606	24.03%	2.938%
45	7.204	1913	1917	1918	rBV	218	136	0.02%	0.002%
46	7.243	1918	1929	1952	rBV	315129	550693	78.96%	9.654%
47	7.555	2017	2026	2054	rBV	61726	110362	15.82%	1.935%
48	7.783	2094	2097	2101	rBV	203	221	0.03%	0.004%
49	7.879	2119	2127	2132	rVB	283	405	0.06%	0.007%
50	7.944	2143	2147	2153	rBV2	214	298	0.04%	0.005%
51	8.024	2163	2172	2218	rBV	184582	358506	51.41%	6.285%
52	8.194	2223	2225	2230	rVV3	486	325	0.05%	0.006%
53	8.307	2258	2260	2262	rBV	208	124	0.02%	0.002%
54	8.333	2267	2268	2274	rVB2	393	338	0.05%	0.006%
55	8.365	2274	2278	2285	rBV3	295	311	0.04%	0.005%
56	8.783	2397	2408	2438	rBV	368267	615341	88.23%	10.788%
57	9.227	2543	2546	2549	rBV	167	165	0.02%	0.003%
58	9.297	2563	2568	2572	rBV	236	316	0.05%	0.006%
59	9.481	2623	2625	2628	rBV2	161	121	0.02%	0.002%
60	9.571	2650	2653	2656	rBV	129	126	0.02%	0.002%
61	9.690	2685	2690	2694	rBV2	221	287	0.04%	0.005%
62	9.809	2722	2727	2729	rBV	222	229	0.03%	0.004%
63	10.075	2807	2810	2813	rVB	272	185	0.03%	0.003%
64	10.114	2819	2822	2823	rBV	169	122	0.02%	0.002%
65	10.153	2823	2834	2859	rVV	216506	333274	47.79%	5.843%
66	10.326	2883	2888	2895	rVV3	308	468	0.07%	0.008%
67	10.407	2906	2913	2916	rBV	207	296	0.04%	0.005%
68	10.516	2945	2947	2952	rBV2	125	129	0.02%	0.002%
69	10.757	3018	3022	3024	rBV2	187	134	0.02%	0.002%
70	10.947	3078	3081	3083	rBV2	222	182	0.03%	0.003%
71	10.989	3091	3094	3098	rVB	170	152	0.02%	0.003%
72	11.185	3145	3155	3186	rBV	384140	602529	86.40%	10.563%
73	11.477	3243	3246	3249	rBV2	212	201	0.03%	0.004%
74	11.561	3260	3272	3305	rBV	329006	512192	73.44%	8.979%
75	11.686	3309	3311	3315	rVV2	414	350	0.05%	0.006%
76	11.722	3319	3322	3328	rVB4	992	837	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033927.D
 Acq On : 31 Jan 2024 17:52
 Operator : SY/MD
 Sample : P1309-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.802	3344	3347	3349	rBV	162	128	0.02%	0.002%
78	11.828	3352	3355	3360	rVV2	203	203	0.03%	0.004%
79	11.963	3395	3397	3405	rVB2	157	194	0.03%	0.003%
80	12.008	3407	3411	3412	rBV	210	161	0.02%	0.003%
81	12.037	3417	3420	3423	rVB2	225	178	0.03%	0.003%
82	12.127	3444	3448	3451	rBV2	202	204	0.03%	0.004%
83	12.172	3459	3462	3469	rVB	225	253	0.04%	0.004%
84	12.204	3469	3472	3474	rBV2	246	188	0.03%	0.003%
85	12.271	3490	3493	3495	rBV	197	165	0.02%	0.003%
86	12.355	3517	3519	3525	rBV	194	242	0.03%	0.004%
87	12.754	3633	3643	3649	rBV5	707	1112	0.16%	0.019%
88	12.786	3649	3653	3655	rBV2	177	170	0.02%	0.003%
89	12.950	3701	3704	3708	rBV	217	188	0.03%	0.003%
90	13.053	3733	3736	3739	rBV	239	212	0.03%	0.004%
91	13.455	3858	3861	3864	rBV	234	137	0.02%	0.002%
92	13.651	3918	3922	3925	rBV	254	240	0.03%	0.004%
93	13.895	3995	3998	4000	rBV	260	203	0.03%	0.004%
94	14.156	4075	4079	4085	rBV2	406	477	0.07%	0.008%
95	14.278	4113	4117	4120	rBV2	419	416	0.06%	0.007%
96	14.320	4127	4130	4132	rBV3	235	164	0.02%	0.003%
97	14.519	4189	4192	4196	rVB3	322	216	0.03%	0.004%
98	14.763	4266	4268	4269	rBV3	306	149	0.02%	0.003%
99	14.927	4316	4319	4323	rBV2	302	321	0.05%	0.006%
100	15.168	4392	4394	4399	rBV2	311	240	0.03%	0.004%




Sum of corrected areas: 5704015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033927.D
Acq On : 31 Jan 2024 17:52
Operator : SY/MD
Sample : P1309-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

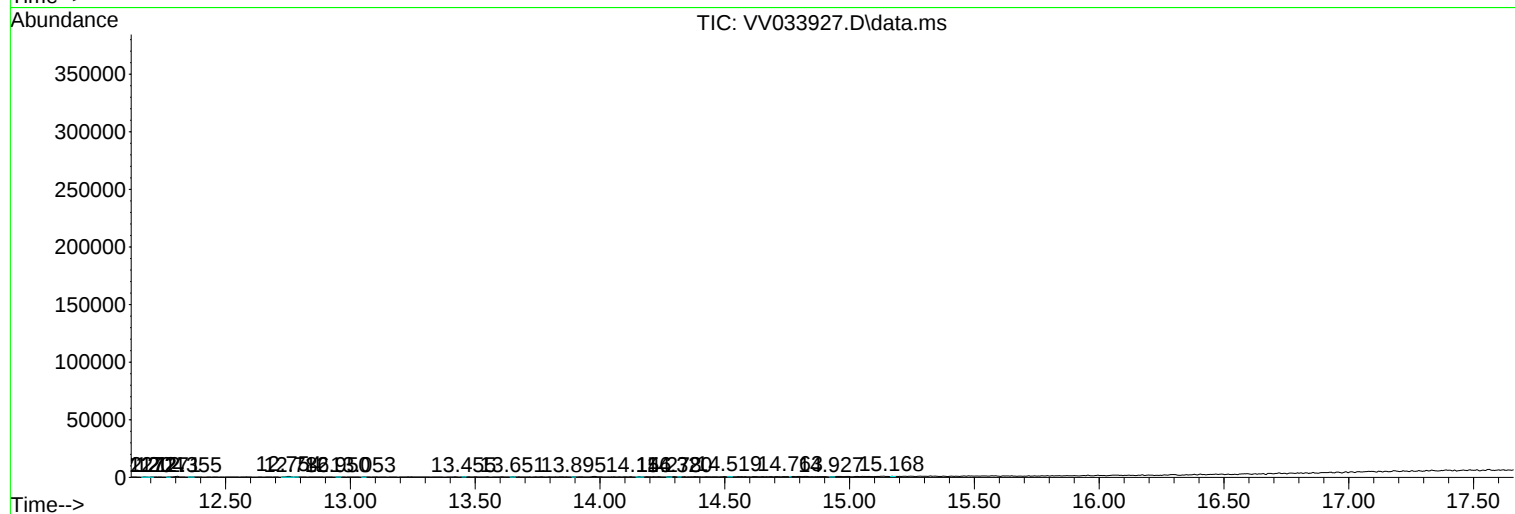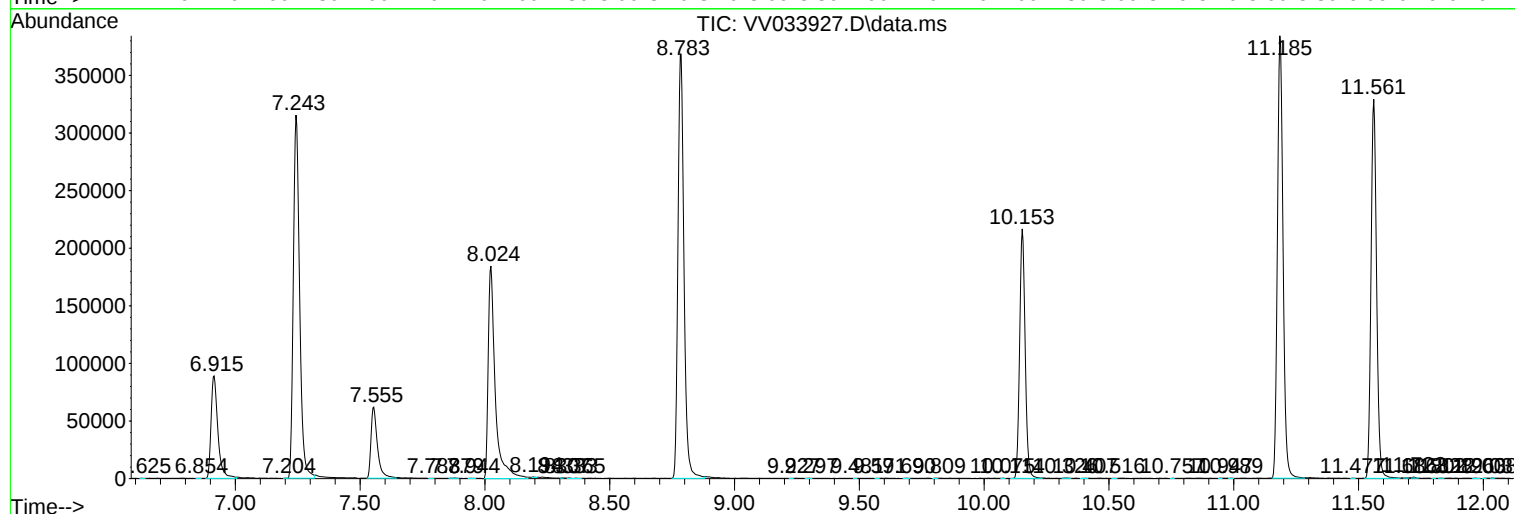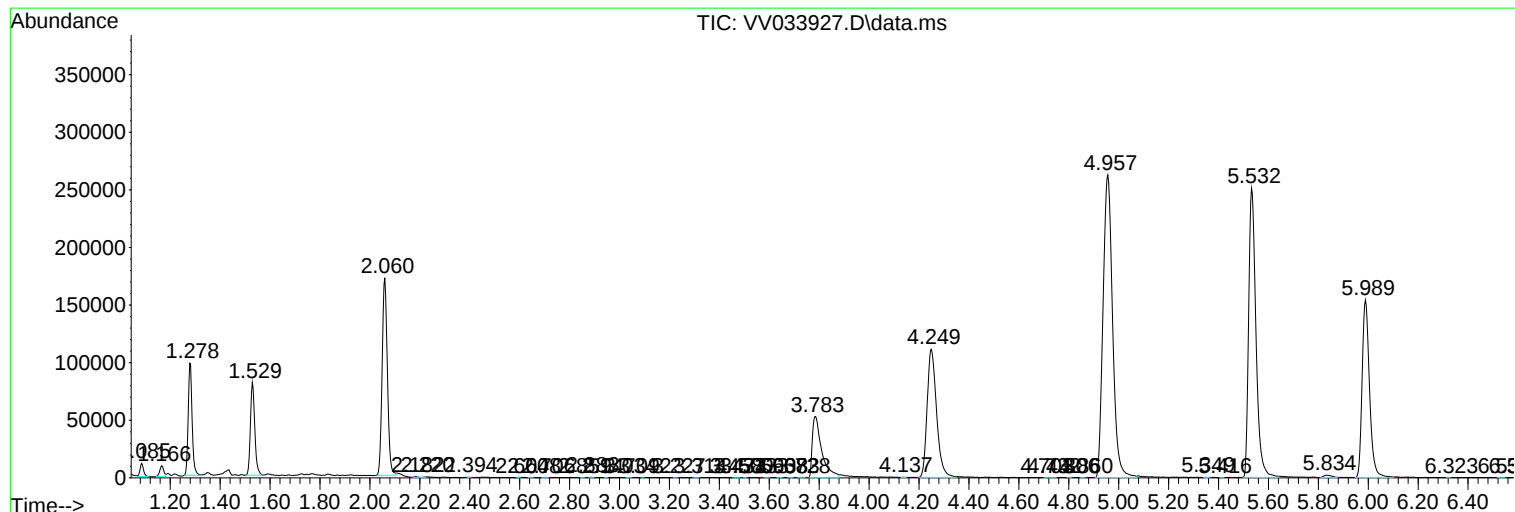

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033927.D
Acq On : 31 Jan 2024 17:52
Operator : SY/MD
Sample : P1309-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033927.D
Acq On : 31 Jan 2024 17:52
Operator : SY/MD
Sample : P1309-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc