

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033928.D
 Acq On : 31 Jan 2024 18:16
 Operator : SY/MD
 Sample : P1309-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	21	rVB	5063	4610	0.67%	0.082%
2	1.166	32	39	44	rBV	9913	11296	1.64%	0.200%
3	1.278	67	74	89	rBV	94663	104554	15.21%	1.850%
4	1.349	91	96	102	rVB	4270	4759	0.69%	0.084%
5	1.529	145	152	168	rVB	78339	97608	14.20%	1.727%
6	2.060	306	317	332	rBV	170445	248401	36.13%	4.396%
7	2.182	351	355	357	rBV3	398	363	0.05%	0.006%
8	2.442	434	436	438	rVV2	420	221	0.03%	0.004%
9	2.455	438	440	442	rVV2	369	175	0.03%	0.003%
10	2.632	491	495	505	rVB2	277	426	0.06%	0.008%
11	2.677	505	509	512	rBV2	211	208	0.03%	0.004%
12	2.908	579	581	586	rVB2	204	168	0.02%	0.003%
13	2.944	586	592	594	rVB2	180	178	0.03%	0.003%
14	3.088	633	637	639	rBV	178	184	0.03%	0.003%
15	3.133	648	651	657	rBV2	140	184	0.03%	0.003%
16	3.542	773	778	781	rBV2	248	285	0.04%	0.005%
17	3.561	781	784	790	rVB	200	241	0.04%	0.004%
18	3.600	790	796	798	rBV2	172	223	0.03%	0.004%
19	3.645	808	810	815	rVB	236	194	0.03%	0.003%
20	3.783	846	853	899	rBV	49672	134357	19.54%	2.378%
21	4.249	982	998	1031	rBV	107988	279461	40.65%	4.946%
22	4.481	1067	1070	1073	rVB3	263	157	0.02%	0.003%
23	4.513	1077	1080	1084	rVB2	343	308	0.04%	0.005%
24	4.831	1176	1179	1183	rBV2	151	178	0.03%	0.003%
25	4.957	1202	1218	1255	rBV2	260804	687494	100.00%	12.166%
26	5.313	1324	1329	1335	rBV2	262	399	0.06%	0.007%
27	5.368	1342	1346	1349	rBV2	197	192	0.03%	0.003%
28	5.535	1385	1398	1432	rBV	252692	519825	75.61%	9.199%
29	5.738	1456	1461	1463	rBV	342	277	0.04%	0.005%
30	5.767	1467	1470	1476	rVB2	239	242	0.04%	0.004%
31	5.831	1484	1490	1500	rBV5	1763	3341	0.49%	0.059%
32	5.944	1521	1525	1527	rBV2	203	174	0.03%	0.003%
33	5.989	1527	1539	1560	rBV	148533	307898	44.79%	5.449%
34	6.114	1576	1578	1583	rVB4	337	243	0.04%	0.004%
35	6.149	1585	1589	1592	rVB4	575	345	0.05%	0.006%
36	6.262	1619	1624	1627	rBV2	312	202	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033928.D
 Acq On : 31 Jan 2024 18:16
 Operator : SY/MD
 Sample : P1309-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.297	1630	1635	1636	rBV2	280	219	0.03%	0.004%
38	6.532	1703	1708	1709	rBV2	149	157	0.02%	0.003%
39	6.754	1772	1777	1780	rBV	198	223	0.03%	0.004%
40	6.815	1793	1796	1802	rVV2	118	162	0.02%	0.003%
41	6.915	1816	1827	1854	rBV	86324	163295	23.75%	2.890%
42	7.117	1888	1890	1894	rBV	197	181	0.03%	0.003%
43	7.243	1918	1929	1952	rBV	306183	535097	77.83%	9.470%
44	7.554	2016	2026	2060	rBV	60045	108849	15.83%	1.926%
45	7.693	2064	2069	2073	rVB4	480	590	0.09%	0.010%
46	7.722	2073	2078	2083	rVB2	431	464	0.07%	0.008%
47	7.747	2083	2086	2090	rBV2	365	329	0.05%	0.006%
48	7.796	2098	2101	2110	rVB	219	325	0.05%	0.006%
49	7.879	2120	2127	2132	rBV2	692	805	0.12%	0.014%
50	7.911	2132	2137	2146	rVB4	1356	1975	0.29%	0.035%
51	7.947	2146	2148	2153	rBV	143	171	0.02%	0.003%
52	8.024	2163	2172	2214	rBV	173864	335170	48.75%	5.931%
53	8.243	2238	2240	2246	rVB3	411	268	0.04%	0.005%
54	8.783	2397	2408	2438	rBV	380513	628274	91.39%	11.118%
55	9.001	2473	2476	2479	rVB	244	166	0.02%	0.003%
56	9.027	2480	2484	2486	rVB	265	166	0.02%	0.003%
57	9.085	2500	2502	2505	rVB3	241	158	0.02%	0.003%
58	9.201	2535	2538	2543	rVB2	183	194	0.03%	0.003%
59	10.152	2823	2834	2853	rVV	206607	323465	47.05%	5.724%
60	10.326	2881	2888	2896	rVB3	825	1231	0.18%	0.022%
61	10.390	2902	2908	2911	rVB2	203	257	0.04%	0.005%
62	10.461	2920	2930	2936	rVB2	232	452	0.07%	0.008%
63	10.587	2965	2969	2975	rBV2	220	258	0.04%	0.005%
64	10.641	2983	2986	2991	rVB	218	188	0.03%	0.003%
65	10.869	3055	3057	3062	rVB	273	181	0.03%	0.003%
66	11.101	3124	3129	3136	rBV2	977	1267	0.18%	0.022%
67	11.185	3144	3155	3177	rBV	401575	613700	89.27%	10.861%
68	11.300	3188	3191	3197	rBV4	339	412	0.06%	0.007%
69	11.561	3260	3272	3297	rBV	323246	508433	73.95%	8.998%
70	11.879	3365	3371	3373	rBV	267	273	0.04%	0.005%
71	12.127	3445	3448	3450	rBV	209	163	0.02%	0.003%
72	12.297	3493	3501	3511	rBV5	3826	5935	0.86%	0.105%
73	12.799	3654	3657	3664	rVB2	222	312	0.05%	0.006%
74	12.837	3664	3669	3672	rBV2	214	260	0.04%	0.005%
75	12.860	3672	3676	3680	rBV2	233	225	0.03%	0.004%
76	12.930	3692	3698	3701	rBV	262	294	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033928.D
 Acq On : 31 Jan 2024 18:16
 Operator : SY/MD
 Sample : P1309-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.985	3711	3715	3717	rVV	161	161	0.02%	0.003%
78	13.043	3731	3733	3740	rVB2	203	201	0.03%	0.004%
79	13.300	3809	3813	3815	rBV	191	193	0.03%	0.003%
80	13.435	3852	3855	3858	rBV	216	215	0.03%	0.004%
81	13.503	3872	3876	3880	rBV2	306	326	0.05%	0.006%
82	13.602	3901	3907	3912	rBV2	257	351	0.05%	0.006%
83	13.635	3912	3917	3919	rBV2	222	210	0.03%	0.004%
84	13.686	3930	3933	3937	rBV	178	189	0.03%	0.003%
85	13.985	4019	4026	4028	rBV3	341	386	0.06%	0.007%
86	14.085	4053	4057	4061	rVB	207	155	0.02%	0.003%
87	14.130	4069	4071	4076	rBV3	307	333	0.05%	0.006%
88	14.165	4079	4082	4084	rBV3	341	252	0.04%	0.004%
89	14.226	4099	4101	4107	rBV3	162	180	0.03%	0.003%
90	14.265	4109	4113	4117	rVB3	387	369	0.05%	0.007%
91	14.310	4123	4127	4132	rBV3	338	454	0.07%	0.008%
92	14.384	4147	4150	4152	rBV2	297	165	0.02%	0.003%
93	14.606	4216	4219	4221	rBV3	427	288	0.04%	0.005%
94	14.779	4271	4273	4277	rBV3	296	213	0.03%	0.004%
95	15.155	4387	4390	4393	rVB2	332	174	0.03%	0.003%
96	15.310	4436	4438	4444	rBV3	283	321	0.05%	0.006%
97	15.426	4471	4474	4480	rBV4	584	662	0.10%	0.012%
98	15.509	4496	4500	4505	rBV5	463	492	0.07%	0.009%
99	15.834	4600	4601	4603	rBV2	413	200	0.03%	0.004%
100	15.914	4624	4626	4628	rBV2	566	309	0.04%	0.005%




Sum of corrected areas: 5650714

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033928.D
Acq On : 31 Jan 2024 18:16
Operator : SY/MD
Sample : P1309-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

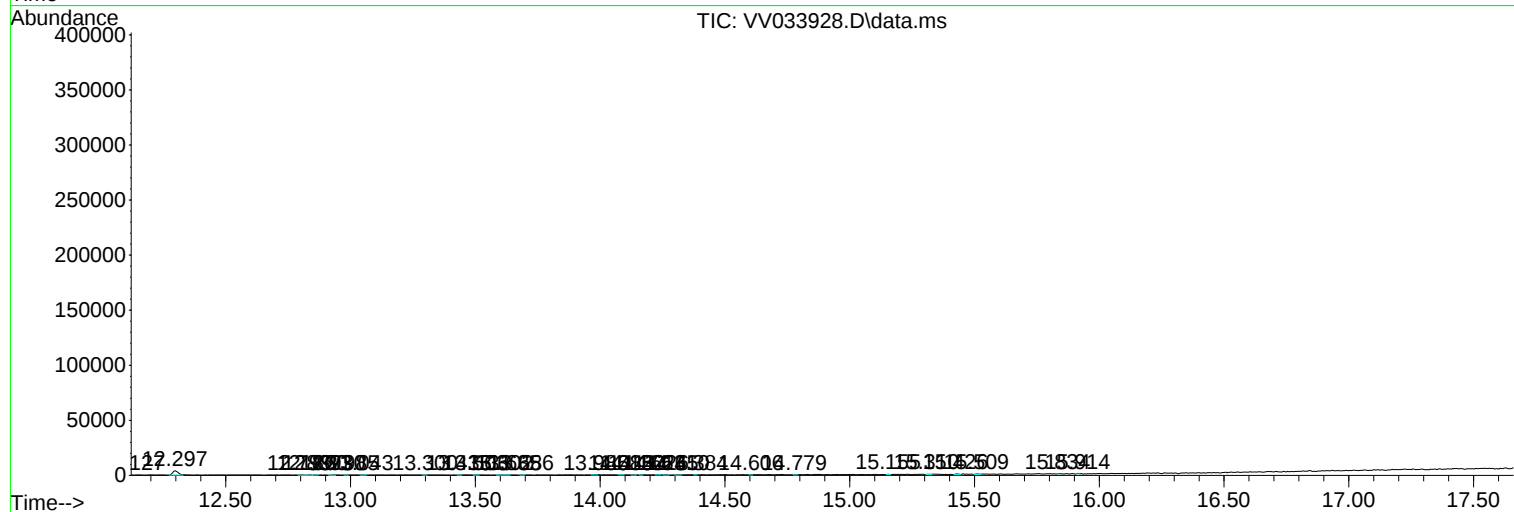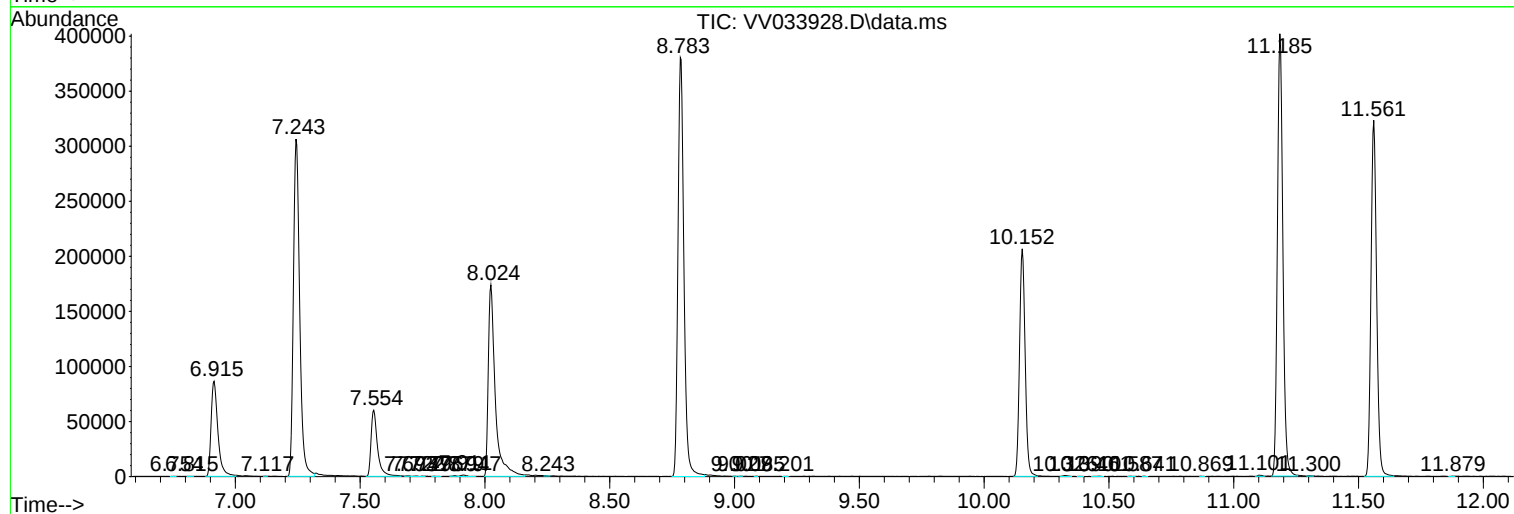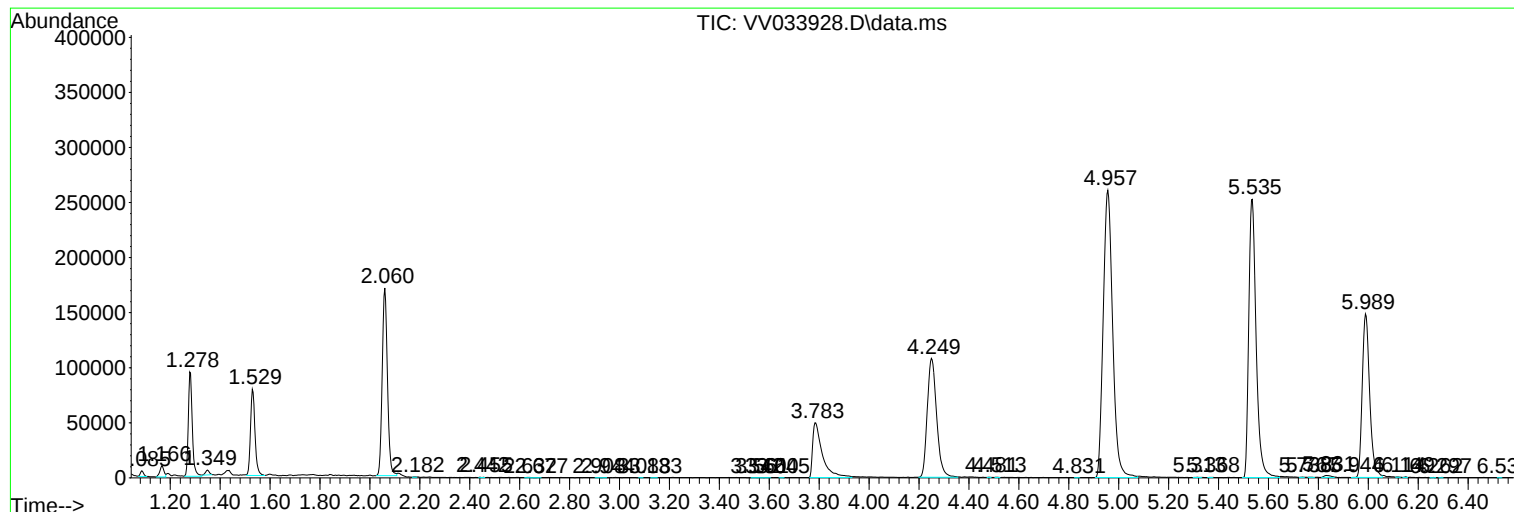

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033928.D
Acq On : 31 Jan 2024 18:16
Operator : SY/MD
Sample : P1309-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033928.D
Acq On : 31 Jan 2024 18:16
Operator : SY/MD
Sample : P1309-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc