

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033930.D
 Acq On : 31 Jan 2024 19:04
 Operator : SY/MD
 Sample : P1309-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH909

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	27	rVB	15506	15995	2.17%	0.265%
2	1.166	32	39	44	rBV	9286	9933	1.35%	0.164%
3	1.281	66	75	90	rBV	102832	115634	15.67%	1.915%
4	1.529	145	152	168	rVB	83954	102381	13.87%	1.695%
5	2.060	306	317	331	rBV	181508	265894	36.02%	4.403%
6	2.188	352	357	361	rVB4	620	676	0.09%	0.011%
7	2.388	416	419	423	rVB2	301	206	0.03%	0.003%
8	2.445	434	437	443	rVB2	451	407	0.06%	0.007%
9	2.474	443	446	451	rVB2	351	311	0.04%	0.005%
10	2.597	481	484	488	rBV2	184	173	0.02%	0.003%
11	2.635	494	496	499	rBV	181	145	0.02%	0.002%
12	2.703	515	517	520	rVV	191	157	0.02%	0.003%
13	2.732	523	526	530	rBV2	162	166	0.02%	0.003%
14	2.757	532	534	539	rVB2	187	168	0.02%	0.003%
15	2.783	539	542	547	rVB2	182	211	0.03%	0.003%
16	2.851	561	563	567	rVB	188	145	0.02%	0.002%
17	2.892	568	576	577	rBV3	439	536	0.07%	0.009%
18	2.973	598	601	603	rBV2	455	241	0.03%	0.004%
19	3.098	638	640	643	rVB	284	178	0.02%	0.003%
20	3.121	643	647	651	rBV2	291	332	0.04%	0.005%
21	3.169	655	662	667	rVB2	247	366	0.05%	0.006%
22	3.301	700	703	705	rBV	206	151	0.02%	0.003%
23	3.339	712	715	719	rBV2	142	151	0.02%	0.003%
24	3.404	728	735	737	rBV2	197	281	0.04%	0.005%
25	3.670	811	818	823	rBV2	246	449	0.06%	0.007%
26	3.732	832	837	840	rBV	173	186	0.03%	0.003%
27	3.783	845	853	890	rBV	56042	147857	20.03%	2.449%
28	4.005	920	922	927	rVB	301	151	0.02%	0.003%
29	4.249	982	998	1029	rBV	116899	301088	40.79%	4.986%
30	4.539	1085	1088	1093	rBV2	301	263	0.04%	0.004%
31	4.957	1202	1218	1253	rBV2	276611	738108	100.00%	12.223%
32	5.362	1341	1344	1347	rBV2	204	151	0.02%	0.003%
33	5.397	1352	1355	1360	rVV2	258	180	0.02%	0.003%
34	5.445	1368	1370	1374	rBV2	257	184	0.02%	0.003%
35	5.535	1387	1398	1426	rBV	265000	539559	73.10%	8.935%
36	5.834	1484	1491	1494	rBV5	1747	2226	0.30%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033930.D
 Acq On : 31 Jan 2024 19:04
 Operator : SY/MD
 Sample : P1309-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH909

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1525	1539	1568	rBV2	160555	332027	44.98%	5.498%
38	6.532	1704	1708	1711	rBV2	168	184	0.02%	0.003%
39	6.706	1754	1762	1764	rBV	189	248	0.03%	0.004%
40	6.828	1796	1800	1802	rBV	148	142	0.02%	0.002%
41	6.915	1817	1827	1856	rBV	97199	180591	24.47%	2.991%
42	7.153	1898	1901	1904	rVB2	288	221	0.03%	0.004%
43	7.243	1917	1929	1971	rBV	334440	589693	79.89%	9.765%
44	7.555	2016	2026	2047	rBV2	65675	117310	15.89%	1.943%
45	7.866	2121	2123	2126	rBV2	224	170	0.02%	0.003%
46	7.927	2136	2142	2147	rBV2	194	335	0.05%	0.006%
47	8.024	2163	2172	2215	rBV	196036	375973	50.94%	6.226%
48	8.410	2286	2292	2295	rBV2	348	454	0.06%	0.008%
49	8.725	2383	2390	2392	rBV	205	243	0.03%	0.004%
50	8.786	2397	2409	2431	rBV	401569	649083	87.94%	10.749%
51	9.021	2479	2482	2484	rBV3	229	157	0.02%	0.003%
52	9.149	2515	2522	2528	rBV2	224	384	0.05%	0.006%
53	9.362	2584	2588	2590	rBV	166	163	0.02%	0.003%
54	9.416	2601	2605	2609	rBV2	135	179	0.02%	0.003%
55	9.538	2637	2643	2645	rBV2	233	282	0.04%	0.005%
56	9.590	2653	2659	2663	rBV2	243	340	0.05%	0.006%
57	9.635	2670	2673	2676	rBV2	198	184	0.02%	0.003%
58	9.741	2703	2706	2708	rBV	184	135	0.02%	0.002%
59	9.776	2712	2717	2720	rBV2	161	147	0.02%	0.002%
60	9.805	2720	2726	2733	rVB2	211	342	0.05%	0.006%
61	9.853	2735	2741	2743	rBV2	228	245	0.03%	0.004%
62	10.098	2814	2817	2820	rBV	249	181	0.02%	0.003%
63	10.152	2822	2834	2860	rVV	227145	353362	47.87%	5.852%
64	10.255	2864	2866	2869	rVB2	278	142	0.02%	0.002%
65	10.294	2873	2878	2880	rBV2	204	199	0.03%	0.003%
66	10.506	2940	2944	2947	rBV2	198	207	0.03%	0.003%
67	10.529	2947	2951	2952	rBV	155	135	0.02%	0.002%
68	10.583	2965	2968	2969	rBV	206	137	0.02%	0.002%
69	10.741	3011	3017	3019	rBV2	187	208	0.03%	0.003%
70	10.760	3019	3023	3026	rVV	123	139	0.02%	0.002%
71	10.831	3039	3045	3048	rBV2	225	285	0.04%	0.005%
72	10.911	3064	3070	3073	rBV2	261	331	0.04%	0.005%
73	11.185	3144	3155	3181	rBV	412339	635986	86.16%	10.532%
74	11.374	3211	3214	3217	rBV3	200	158	0.02%	0.003%
75	11.561	3260	3272	3297	rBV	348027	545139	73.86%	9.027%
76	11.731	3320	3325	3326	rBV2	244	223	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033930.D
 Acq On : 31 Jan 2024 19:04
 Operator : SY/MD
 Sample : P1309-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH909

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.763	3332	3335	3337	rBV	194	173	0.02%	0.003%
78	11.844	3357	3360	3363	rVB	244	189	0.03%	0.003%
79	11.869	3363	3368	3369	rBV	218	203	0.03%	0.003%
80	12.226	3474	3479	3482	rVB2	199	182	0.02%	0.003%
81	12.246	3482	3485	3488	rBV2	176	174	0.02%	0.003%
82	12.300	3496	3502	3506	rBV2	1349	1374	0.19%	0.023%
83	12.377	3519	3526	3528	rBV2	185	280	0.04%	0.005%
84	12.451	3546	3549	3552	rBV2	207	207	0.03%	0.003%
85	12.924	3692	3696	3697	rBV2	233	149	0.02%	0.002%
86	13.043	3730	3733	3735	rBV	255	205	0.03%	0.003%
87	13.249	3794	3797	3801	rBV	177	161	0.02%	0.003%
88	13.619	3908	3912	3914	rBV2	180	185	0.03%	0.003%
89	13.660	3922	3925	3927	rBV	337	257	0.03%	0.004%
90	13.731	3944	3947	3949	rBV2	215	178	0.02%	0.003%
91	13.988	4024	4027	4030	rVB	380	254	0.03%	0.004%
92	14.104	4059	4063	4066	rBV2	476	434	0.06%	0.007%
93	14.210	4094	4096	4100	rVB3	281	152	0.02%	0.003%
94	14.229	4100	4102	4108	rBV2	383	442	0.06%	0.007%
95	14.538	4195	4198	4201	rBV2	261	192	0.03%	0.003%
96	14.654	4230	4234	4237	rBV3	347	303	0.04%	0.005%
97	15.001	4335	4342	4343	rBV2	413	495	0.07%	0.008%
98	15.046	4353	4356	4360	rBV2	376	248	0.03%	0.004%
99	15.368	4452	4456	4460	rBV4	638	655	0.09%	0.011%
100	15.474	4486	4489	4491	rBV2	314	267	0.04%	0.004%




Sum of corrected areas: 6038663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033930.D
Acq On : 31 Jan 2024 19:04
Operator : SY/MD
Sample : P1309-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH909

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

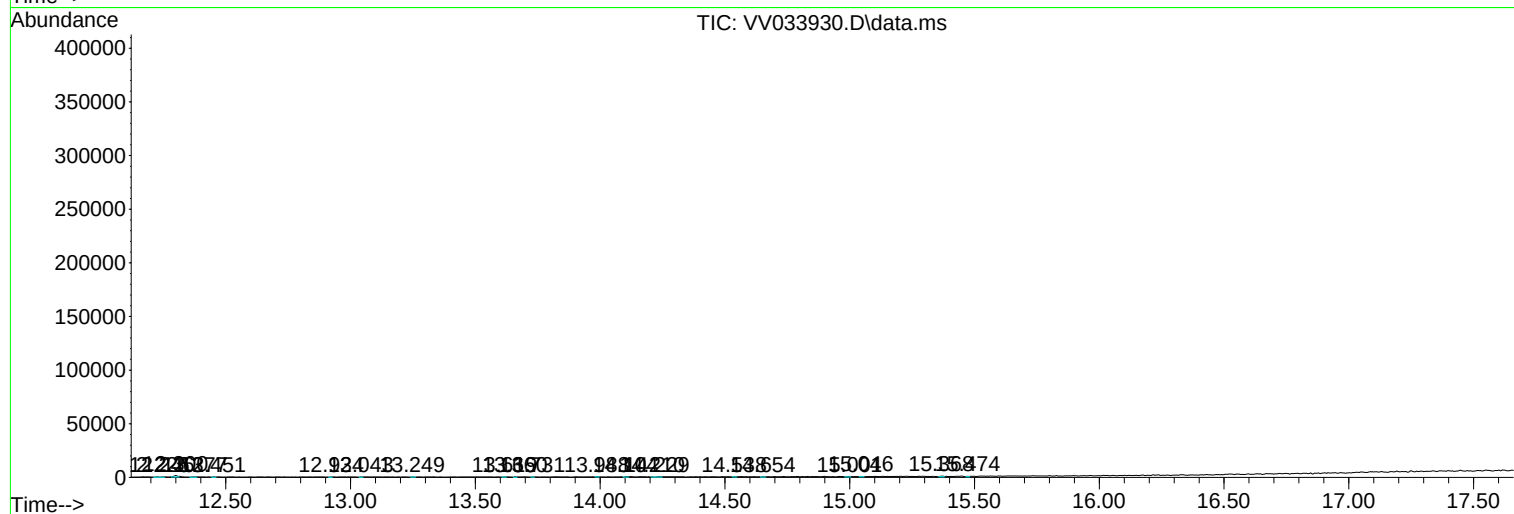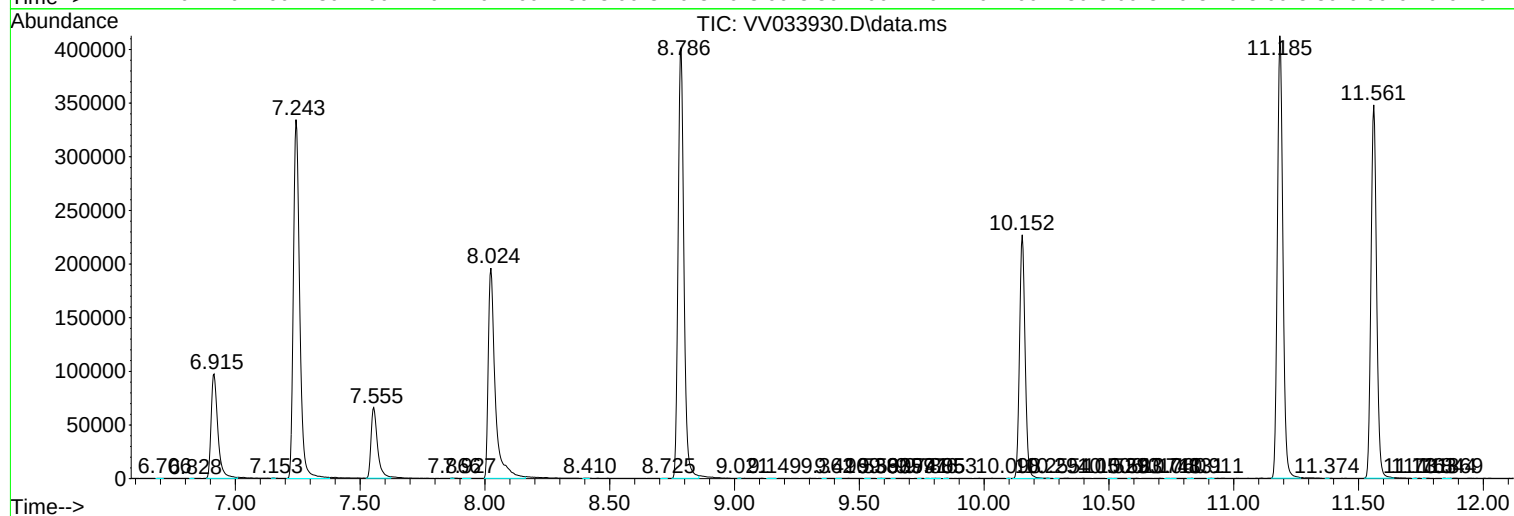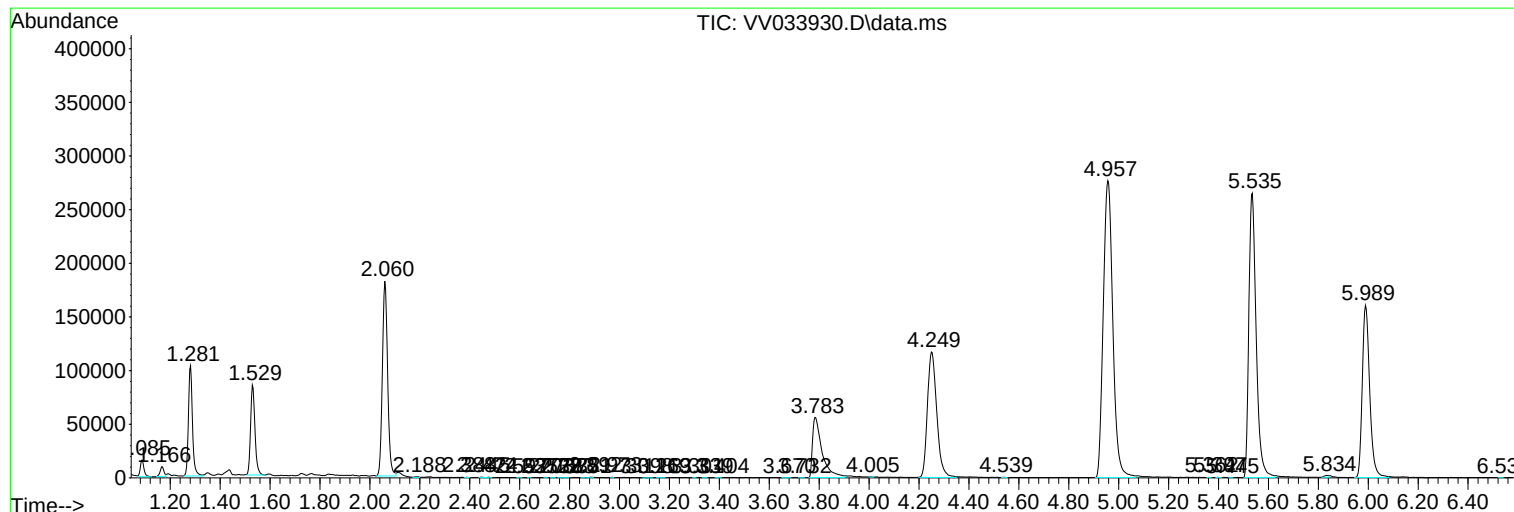

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033930.D
Acq On : 31 Jan 2024 19:04
Operator : SY/MD
Sample : P1309-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH909

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033930.D
Acq On : 31 Jan 2024 19:04
Operator : SY/MD
Sample : P1309-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH909

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc