

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033931.D
 Acq On : 31 Jan 2024 19:28
 Operator : SY/MD
 Sample : P1309-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH913

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.086	10	14	23	rVB2	4674	5277	0.75%	0.092%
2	1.166	31	39	44	rBV2	9162	10874	1.55%	0.189%
3	1.214	51	54	62	rVB	1884	1860	0.27%	0.032%
4	1.278	67	74	90	rBV	97103	103669	14.81%	1.806%
5	1.349	92	96	102	rVB2	2864	2863	0.41%	0.050%
6	1.529	144	152	168	rVB	80119	95688	13.67%	1.667%
7	2.060	306	317	330	rBV	169638	251342	35.91%	4.380%
8	2.179	351	354	361	rVB3	659	736	0.11%	0.013%
9	2.230	366	370	375	rVB4	348	374	0.05%	0.007%
10	2.275	382	384	386	rBV	315	171	0.02%	0.003%
11	2.391	418	420	425	rVB2	300	191	0.03%	0.003%
12	2.446	433	437	441	rBV4	535	555	0.08%	0.010%
13	2.520	455	460	464	rBV2	220	295	0.04%	0.005%
14	2.851	556	563	565	rBV2	182	182	0.03%	0.003%
15	2.976	599	602	604	rBV3	312	209	0.03%	0.004%
16	3.220	675	678	684	rBV2	222	262	0.04%	0.005%
17	3.349	714	718	721	rBV	176	176	0.03%	0.003%
18	3.397	730	733	735	rBV	213	163	0.02%	0.003%
19	3.516	762	770	775	rVB2	202	325	0.05%	0.006%
20	3.565	781	785	788	rBV	194	205	0.03%	0.004%
21	3.664	809	816	820	rBV2	226	275	0.04%	0.005%
22	3.706	826	829	834	rBV2	173	168	0.02%	0.003%
23	3.783	843	853	897	rBV	51093	140284	20.04%	2.444%
24	4.249	980	998	1026	rBV2	111020	284399	40.63%	4.956%
25	4.458	1059	1063	1064	rBV	301	201	0.03%	0.004%
26	4.558	1091	1094	1096	rBV2	316	215	0.03%	0.004%
27	4.651	1119	1123	1130	rBV2	238	324	0.05%	0.006%
28	4.902	1193	1201	1202	rBV	268	304	0.04%	0.005%
29	4.957	1202	1218	1250	rBV2	262860	699958	100.00%	12.197%
30	5.169	1283	1284	1288	rBV3	245	166	0.02%	0.003%
31	5.208	1294	1296	1300	rVB2	443	296	0.04%	0.005%
32	5.346	1337	1339	1344	rVV2	241	217	0.03%	0.004%
33	5.532	1386	1397	1427	rBV	253591	521057	74.44%	9.080%
34	5.831	1484	1490	1491	rBV4	1425	1287	0.18%	0.022%
35	5.989	1524	1539	1573	rVV2	154334	318223	45.46%	5.545%
36	6.188	1598	1601	1605	rVV3	241	199	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033931.D
 Acq On : 31 Jan 2024 19:28
 Operator : SY/MD
 Sample : P1309-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH913

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.738	1768	1772	1776	rBV2	153	168	0.02%	0.003%
38	6.764	1776	1780	1783	rBV2	180	175	0.03%	0.003%
39	6.812	1791	1795	1797	rBV	171	175	0.03%	0.003%
40	6.915	1815	1827	1857	rBV	91058	172073	24.58%	2.998%
41	7.092	1880	1882	1886	rVB	304	179	0.03%	0.003%
42	7.137	1891	1896	1900	rVV2	260	253	0.04%	0.004%
43	7.179	1904	1909	1913	rVB2	265	259	0.04%	0.005%
44	7.243	1918	1929	1956	rBV	314497	553441	79.07%	9.644%
45	7.555	2016	2026	2055	rBV	62072	111552	15.94%	1.944%
46	7.654	2055	2057	2062	rVB2	366	255	0.04%	0.004%
47	7.712	2073	2075	2082	rVB3	275	198	0.03%	0.003%
48	7.851	2110	2118	2120	rBV	235	301	0.04%	0.005%
49	7.876	2120	2126	2135	rVB2	448	739	0.11%	0.013%
50	8.024	2163	2172	2214	rBV	177041	343354	49.05%	5.983%
51	8.362	2275	2277	2281	rVV2	355	211	0.03%	0.004%
52	8.645	2362	2365	2368	rBV	169	161	0.02%	0.003%
53	8.783	2398	2408	2437	rBV	378486	626503	89.51%	10.917%
54	8.963	2460	2464	2466	rBV2	290	200	0.03%	0.003%
55	8.995	2470	2474	2477	rBV3	194	164	0.02%	0.003%
56	9.082	2497	2501	2503	rBV2	445	307	0.04%	0.005%
57	9.182	2529	2532	2539	rVB2	260	287	0.04%	0.005%
58	9.220	2539	2544	2550	rBV2	184	241	0.03%	0.004%
59	9.410	2599	2603	2612	rVB2	253	372	0.05%	0.006%
60	9.465	2614	2620	2622	rBV2	494	418	0.06%	0.007%
61	9.693	2689	2691	2698	rVB2	162	193	0.03%	0.003%
62	10.153	2823	2834	2857	rVV	207197	330141	47.17%	5.753%
63	10.307	2877	2882	2883	rBV	307	224	0.03%	0.004%
64	10.330	2884	2889	2895	rVB2	514	729	0.10%	0.013%
65	10.699	3000	3004	3010	rVB2	250	328	0.05%	0.006%
66	10.744	3010	3018	3020	rBV2	236	375	0.05%	0.007%
67	10.793	3028	3033	3041	rBV2	230	355	0.05%	0.006%
68	10.828	3041	3044	3047	rBV2	200	185	0.03%	0.003%
69	10.911	3067	3070	3073	rBV2	211	203	0.03%	0.004%
70	11.034	3099	3108	3111	rBV3	419	617	0.09%	0.011%
71	11.101	3122	3129	3137	rBV6	1524	2390	0.34%	0.042%
72	11.185	3141	3155	3185	rVV	396066	618349	88.34%	10.775%
73	11.561	3259	3272	3291	rBV	330087	516333	73.77%	8.997%
74	11.722	3317	3322	3325	rBV2	509	543	0.08%	0.009%
75	11.918	3379	3383	3387	rBV2	129	160	0.02%	0.003%
76	11.940	3387	3390	3395	rVB2	274	233	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
 Data File : VV033931.D
 Acq On : 31 Jan 2024 19:28
 Operator : SY/MD
 Sample : P1309-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH913

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.995	3404	3407	3414	rBV2	167	233	0.03%	0.004%
78	12.043	3419	3422	3426	rVB2	302	243	0.03%	0.004%
79	12.066	3426	3429	3434	rBV2	194	241	0.03%	0.004%
80	12.230	3477	3480	3483	rBV2	196	182	0.03%	0.003%
81	12.297	3493	3501	3509	rVV5	4416	6526	0.93%	0.114%
82	12.333	3509	3512	3516	rVB3	717	458	0.07%	0.008%
83	12.706	3623	3628	3629	rBV	197	194	0.03%	0.003%
84	12.918	3689	3694	3696	rBV	173	163	0.02%	0.003%
85	13.477	3861	3868	3870	rBV	269	312	0.04%	0.005%
86	13.577	3894	3899	3902	rBV2	185	218	0.03%	0.004%
87	13.847	3979	3983	3986	rBV	154	169	0.02%	0.003%
88	13.989	4023	4027	4030	rBV	277	228	0.03%	0.004%
89	14.230	4098	4102	4103	rBV2	290	171	0.02%	0.003%
90	14.374	4142	4147	4150	rVB2	379	389	0.06%	0.007%
91	14.403	4152	4156	4158	rBV3	312	268	0.04%	0.005%
92	14.593	4209	4215	4217	rBV3	303	353	0.05%	0.006%
93	14.670	4237	4239	4246	rVB3	256	253	0.04%	0.004%
94	14.985	4334	4337	4339	rBV	238	194	0.03%	0.003%
95	15.050	4355	4357	4362	rBV3	261	242	0.03%	0.004%
96	15.178	4395	4397	4401	rVB2	288	184	0.03%	0.003%
97	15.545	4509	4511	4513	rBV	448	300	0.04%	0.005%
98	15.609	4529	4531	4537	rBV3	530	405	0.06%	0.007%
99	15.818	4594	4596	4599	rBV2	469	266	0.04%	0.005%
100	16.030	4660	4662	4664	rVB3	651	271	0.04%	0.005%




Sum of corrected areas: 5738797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033931.D
Acq On : 31 Jan 2024 19:28
Operator : SY/MD
Sample : P1309-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH913

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

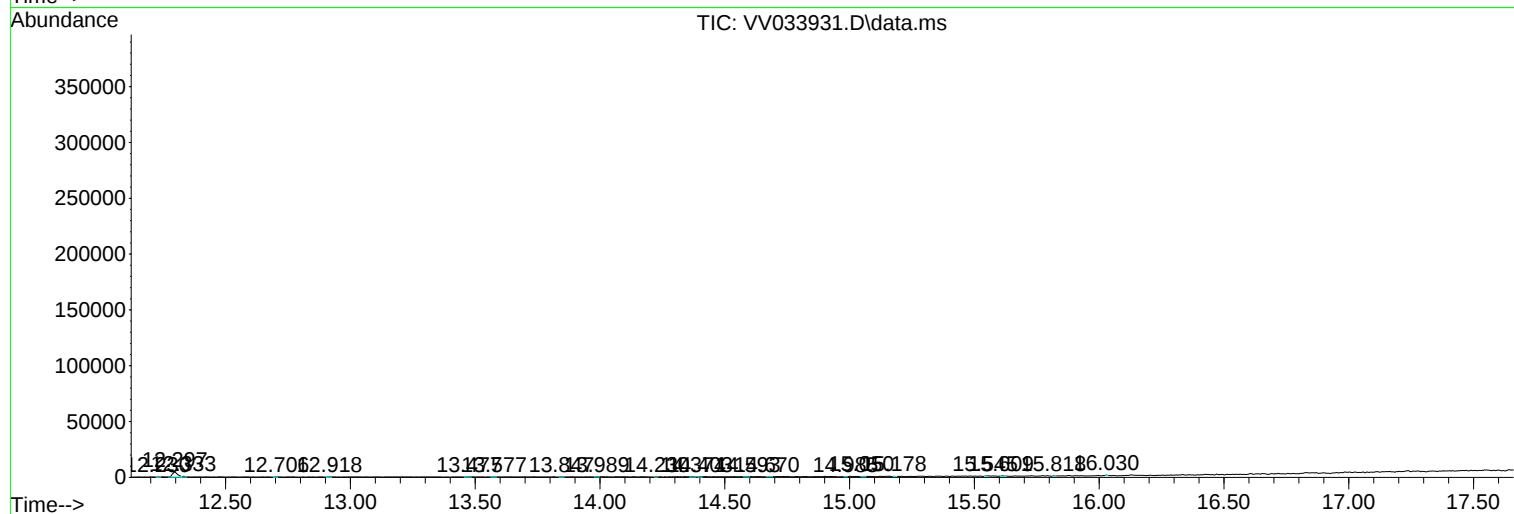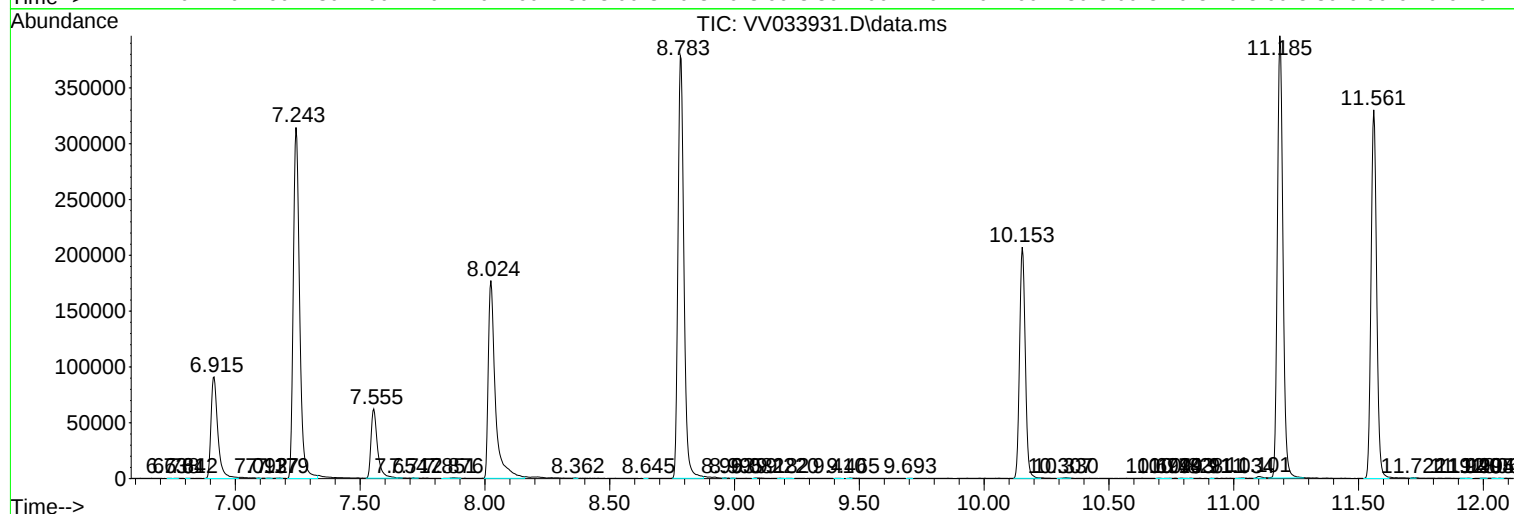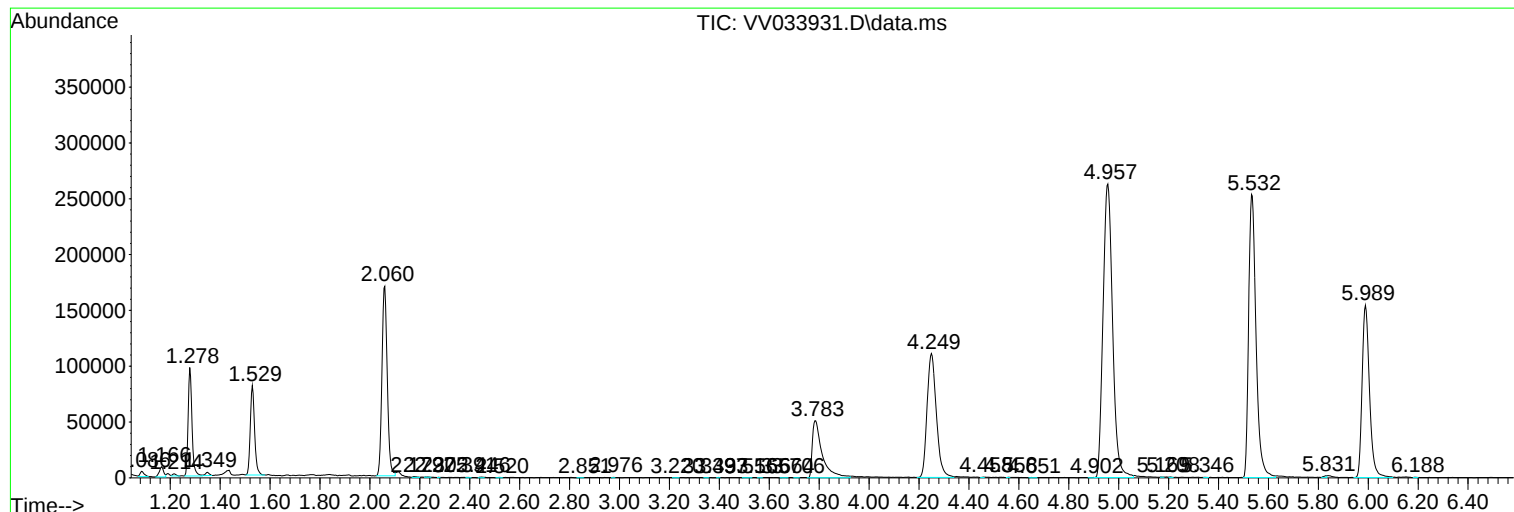

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033931.D
Acq On : 31 Jan 2024 19:28
Operator : SY/MD
Sample : P1309-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH913

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033931.D
Acq On : 31 Jan 2024 19:28
Operator : SY/MD
Sample : P1309-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH913

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------