


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV013124\
Data File : VV033910.D
Acq On : 31 Jan 2024 08:36
Operator : SY/MD
Sample : BFB259
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB259

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Fri Feb 02 04:28:29 2024

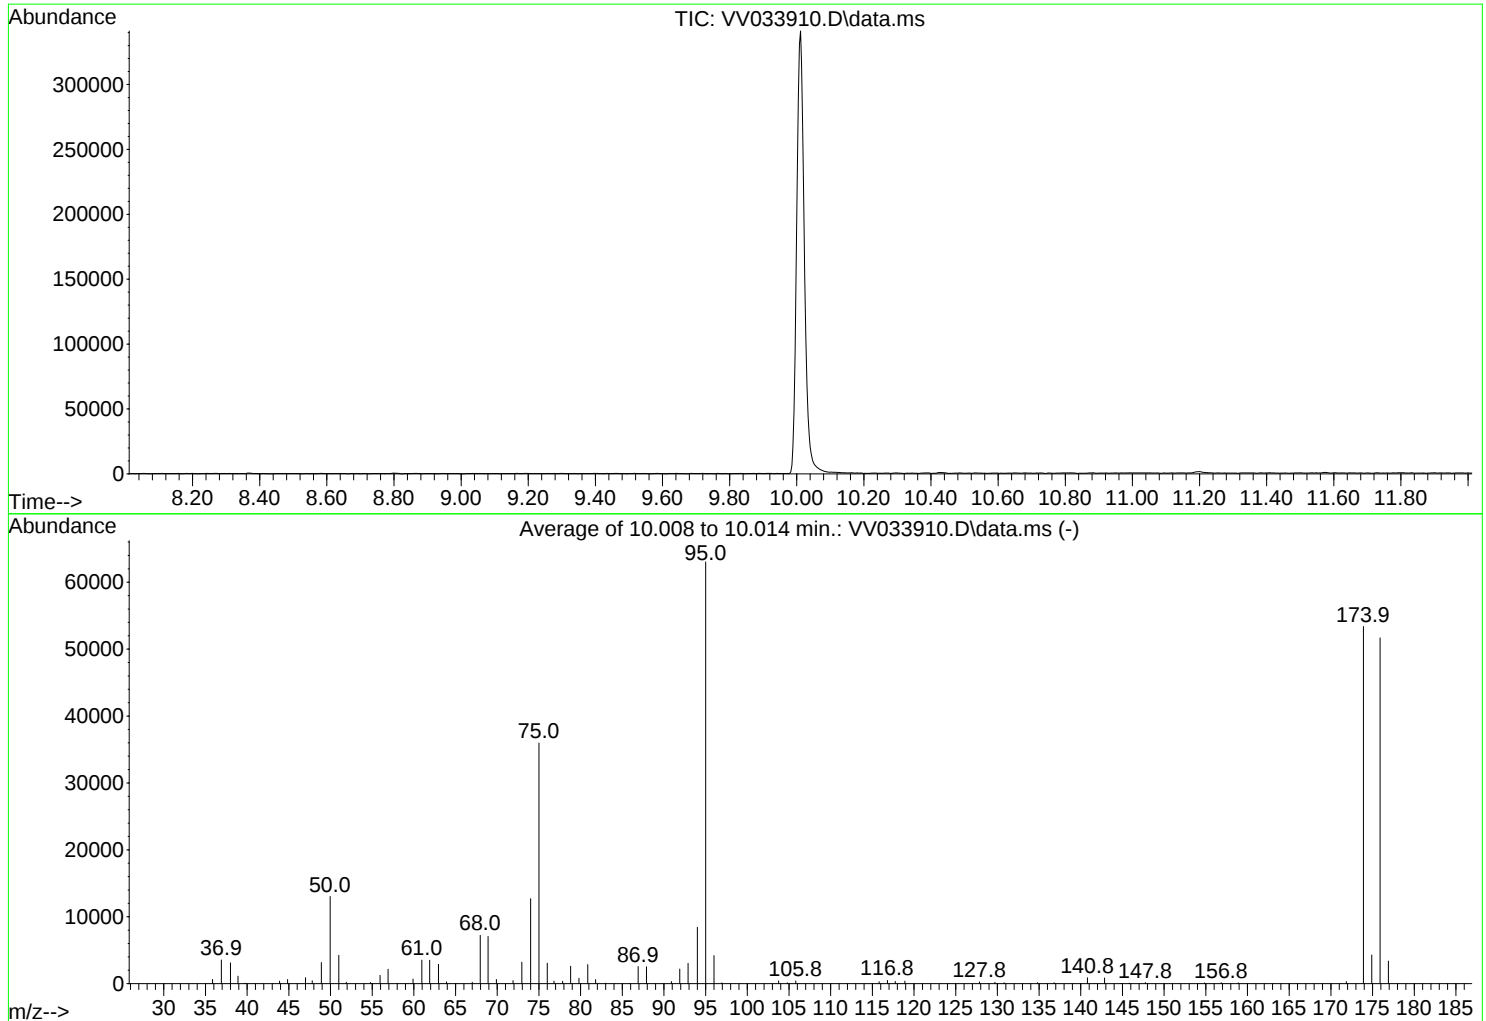

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	13033	PASS
75	95	30	80	57.1	35976	PASS
95	95	100	100	100.0	63048	PASS
96	95	5	9	6.6	4187	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	53392	PASS
175	174	5	9	8.0	4274	PASS
176	174	95	105	96.8	51693	PASS
177	176	5	10	6.5	3369	PASS

m/z	Abundance
39.70	145.0
43.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.80	596.0
36.90	3611.0
38.00	3177.0
38.90	1174.0
39.90	237.0
43.90	567.0
44.90	646.0
47.00	981.0
47.80	403.0
48.90	3263.0
50.00	13386.0
51.00	4382.0
51.90	191.0
54.80	164.0
56.00	1333.0
56.90	2208.0
58.00	120.0
59.90	704.0
60.90	3520.0
61.90	3482.0
63.00	2986.0
63.90	239.0
67.00	212.0
67.90	7302.0
68.90	7287.0
69.90	699.0
71.90	413.0
73.00	3240.0
74.00	12645.0
75.00	35840.0
76.00	3104.0
76.80	323.0
77.80	346.0
78.80	2626.0
79.80	833.0
80.80	2966.0
81.80	596.0
82.90	122.0
85.90	108.0
86.90	2578.0
87.90	2410.0
91.00	348.0
91.90	2142.0
92.90	3009.0
94.00	8436.0
95.00	64016.0
96.00	4345.0
97.00	108.0
103.80	388.0
104.80	151.0
105.80	411.0
115.80	334.0
116.80	444.0
117.80	341.0
118.80	373.0
127.90	258.0
129.70	226.0
130.80	146.0
134.80	172.0
136.80	133.0
140.80	876.0
142.00	104.0
142.90	902.0
147.80	176.0
154.80	139.0
156.80	144.0
158.90	126.0
171.80	325.0
173.90	52448.0
174.90	4380.0
175.90	51296.0
176.90	3338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.90	632.0
36.90	3689.0
38.00	3231.0
38.90	1180.0
39.80	204.0
43.90	535.0
44.80	653.0
47.00	921.0
47.80	453.0
48.90	3271.0
50.00	13434.0
51.00	4458.0
51.90	210.0
54.80	173.0
55.90	1311.0
56.90	2234.0
59.90	743.0
60.90	3646.0
61.90	3593.0
63.00	3018.0
63.90	273.0
67.00	226.0
67.90	7503.0
68.90	7243.0
69.90	635.0
71.90	483.0
72.90	3282.0
74.00	13189.0
75.00	37168.0
76.00	3198.0
76.80	393.0
77.90	387.0
78.80	2727.0
79.80	859.0
80.90	2904.0
81.80	610.0
83.00	124.0
86.90	2625.0
87.90	2620.0
90.90	313.0
91.90	2259.0
92.90	3144.0
94.00	8715.0
95.00	65144.0
96.00	4275.0
96.90	117.0
103.70	421.0
104.80	143.0
105.80	429.0
115.80	309.0
116.80	508.0
117.80	357.0
118.90	407.0
127.90	271.0
129.70	229.0
130.80	146.0
134.80	159.0
136.80	167.0
140.80	914.0
141.60	104.0
142.90	882.0
145.80	117.0
147.70	186.0
154.90	130.0
156.90	152.0
158.90	140.0
171.90	322.0
173.90	55272.0
174.90	4417.0
175.90	53528.0
176.90	3519.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.90	618.0
36.90	3345.0
38.00	2946.0
38.90	1040.0
39.80	190.0
43.90	492.0
44.90	572.0
47.00	786.0
47.80	442.0
48.90	2914.0
49.90	12280.0
51.00	3880.0
51.90	224.0
54.80	163.0
55.90	1122.0
56.90	2039.0
59.90	664.0
61.00	3407.0
61.90	3410.0
62.90	2680.0
63.90	257.0
67.00	205.0
68.00	6899.0
68.90	6622.0
69.90	542.0
71.90	467.0
72.90	3065.0
74.00	12282.0
75.00	34920.0
76.00	2917.0
76.80	407.0
77.90	372.0
78.80	2493.0
79.80	776.0
80.90	2645.0
81.80	563.0
86.90	2452.0
87.90	2506.0
90.80	271.0
91.90	2111.0
92.90	2947.0
94.00	8096.0
95.00	59984.0
96.00	3940.0
97.00	114.0
103.70	385.0
104.80	127.0
105.80	380.0
115.80	246.0
116.80	512.0
117.70	329.0
118.90	383.0
127.80	264.0
128.90	101.0
129.70	219.0
130.80	130.0
134.80	133.0
136.80	165.0
140.80	854.0
142.80	735.0
144.80	117.0
145.80	128.0
147.70	164.0
154.90	125.0
156.90	145.0
158.90	125.0
171.80	260.0
173.90	52456.0
174.90	4025.0
175.90	50256.0
176.90	3251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259