
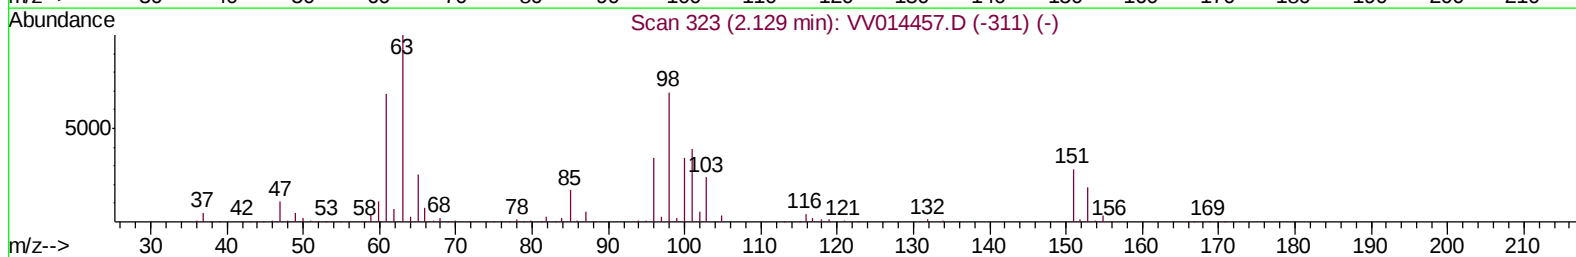
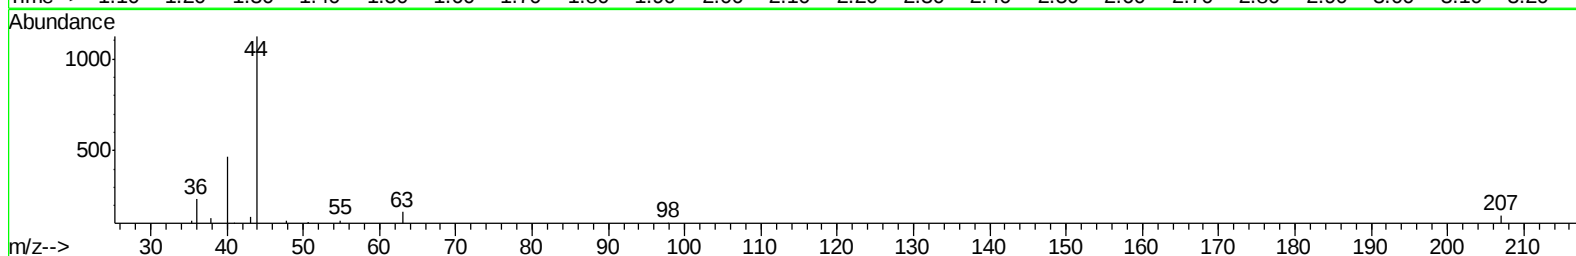


Data File : VV014458.D  
Acq On : 31 Jan 2020 18:36  
Operator : SY/MD  
Sample : VV0131MBL01  
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 01 02:40:26 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM020120WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Feb 01 02:36:06 2020  
Response via : Initial Calibration

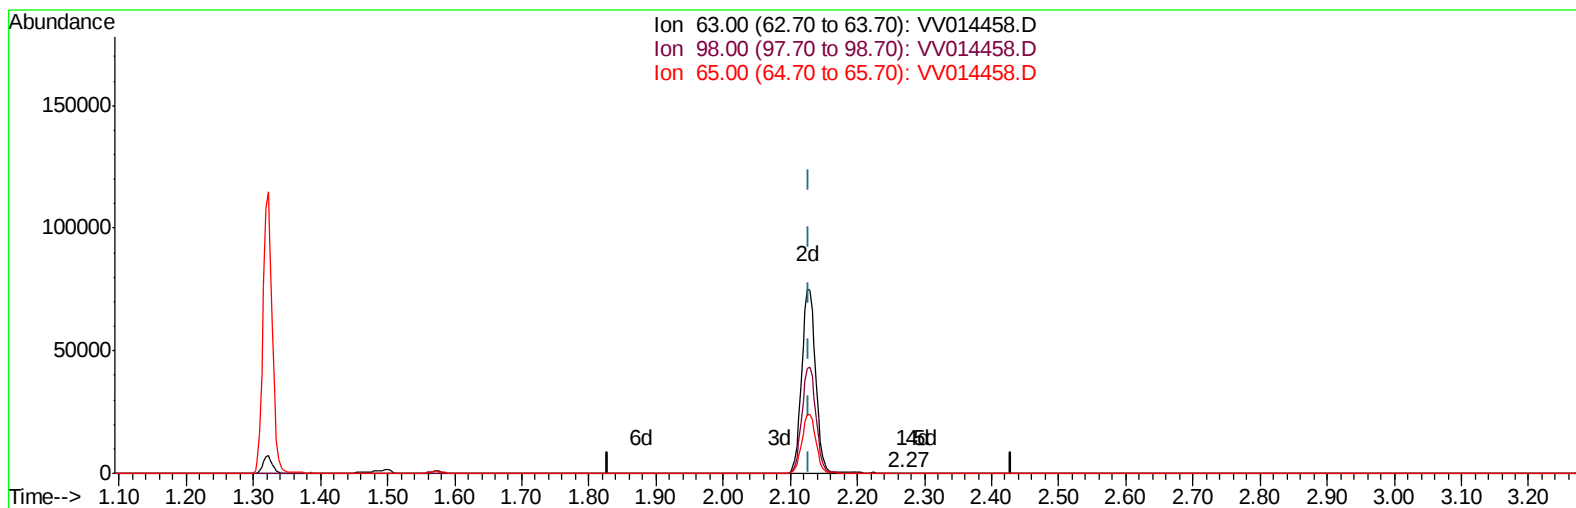

TIC: VV014458.D

(11) 1,1-Dichloroethene-d2 (S)

2.267min (+0.138) 0.05ug/L

response 164

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 63.00 | 100   | 100   |
| 98.00 | 74.30 | 78.66 |
| 65.00 | 22.80 | 25.61 |
| 0.00  | 0.00  | 0.00  |