
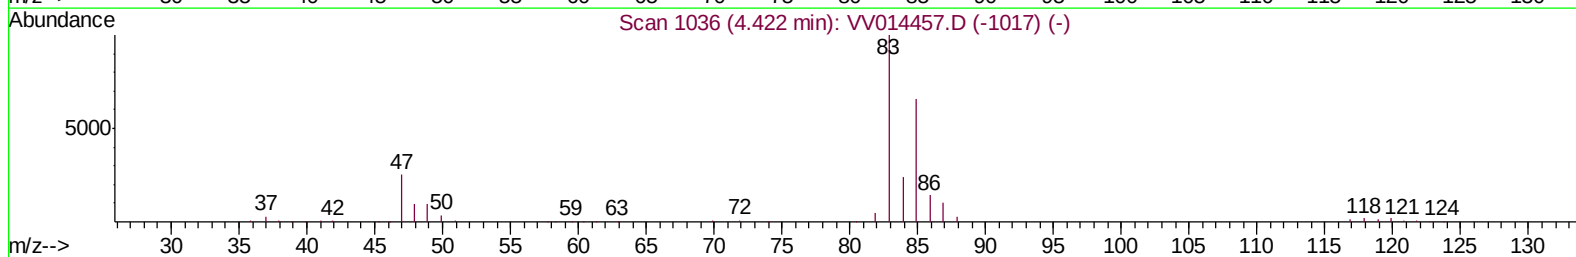
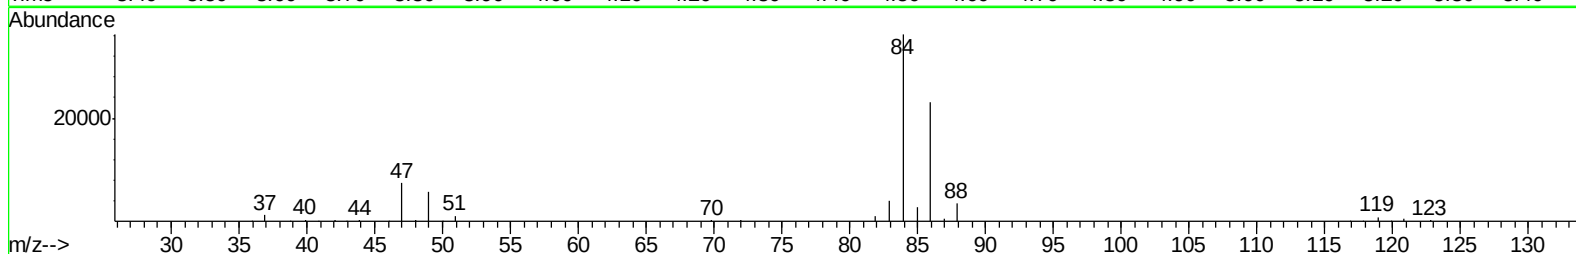


Data File : VV014475.D
Acq On : 01 Feb 2020 01:20
Operator : SY/MD
Sample : L1323-12 10X
Misc : 5.09g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Feb 01 02:42:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 01 02:36:06 2020
Response via : Initial Calibration

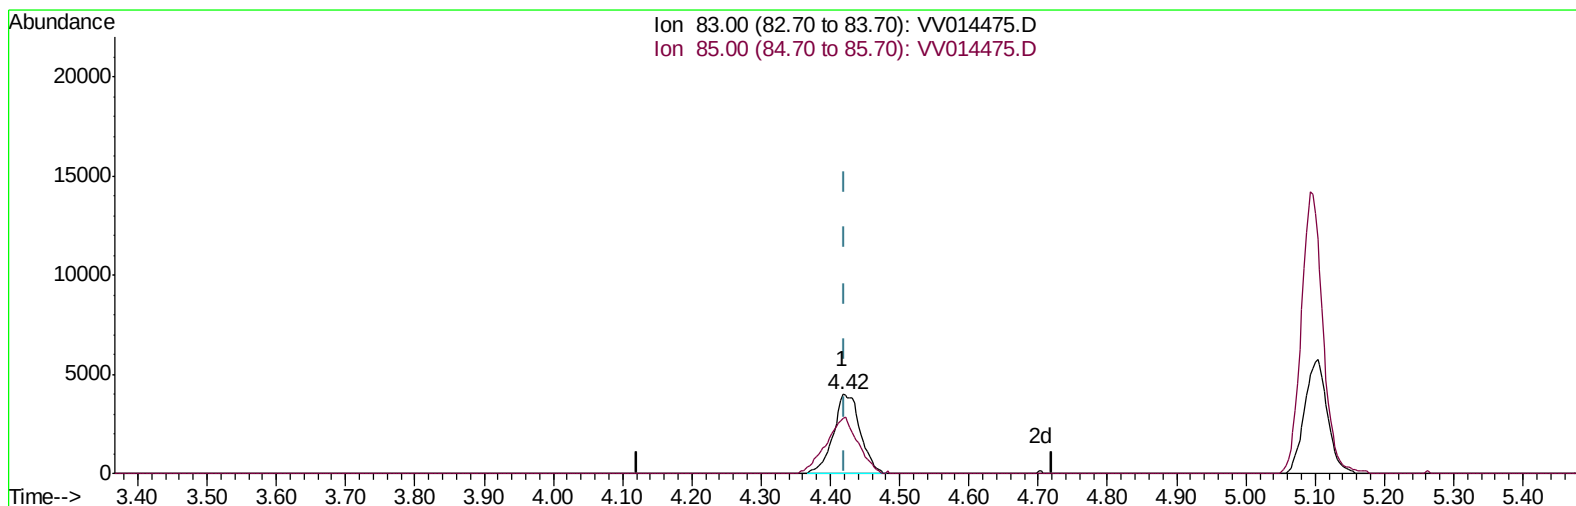

TIC: VV014475.D

(25) Chloroform (T)

4.418min (-0.003) 2.13ug/L m

response 10638

Ion	Exp%	Act%
83.00	100	100
85.00	64.40	69.83
0.00	0.00	0.00
0.00	0.00	0.00