

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020120\
 Data File : VV014471.D
 Acq On : 31 Jan 2020 23:45
 Operator : SY/MD
 Sample : L1323-03 10X
 Misc : 5.03g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAT43

Quant Time: Feb 01 03:52:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Feb 01 02:36:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	453751	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	427293	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	214792	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	104603	41.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.02%
7) Chloroethane-d5	1.58	69	72444	46.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.48%
11) 1,1-Dichloroethene-d2	2.13	63	116034	34.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.98%
21) 2-Butanone-d5	3.92	46	179739	106.00	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.00%
24) Chloroform-d	4.40	84	230326	43.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.36%
26) 1,2-Dichloroethane-d4	5.08	65	152711	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
32) Benzene-d6	5.10	84	503491	44.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.50%
36) 1,2-Dichloropropane-d6	6.11	67	159206	44.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.46%
41) Toluene-d8	7.35	98	473615	45.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.66	79	81994	45.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.64%
47) 2-Hexanone-d5	8.13	63	149973	107.69	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.69%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	203037	44.27	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.54%
64) 1,2-Dichlorobenzene-d4	11.67	152	180274	45.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.14%


Target Compounds					Ovalue
13) Acetone	2.19	43	2463	1.702 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020120\
Data File : VV014471.D
Acq On : 31 Jan 2020 23:45
Operator : SY/MD
Sample : L1323-03 10X
Misc : 5.03g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAT43

Quant Time: Feb 01 03:52:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 01 02:36:06 2020
Response via : Initial Calibration

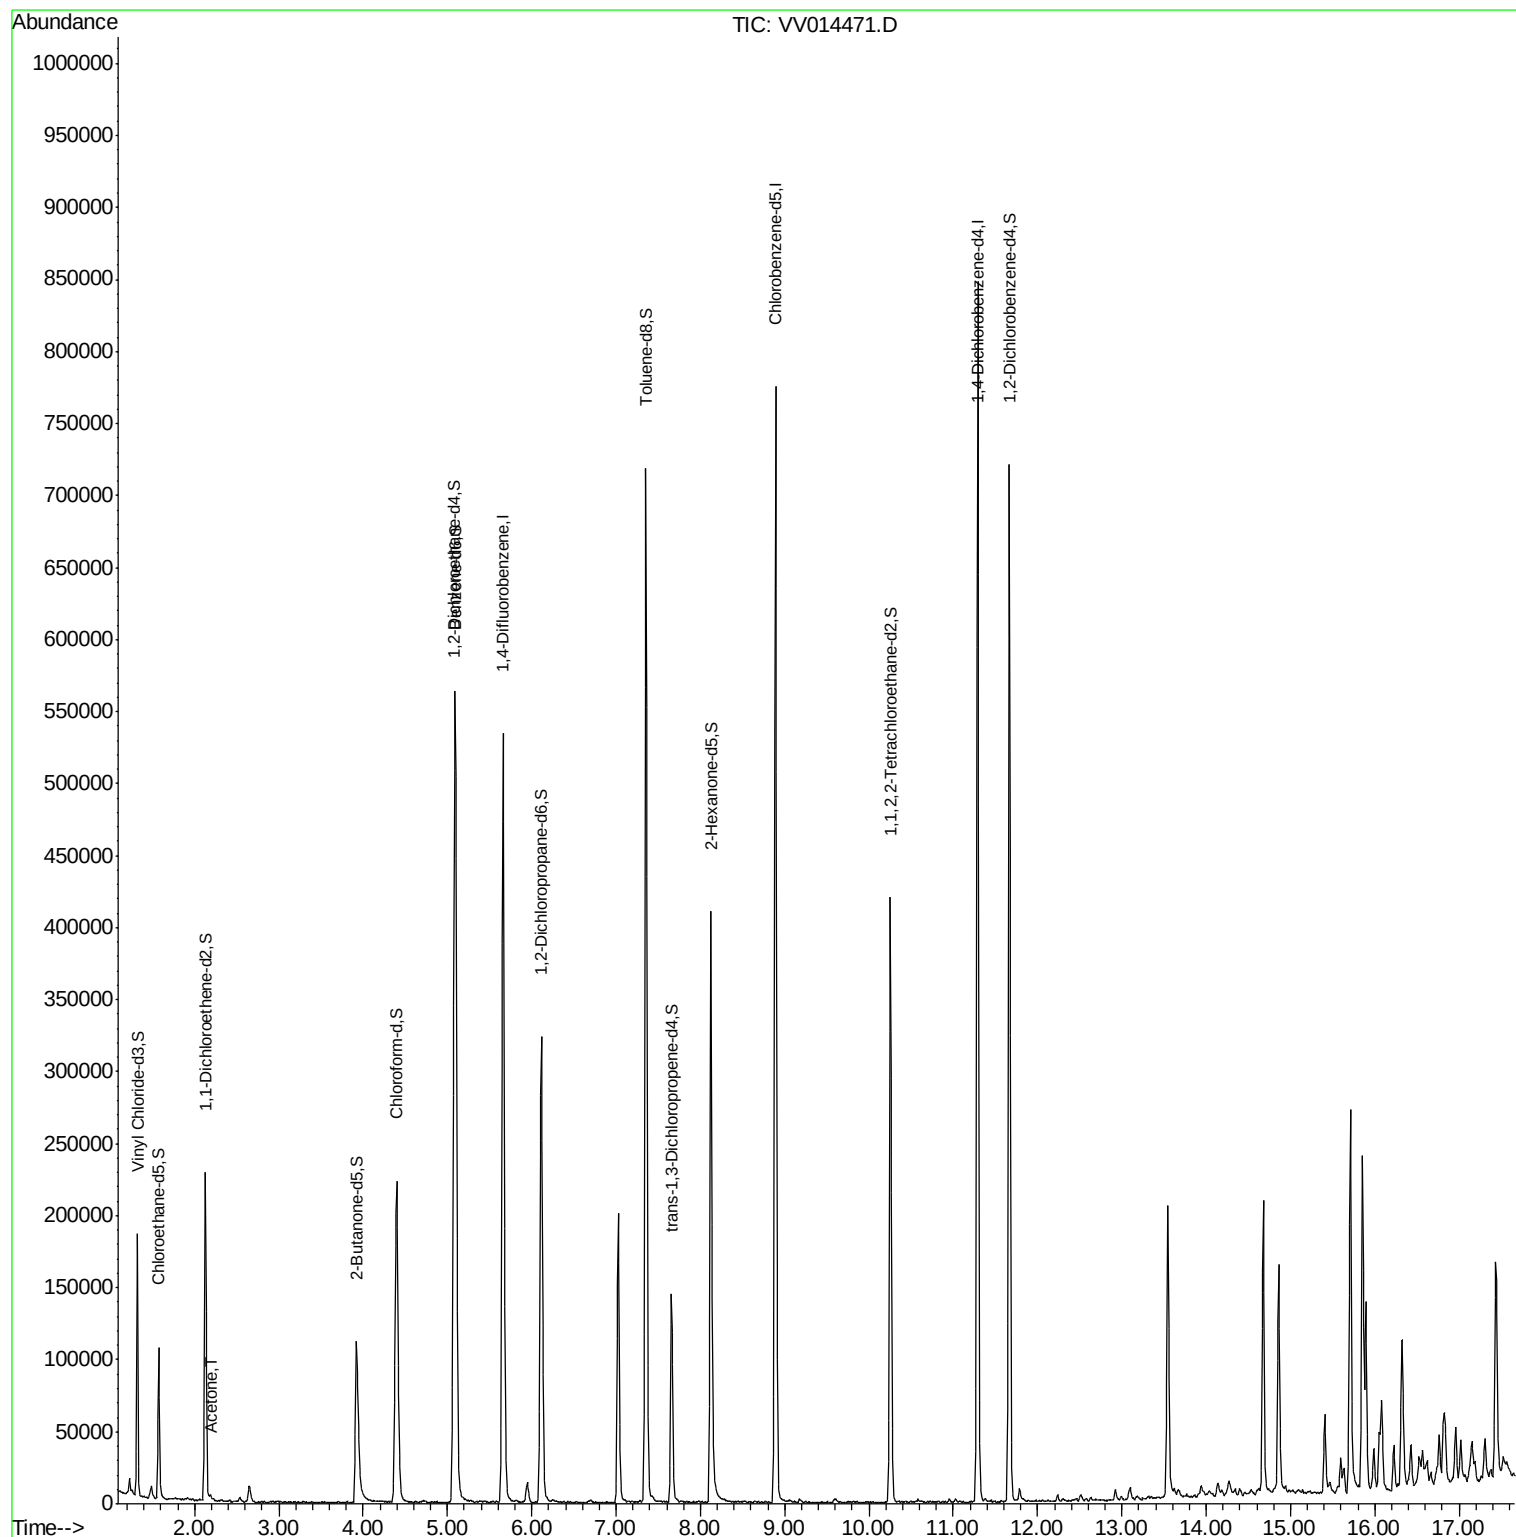

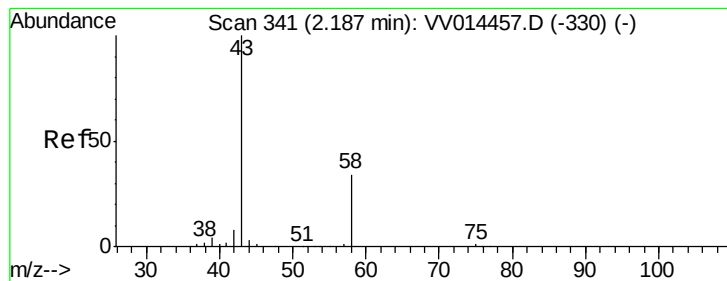

#13

Acetone

Concen: 1.702 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV014471.D

Acq: 31 Jan 2020 23:45

Instrument :
MSVOA_V
ClientSampleId :
GAT43

Tot Ion: 43 Resp: 2463

Ion Ratio Lower Upper

43 100

58 42.5 0.0 61.2

