


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV020120\
 Data File : VV014450.D
 Acq On : 31 Jan 2020 13:45
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 01 02:36:06 2020

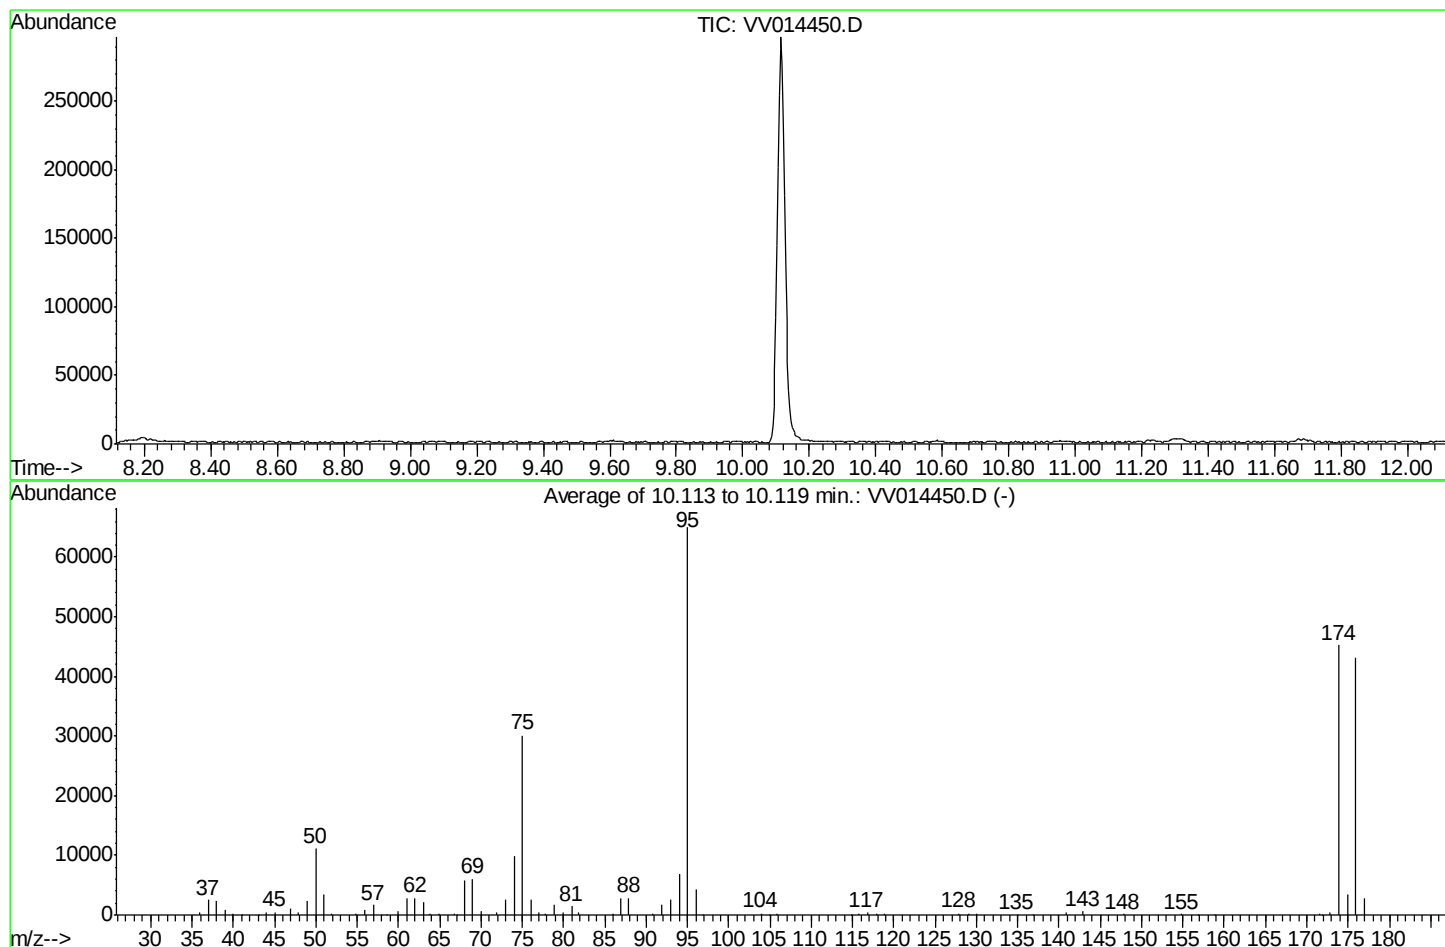

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	11123	PASS
75	95	30	80	46.3	30064	PASS
95	95	100	100	100.0	65000	PASS
96	95	5	9	6.5	4224	PASS
173	174	0.00	2	0.9	404	PASS
174	95	50	120	69.5	45189	PASS
175	174	5	9	7.7	3473	PASS
176	174	95	101	95.4	43114	PASS
177	176	5	9	6.7	2907	PASS

Scan 2793 (10.071 min): VV014450.D
BFB84

m/z	Abundance
39.90	415.0
41.70	112.0
43.00	135.0
44.00	525.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	514.0
37.00	2635.0
38.00	2405.0
38.90	1000.0
39.90	496.0
41.80	103.0
43.20	159.0
44.00	847.0
45.00	570.0
47.00	1066.0
47.80	412.0
49.00	2423.0
50.00	11504.0
51.00	3418.0
51.90	150.0
54.90	186.0
55.90	891.0
57.00	1706.0
60.00	566.0
61.00	2826.0
62.00	2907.0
63.00	2340.0
63.80	203.0
64.90	125.0
66.80	172.0
68.00	5725.0
69.00	6204.0
70.00	572.0
71.90	432.0
72.90	2756.0
74.00	10320.0
75.00	30256.0
76.00	2718.0
77.00	468.0
77.80	244.0
78.90	1674.0
79.80	551.0
81.00	1560.0
81.90	399.0
86.00	104.0
86.90	2855.0
87.90	2807.0
90.70	237.0
92.00	1730.0
93.00	2495.0
94.00	6702.0
95.00	65616.0
96.00	4434.0
96.90	146.0
103.90	237.0
105.80	246.0
114.80	132.0
115.80	265.0
116.80	359.0
117.90	243.0
118.90	270.0
127.90	277.0
129.10	124.0
129.90	122.0
134.80	117.0
140.90	576.0
142.90	617.0
147.80	196.0
154.80	157.0
156.90	106.0
171.50	154.0
172.90	416.0
173.90	45008.0
175.00	3621.0
175.90	41976.0
176.90	2840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	439.0
37.00	2587.0
38.00	2344.0
38.90	998.0
39.90	567.0
41.00	131.0
43.20	141.0
44.00	910.0
45.00	539.0
47.00	1114.0
47.80	417.0
49.00	2557.0
50.00	11525.0
51.00	3519.0
51.90	149.0
54.90	183.0
55.90	877.0
57.00	1783.0
58.00	102.0
58.60	103.0
59.90	634.0
61.00	2799.0
62.00	2883.0
63.00	2274.0
63.90	204.0
64.90	151.0
66.70	153.0
67.10	168.0
68.00	5928.0
69.00	6326.0
70.00	583.0
72.00	425.0
72.90	2782.0
74.00	10299.0
75.00	30912.0
76.00	2803.0
77.00	498.0
77.80	243.0
78.90	1674.0
79.90	541.0
81.00	1429.0
81.80	411.0
86.00	144.0
86.90	2853.0
87.90	2958.0
90.70	220.0
92.00	1674.0
93.00	2574.0
94.00	7109.0
95.00	67168.0
96.00	4364.0
96.90	112.0
103.90	278.0
104.90	126.0
105.80	275.0
115.80	242.0
116.80	382.0
117.90	250.0
118.90	235.0
127.80	278.0
129.10	132.0
130.00	145.0
134.90	111.0
136.80	103.0
140.90	524.0
142.90	642.0
147.80	194.0
154.90	165.0
158.90	121.0
171.50	175.0
172.80	401.0
173.90	46776.0
175.00	3624.0
175.90	44536.0
176.90	2999.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	421.0
37.00	2349.0
38.00	2111.0
39.00	881.0
39.90	631.0
41.10	165.0
43.10	136.0
44.00	861.0
45.00	495.0
46.90	991.0
47.80	378.0
49.00	2329.0
50.00	10342.0
51.00	3194.0
51.90	139.0
54.90	175.0
56.00	740.0
57.00	1624.0
57.90	116.0
58.60	121.0
59.90	557.0
61.00	2616.0
62.00	2611.0
63.00	1976.0
63.90	213.0
64.90	173.0
66.70	146.0
67.10	172.0
68.00	5694.0
69.00	5690.0
69.90	506.0
72.00	401.0
73.00	2519.0
74.00	9284.0
75.00	29024.0
76.00	2475.0
76.90	500.0
77.80	240.0
78.90	1598.0
80.00	518.0
81.00	1228.0
81.80	409.0
86.00	133.0
86.90	2696.0
87.90	2676.0
90.80	202.0
91.90	1555.0
93.00	2378.0
94.00	6842.0
95.00	62216.0
96.00	3875.0
103.90	292.0
104.90	146.0
105.80	284.0
115.80	205.0
116.80	388.0
117.90	234.0
118.90	227.0
127.80	251.0
129.00	114.0
130.00	154.0
135.00	103.0
140.90	486.0
142.90	566.0
147.80	167.0
154.90	169.0
156.70	106.0
157.00	107.0
158.80	116.0
171.60	165.0
171.90	163.0
172.70	395.0
173.90	43784.0
175.00	3174.0
175.90	42832.0
176.90	2884.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84