

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033937.D
 Acq On : 01 Feb 2024 10:38
 Operator : SY/MD
 Sample : P1309-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	23	rVB	14846	14685	2.01%	0.251%
2	1.191	41	47	52	rBV2	4549	4677	0.64%	0.080%
3	1.278	66	74	90	rBV	98622	109719	15.01%	1.877%
4	1.529	145	152	166	rVB	84027	100886	13.81%	1.726%
5	1.597	168	173	181	rVB3	2764	3599	0.49%	0.062%
6	2.060	307	317	331	rBV	177553	258337	35.35%	4.419%
7	2.179	351	354	355	rBV	514	259	0.04%	0.004%
8	2.413	420	427	432	rBV2	355	436	0.06%	0.007%
9	2.622	486	492	496	rBV2	219	340	0.05%	0.006%
10	2.815	546	552	555	rVB	244	302	0.04%	0.005%
11	2.966	595	599	602	rVV3	706	662	0.09%	0.011%
12	2.979	602	603	608	rVB2	765	382	0.05%	0.007%
13	3.021	612	616	619	rVB2	292	197	0.03%	0.003%
14	3.056	623	627	632	rBV2	265	274	0.04%	0.005%
15	3.153	653	657	658	rBV2	278	184	0.03%	0.003%
16	3.179	661	665	673	rVV2	290	514	0.07%	0.009%
17	3.455	748	751	754	rVB	326	251	0.03%	0.004%
18	3.551	778	781	786	rBB2	250	269	0.04%	0.005%
19	3.786	846	854	881	rBV	46948	124161	16.99%	2.124%
20	4.246	981	997	1025	rBV	114349	294632	40.32%	5.040%
21	4.529	1082	1085	1090	rBV3	408	502	0.07%	0.009%
22	4.590	1101	1104	1108	rBV2	188	198	0.03%	0.003%
23	4.748	1149	1153	1157	rBV	158	199	0.03%	0.003%
24	4.857	1184	1187	1189	rBV	219	167	0.02%	0.003%
25	4.953	1201	1217	1260	rBV2	271963	730766	100.00%	12.500%
26	5.233	1302	1304	1308	rVB2	311	215	0.03%	0.004%
27	5.420	1360	1362	1366	rVB2	284	183	0.03%	0.003%
28	5.455	1372	1373	1377	rBV	249	164	0.02%	0.003%
29	5.532	1386	1397	1431	rBV	251954	513731	70.30%	8.787%
30	5.793	1474	1478	1483	rBV2	213	220	0.03%	0.004%
31	5.834	1483	1491	1503	rBV4	2680	5475	0.75%	0.094%
32	5.918	1514	1517	1519	rBV2	324	224	0.03%	0.004%
33	5.985	1526	1538	1570	rBV	158156	330043	45.16%	5.645%
34	6.310	1634	1639	1642	rBV	222	255	0.03%	0.004%
35	6.387	1658	1663	1667	rBV2	211	220	0.03%	0.004%
36	6.439	1676	1679	1684	rVB2	325	335	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033937.D
 Acq On : 01 Feb 2024 10:38
 Operator : SY/MD
 Sample : P1309-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.468	1684	1688	1691	rBV2	318	388	0.05%	0.007%
38	6.542	1706	1711	1714	rBV	216	221	0.03%	0.004%
39	6.783	1782	1786	1789	rBV	188	196	0.03%	0.003%
40	6.841	1802	1804	1809	rBV	153	197	0.03%	0.003%
41	6.911	1815	1826	1860	rBV	95494	179646	24.58%	3.073%
42	7.159	1899	1903	1908	rBV3	280	200	0.03%	0.003%
43	7.243	1917	1929	1972	rBV	331233	586450	80.25%	10.031%
44	7.555	2016	2026	2054	rBV	63100	116417	15.93%	1.991%
45	7.802	2100	2103	2107	rBV	277	239	0.03%	0.004%
46	7.860	2118	2121	2122	rBV	314	185	0.03%	0.003%
47	7.876	2123	2126	2138	rVB3	737	1063	0.15%	0.018%
48	8.024	2163	2172	2186	rBV	163564	291298	39.86%	4.983%
49	8.284	2247	2253	2258	rBV3	566	792	0.11%	0.014%
50	8.381	2278	2283	2284	rBV2	190	186	0.03%	0.003%
51	8.548	2331	2335	2338	rBV2	227	221	0.03%	0.004%
52	8.612	2352	2355	2359	rBV	202	224	0.03%	0.004%
53	8.715	2383	2387	2391	rBV	209	225	0.03%	0.004%
54	8.783	2397	2408	2440	rBV	379840	625716	85.62%	10.703%
55	9.005	2473	2477	2484	rVB2	379	427	0.06%	0.007%
56	9.037	2484	2487	2490	rBV	220	176	0.02%	0.003%
57	9.088	2496	2503	2505	rBV2	510	391	0.05%	0.007%
58	9.220	2538	2544	2546	rBV2	240	310	0.04%	0.005%
59	9.410	2600	2603	2607	rVB	197	157	0.02%	0.003%
60	9.452	2612	2616	2618	rBV	154	157	0.02%	0.003%
61	9.644	2673	2676	2681	rVB2	199	190	0.03%	0.003%
62	9.770	2706	2715	2720	rBV2	178	385	0.05%	0.007%
63	10.037	2793	2798	2800	rBV2	234	233	0.03%	0.004%
64	10.072	2804	2809	2811	rBV2	215	204	0.03%	0.003%
65	10.153	2823	2834	2856	rVV	211083	329893	45.14%	5.643%
66	10.329	2881	2889	2892	rBV3	822	1157	0.16%	0.020%
67	10.403	2906	2912	2915	rBV2	219	287	0.04%	0.005%
68	10.471	2930	2933	2938	rBV	207	246	0.03%	0.004%
69	10.908	3067	3069	3074	rVB	292	196	0.03%	0.003%
70	11.101	3123	3129	3137	rBV5	1231	1866	0.26%	0.032%
71	11.185	3144	3155	3180	rBV	406886	631405	86.40%	10.800%
72	11.519	3255	3259	3260	rBV	254	190	0.03%	0.003%
73	11.561	3260	3272	3297	rVV	349730	556119	76.10%	9.512%
74	11.831	3352	3356	3359	rBV	219	209	0.03%	0.004%
75	11.924	3381	3385	3387	rBV	183	159	0.02%	0.003%
76	12.024	3413	3416	3418	rBV2	212	156	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033937.D
 Acq On : 01 Feb 2024 10:38
 Operator : SY/MD
 Sample : P1309-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.294	3494	3500	3515	rVB5	4899	8019	1.10%	0.137%
78	12.529	3570	3573	3579	rBV	259	240	0.03%	0.004%
79	12.561	3579	3583	3586	rBV	183	191	0.03%	0.003%
80	12.619	3596	3601	3607	rVB2	218	293	0.04%	0.005%
81	12.651	3607	3611	3620	rBV2	266	503	0.07%	0.009%
82	12.734	3634	3637	3641	rBV	228	263	0.04%	0.004%
83	13.011	3720	3723	3726	rBV	302	235	0.03%	0.004%
84	13.082	3742	3745	3750	rBV	190	199	0.03%	0.003%
85	13.165	3768	3771	3775	rVV	189	198	0.03%	0.003%
86	13.207	3779	3784	3792	rVB4	777	880	0.12%	0.015%
87	13.448	3850	3859	3875	rBV2	2951	4854	0.66%	0.083%
88	13.570	3893	3897	3899	rBV2	261	159	0.02%	0.003%
89	13.686	3929	3933	3939	rVB3	585	704	0.10%	0.012%
90	13.773	3956	3960	3964	rBV2	200	204	0.03%	0.003%
91	13.927	4005	4008	4012	rVB3	217	176	0.02%	0.003%
92	13.947	4012	4014	4019	rVB3	289	183	0.03%	0.003%
93	13.985	4019	4026	4038	rBV2	772	1357	0.19%	0.023%
94	14.037	4038	4042	4044	rBV2	186	194	0.03%	0.003%
95	14.120	4066	4068	4074	rVB2	229	228	0.03%	0.004%
96	14.149	4074	4077	4079	rBV2	261	185	0.03%	0.003%
97	14.477	4176	4179	4181	rBV2	232	186	0.03%	0.003%
98	14.744	4260	4262	4268	rVB2	266	209	0.03%	0.004%
99	15.249	4417	4419	4423	rBV2	385	285	0.04%	0.005%
100	15.313	4435	4439	4443	rBV3	363	375	0.05%	0.006%




Sum of corrected areas: 5846360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033937.D
Acq On : 01 Feb 2024 10:38
Operator : SY/MD
Sample : P1309-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

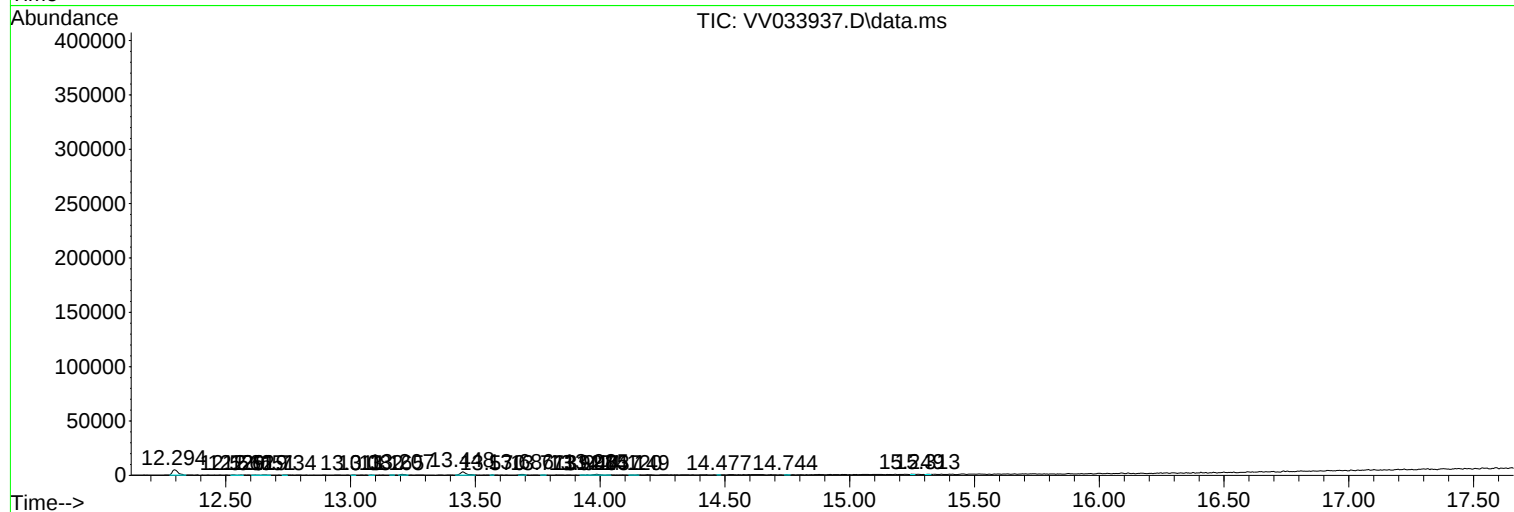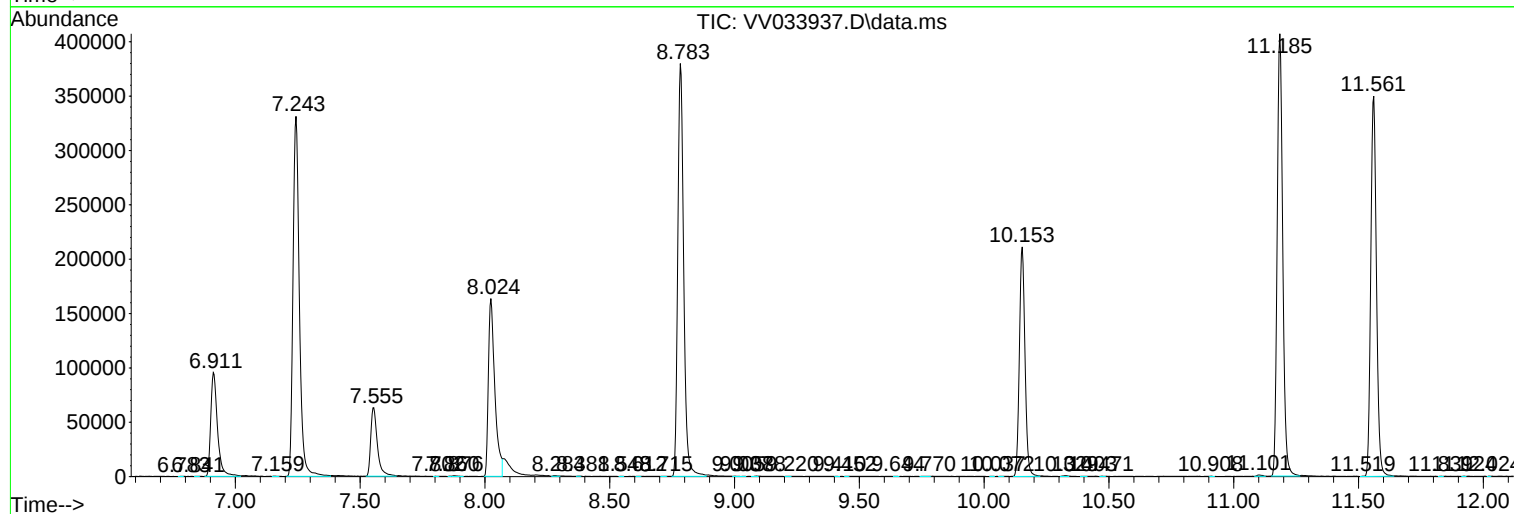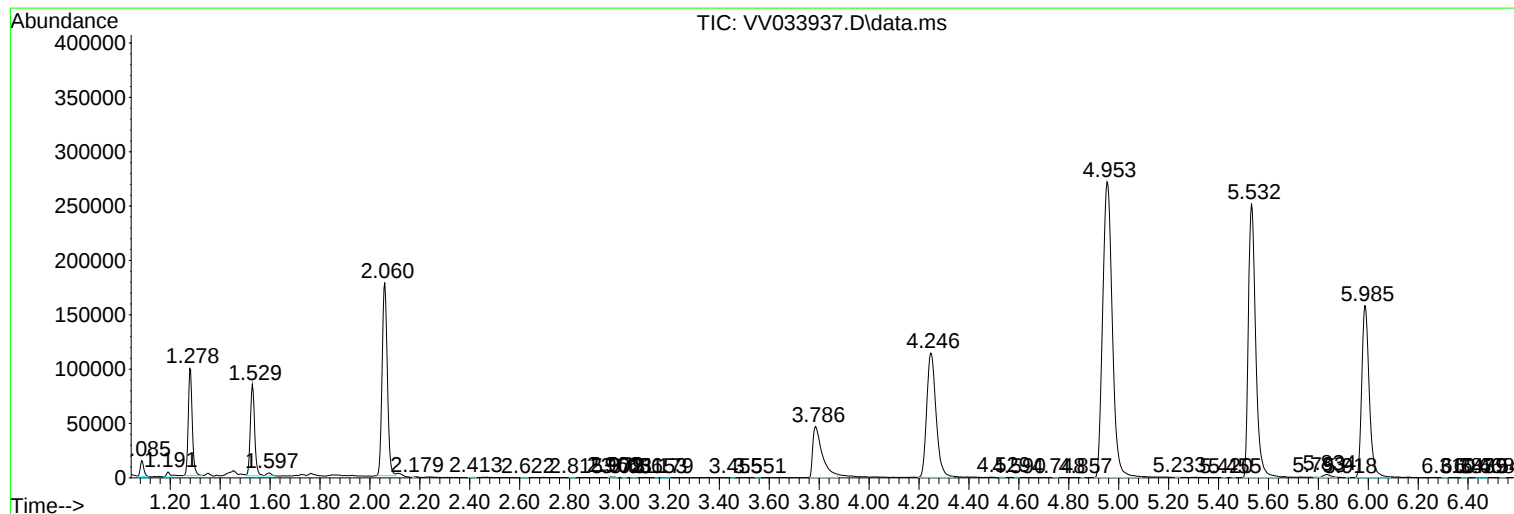

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033937.D
Acq On : 01 Feb 2024 10:38
Operator : SY/MD
Sample : P1309-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033937.D
Acq On : 01 Feb 2024 10:38
Operator : SY/MD
Sample : P1309-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc