

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033938.D
 Acq On : 01 Feb 2024 11:02
 Operator : SY/MD
 Sample : P1309-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH915

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	31	rVB	20992	21544	2.89%	0.364%
2	1.166	32	39	44	rBV	7564	8456	1.13%	0.143%
3	1.192	44	47	52	rVB2	3186	2725	0.37%	0.046%
4	1.282	66	75	86	rBV	103902	117057	15.70%	1.977%
5	1.349	93	96	103	rVB2	2443	2210	0.30%	0.037%
6	1.429	113	121	129	rBV6	4271	5618	0.75%	0.095%
7	1.529	145	152	166	rBV	84493	101848	13.66%	1.720%
8	2.060	306	317	331	rBV	181586	264392	35.47%	4.465%
9	2.220	364	367	370	rBV3	337	246	0.03%	0.004%
10	2.298	389	391	394	rVB	280	169	0.02%	0.003%
11	2.455	435	440	443	rBV2	398	335	0.04%	0.006%
12	2.532	460	464	468	rBV2	140	165	0.02%	0.003%
13	2.609	483	488	491	rVB2	158	163	0.02%	0.003%
14	2.693	510	514	518	rBV3	321	338	0.05%	0.006%
15	2.915	580	583	590	rVB2	241	237	0.03%	0.004%
16	2.957	593	596	598	rVV	208	162	0.02%	0.003%
17	2.976	598	602	606	rVV2	432	471	0.06%	0.008%
18	3.240	679	684	689	rBV2	330	501	0.07%	0.008%
19	3.298	698	702	708	rBV2	187	234	0.03%	0.004%
20	3.333	708	713	716	rBV	194	200	0.03%	0.003%
21	3.564	781	785	789	rVB2	167	168	0.02%	0.003%
22	3.593	789	794	796	rBV2	223	206	0.03%	0.003%
23	3.642	805	809	811	rBV	172	174	0.02%	0.003%
24	3.674	815	819	823	rVB2	202	208	0.03%	0.004%
25	3.699	823	827	830	rBV2	245	273	0.04%	0.005%
26	3.783	845	853	891	rBV	53076	141036	18.92%	2.382%
27	4.027	927	929	932	rBV	410	227	0.03%	0.004%
28	4.249	982	998	1030	rBV	118388	301079	40.39%	5.085%
29	4.494	1071	1074	1076	rBV	245	185	0.02%	0.003%
30	4.561	1093	1095	1099	rVB	473	327	0.04%	0.006%
31	4.590	1099	1104	1106	rBV2	317	277	0.04%	0.005%
32	4.642	1117	1120	1123	rBV2	348	225	0.03%	0.004%
33	4.844	1179	1183	1184	rBV2	232	163	0.02%	0.003%
34	4.957	1202	1218	1248	rBV2	280191	745457	100.00%	12.589%
35	5.240	1303	1306	1308	rBV2	257	193	0.03%	0.003%
36	5.346	1337	1339	1342	rVB2	265	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033938.D
 Acq On : 01 Feb 2024 11:02
 Operator : SY/MD
 Sample : P1309-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH915

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.362	1342	1344	1349	rVB2	394	294	0.04%	0.005%
38	5.388	1349	1352	1355	rBV2	336	297	0.04%	0.005%
39	5.420	1359	1362	1365	rBV	357	284	0.04%	0.005%
40	5.452	1369	1372	1376	rVB3	340	264	0.04%	0.004%
41	5.478	1376	1380	1382	rBV2	276	260	0.03%	0.004%
42	5.532	1386	1397	1427	rBV	245430	499117	66.95%	8.429%
43	5.831	1483	1490	1501	rBV4	2496	4897	0.66%	0.083%
44	5.989	1526	1539	1567	rBV	163286	338966	45.47%	5.724%
45	6.191	1600	1602	1606	rVB2	321	152	0.02%	0.003%
46	6.461	1682	1686	1691	rBV2	224	262	0.04%	0.004%
47	6.686	1752	1756	1759	rBV2	207	218	0.03%	0.004%
48	6.818	1790	1797	1799	rBV	190	241	0.03%	0.004%
49	6.912	1817	1826	1853	rBV	96003	181094	24.29%	3.058%
50	7.243	1918	1929	1962	rBV	331520	589046	79.02%	9.948%
51	7.487	2002	2005	2007	rBV2	458	410	0.05%	0.007%
52	7.551	2016	2025	2056	rBV2	65518	118303	15.87%	1.998%
53	7.748	2082	2086	2094	rBV4	405	530	0.07%	0.009%
54	7.876	2120	2126	2133	rBV2	712	892	0.12%	0.015%
55	8.024	2163	2172	2214	rBV	175586	356761	47.86%	6.025%
56	8.522	2323	2327	2332	rBV2	174	217	0.03%	0.004%
57	8.635	2359	2362	2364	rBV	221	171	0.02%	0.003%
58	8.706	2377	2384	2386	rBV2	221	300	0.04%	0.005%
59	8.783	2397	2408	2437	rBV	366803	600713	80.58%	10.145%
60	8.992	2469	2473	2478	rVB3	199	171	0.02%	0.003%
61	9.165	2525	2527	2532	rBV2	147	149	0.02%	0.003%
62	9.275	2557	2561	2565	rVB2	331	340	0.05%	0.006%
63	9.304	2565	2570	2572	rBV	349	379	0.05%	0.006%
64	9.513	2632	2635	2640	rBV2	204	216	0.03%	0.004%
65	9.683	2684	2688	2691	rBV	205	183	0.02%	0.003%
66	9.728	2699	2702	2708	rBV	175	226	0.03%	0.004%
67	9.976	2775	2779	2783	rVB2	204	215	0.03%	0.004%
68	10.153	2823	2834	2859	rBV	224760	347765	46.65%	5.873%
69	10.262	2866	2868	2872	rBV	218	168	0.02%	0.003%
70	10.326	2879	2888	2897	rBV3	871	1572	0.21%	0.027%
71	10.407	2907	2913	2916	rBV	215	312	0.04%	0.005%
72	10.474	2928	2934	2937	rBV2	175	234	0.03%	0.004%
73	10.532	2946	2952	2956	rBV2	174	206	0.03%	0.003%
74	10.693	2998	3002	3006	rBV2	155	195	0.03%	0.003%
75	10.940	3072	3079	3086	rVB2	257	455	0.06%	0.008%
76	11.059	3114	3116	3120	rBV2	185	164	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033938.D
 Acq On : 01 Feb 2024 11:02
 Operator : SY/MD
 Sample : P1309-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH915

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3183	rVV	378247	593549	79.62%	10.024%
78	11.445	3233	3236	3240	rBV2	218	232	0.03%	0.004%
79	11.561	3260	3272	3301	rBV	347982	554300	74.36%	9.361%
80	11.841	3356	3359	3362	rVB	215	146	0.02%	0.002%
81	11.982	3399	3403	3406	rBV2	203	161	0.02%	0.003%
82	12.297	3495	3501	3512	rBV5	2226	3516	0.47%	0.059%
83	12.419	3536	3539	3543	rBV2	169	160	0.02%	0.003%
84	12.686	3619	3622	3628	rBV2	229	276	0.04%	0.005%
85	13.050	3731	3735	3737	rBV	185	178	0.02%	0.003%
86	13.149	3764	3766	3770	rVB2	248	149	0.02%	0.003%
87	13.175	3770	3774	3778	rVB	262	210	0.03%	0.004%
88	13.210	3782	3785	3788	rBV3	221	149	0.02%	0.003%
89	13.339	3819	3825	3828	rBV2	194	287	0.04%	0.005%
90	13.455	3854	3861	3866	rBV3	1196	1607	0.22%	0.027%
91	13.558	3891	3893	3897	rVB2	232	149	0.02%	0.003%
92	13.657	3920	3924	3926	rBV	289	217	0.03%	0.004%
93	13.693	3931	3935	3937	rBV2	463	386	0.05%	0.007%
94	13.824	3974	3976	3979	rBV2	242	153	0.02%	0.003%
95	13.979	4020	4024	4026	rBV3	423	342	0.05%	0.006%
96	14.252	4104	4109	4112	rBV2	343	368	0.05%	0.006%
97	14.281	4113	4118	4119	rBV	201	164	0.02%	0.003%
98	14.541	4197	4199	4206	rVB3	356	251	0.03%	0.004%
99	14.638	4226	4229	4231	rBV2	300	157	0.02%	0.003%
100	15.130	4380	4382	4386	rBV2	368	216	0.03%	0.004%




Sum of corrected areas: 5921407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033938.D
Acq On : 01 Feb 2024 11:02
Operator : SY/MD
Sample : P1309-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

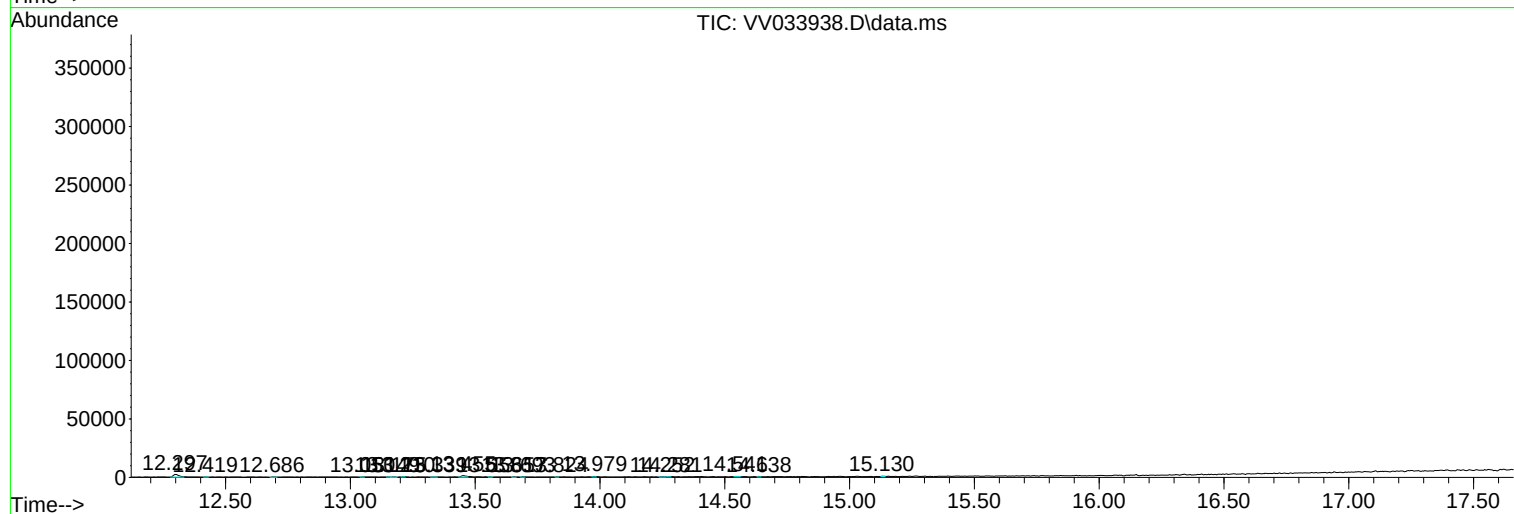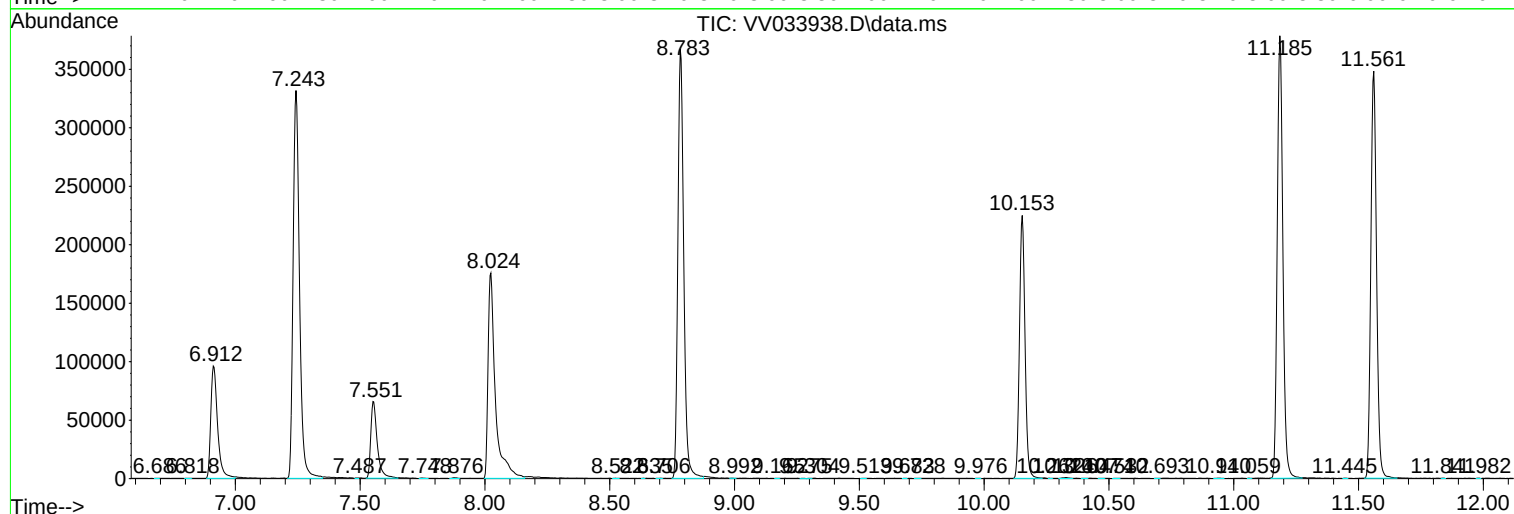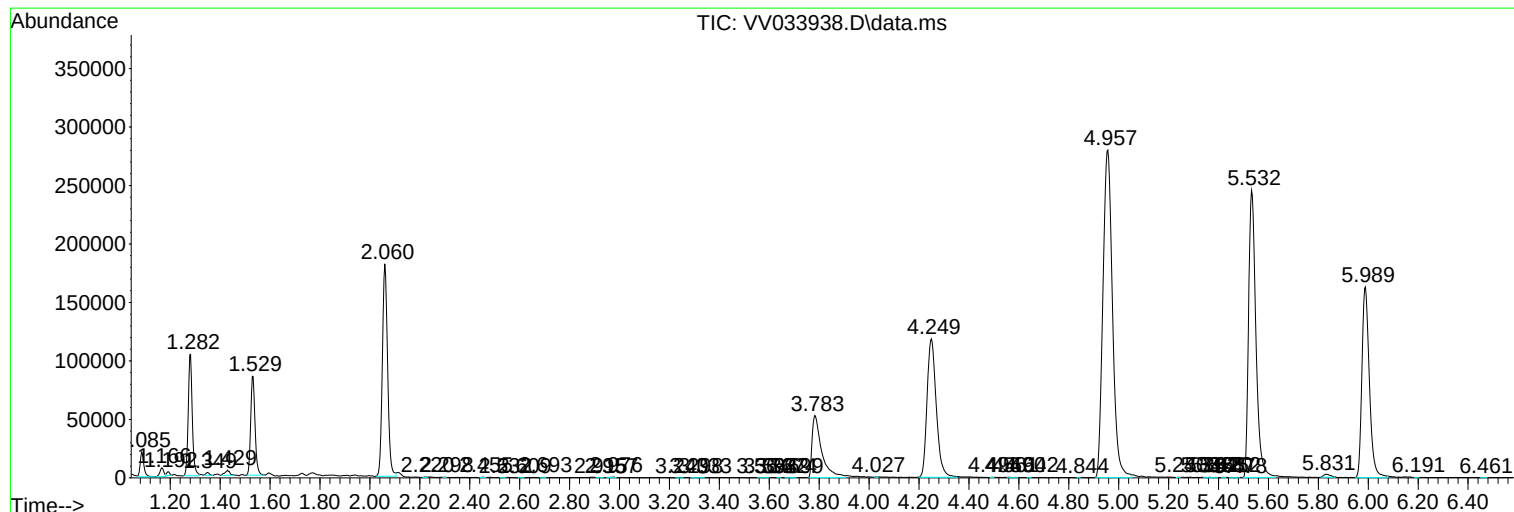

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033938.D
Acq On : 01 Feb 2024 11:02
Operator : SY/MD
Sample : P1309-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033938.D
Acq On : 01 Feb 2024 11:02
Operator : SY/MD
Sample : P1309-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------