

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033939.D
 Acq On : 01 Feb 2024 11:26
 Operator : SY/MD
 Sample : P1309-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	51	rBV	7583	8288	1.16%	0.145%
2	1.282	68	75	90	rBV	92860	100936	14.13%	1.765%
3	1.417	112	117	122	rBV5	6557	8305	1.16%	0.145%
4	1.532	145	153	170	rVB	79182	98837	13.84%	1.728%
5	2.060	307	317	341	rBV	171574	253233	35.45%	4.428%
6	2.237	370	372	376	rBV	448	305	0.04%	0.005%
7	2.507	451	456	458	rBV2	255	280	0.04%	0.005%
8	2.590	479	482	483	rBV	198	113	0.02%	0.002%
9	2.915	580	583	588	rVB	194	197	0.03%	0.003%
10	2.941	588	591	595	rBV2	179	147	0.02%	0.003%
11	2.963	595	598	601	rBV	179	182	0.03%	0.003%
12	3.111	639	644	650	rBV2	213	335	0.05%	0.006%
13	3.259	684	690	695	rBB2	192	262	0.04%	0.005%
14	3.404	733	735	738	rBV2	176	123	0.02%	0.002%
15	3.510	762	768	771	rVB	199	189	0.03%	0.003%
16	3.555	776	782	785	rBV2	275	293	0.04%	0.005%
17	3.619	799	802	805	rBV2	171	122	0.02%	0.002%
18	3.658	810	814	819	rVB2	208	237	0.03%	0.004%
19	3.690	819	824	826	rBV	187	194	0.03%	0.003%
20	3.783	845	853	895	rBV	51158	140419	19.66%	2.456%
21	4.249	983	998	1027	rBV	113417	287419	40.24%	5.026%
22	4.478	1067	1069	1072	rBV	255	148	0.02%	0.003%
23	4.516	1079	1081	1084	rVB3	283	130	0.02%	0.002%
24	4.535	1084	1087	1090	rVB2	286	215	0.03%	0.004%
25	4.577	1097	1100	1101	rBV2	233	150	0.02%	0.003%
26	4.654	1119	1124	1125	rBV	164	127	0.02%	0.002%
27	4.728	1144	1147	1150	rVB	176	145	0.02%	0.003%
28	4.957	1202	1218	1260	rBV2	268862	714347	100.00%	12.492%
29	5.535	1386	1398	1425	rBV	245857	501750	70.24%	8.774%
30	5.834	1482	1491	1502	rBV3	2674	5623	0.79%	0.098%
31	5.989	1527	1539	1568	rBV	154002	321926	45.07%	5.630%
32	6.166	1592	1594	1597	rBV2	288	134	0.02%	0.002%
33	6.220	1608	1611	1614	rVB2	207	141	0.02%	0.002%
34	6.304	1633	1637	1640	rBV	287	251	0.04%	0.004%
35	6.381	1657	1661	1665	rBV2	219	230	0.03%	0.004%
36	6.442	1676	1680	1683	rBV	138	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033939.D
 Acq On : 01 Feb 2024 11:26
 Operator : SY/MD
 Sample : P1309-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.468	1683	1688	1691	rBV2	165	200	0.03%	0.003%
38	6.542	1704	1711	1714	rBV2	148	210	0.03%	0.004%
39	6.625	1735	1737	1739	rBV2	159	109	0.02%	0.002%
40	6.725	1765	1768	1769	rBV	170	112	0.02%	0.002%
41	6.799	1788	1791	1794	rBV	175	163	0.02%	0.003%
42	6.831	1798	1801	1804	rBV2	161	114	0.02%	0.002%
43	6.857	1804	1809	1814	rBV2	235	307	0.04%	0.005%
44	6.915	1817	1827	1849	rBV	91969	170674	23.89%	2.985%
45	7.137	1893	1896	1899	rBV	334	278	0.04%	0.005%
46	7.243	1917	1929	1963	rBV	320789	565676	79.19%	9.892%
47	7.555	2016	2026	2049	rBV	63281	114283	16.00%	1.998%
48	7.876	2120	2126	2127	rBV2	327	319	0.04%	0.006%
49	8.024	2163	2172	2211	rBV	173578	346570	48.52%	6.060%
50	8.477	2311	2313	2316	rBV	148	124	0.02%	0.002%
51	8.658	2365	2369	2370	rBV	172	146	0.02%	0.003%
52	8.783	2397	2408	2443	rBV	370182	609656	85.34%	10.661%
53	9.326	2573	2577	2585	rVV2	173	318	0.04%	0.006%
54	9.484	2623	2626	2628	rBV	166	121	0.02%	0.002%
55	9.497	2628	2630	2634	rVB2	184	126	0.02%	0.002%
56	9.542	2641	2644	2645	rBV2	202	116	0.02%	0.002%
57	9.661	2677	2681	2689	rBV	137	241	0.03%	0.004%
58	9.699	2689	2693	2695	rBV2	164	152	0.02%	0.003%
59	9.754	2707	2710	2715	rBV2	185	187	0.03%	0.003%
60	9.783	2715	2719	2720	rBV	137	119	0.02%	0.002%
61	9.818	2728	2730	2733	rBV	148	128	0.02%	0.002%
62	9.841	2735	2737	2740	rBV	162	113	0.02%	0.002%
63	9.982	2777	2781	2783	rBV	221	186	0.03%	0.003%
64	10.098	2813	2817	2820	rBV2	173	192	0.03%	0.003%
65	10.153	2823	2834	2858	rVV	210178	333043	46.62%	5.824%
66	10.323	2884	2887	2888	rBV	251	166	0.02%	0.003%
67	10.365	2897	2900	2903	rBV	203	157	0.02%	0.003%
68	10.445	2921	2925	2927	rBV	207	152	0.02%	0.003%
69	10.487	2934	2938	2942	rBV2	216	243	0.03%	0.004%
70	10.510	2942	2945	2950	rBV2	164	183	0.03%	0.003%
71	10.538	2950	2954	2958	rBV2	184	202	0.03%	0.004%
72	10.587	2965	2969	2972	rBV2	171	159	0.02%	0.003%
73	10.789	3029	3032	3035	rBV	196	156	0.02%	0.003%
74	10.844	3045	3049	3052	rBV2	160	131	0.02%	0.002%
75	10.873	3055	3058	3061	rBV	186	147	0.02%	0.003%
76	11.185	3144	3155	3180	rBV	389024	596303	83.48%	10.428%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033939.D
 Acq On : 01 Feb 2024 11:26
 Operator : SY/MD
 Sample : P1309-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.423	3227	3229	3232	rBV2	185	112	0.02%	0.002%
78	11.487	3243	3249	3252	rBV2	235	247	0.03%	0.004%
79	11.503	3252	3254	3257	rBV	211	161	0.02%	0.003%
80	11.561	3260	3272	3292	rBV	325148	525572	73.57%	9.191%
81	11.760	3330	3334	3337	rBV2	333	272	0.04%	0.005%
82	11.915	3380	3382	3386	rBV2	181	190	0.03%	0.003%
83	11.982	3397	3403	3406	rBV2	241	261	0.04%	0.005%
84	12.001	3406	3409	3412	rVB2	258	176	0.02%	0.003%
85	12.262	3484	3490	3496	rBV2	204	392	0.05%	0.007%
86	12.448	3544	3548	3552	rBV2	222	255	0.04%	0.004%
87	12.596	3590	3594	3597	rBV2	197	220	0.03%	0.004%
88	12.651	3609	3611	3616	rBV2	160	144	0.02%	0.003%
89	12.751	3637	3642	3648	rBV3	694	710	0.10%	0.012%
90	12.866	3675	3678	3681	rBV2	188	141	0.02%	0.002%
91	12.960	3701	3707	3709	rBV2	205	248	0.03%	0.004%
92	12.985	3713	3715	3718	rVB	200	135	0.02%	0.002%
93	13.156	3764	3768	3769	rBV	232	189	0.03%	0.003%
94	13.294	3807	3811	3816	rBV2	237	288	0.04%	0.005%
95	13.400	3840	3844	3846	rBV2	246	176	0.02%	0.003%
96	13.416	3846	3849	3851	rBV2	247	151	0.02%	0.003%
97	13.516	3876	3880	3883	rBV2	195	153	0.02%	0.003%
98	13.686	3930	3933	3936	rBV	293	124	0.02%	0.002%
99	13.747	3950	3952	3955	rBV2	278	166	0.02%	0.003%
100	13.850	3980	3984	3986	rBV2	278	204	0.03%	0.004%




Sum of corrected areas: 5718539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033939.D
Acq On : 01 Feb 2024 11:26
Operator : SY/MD
Sample : P1309-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

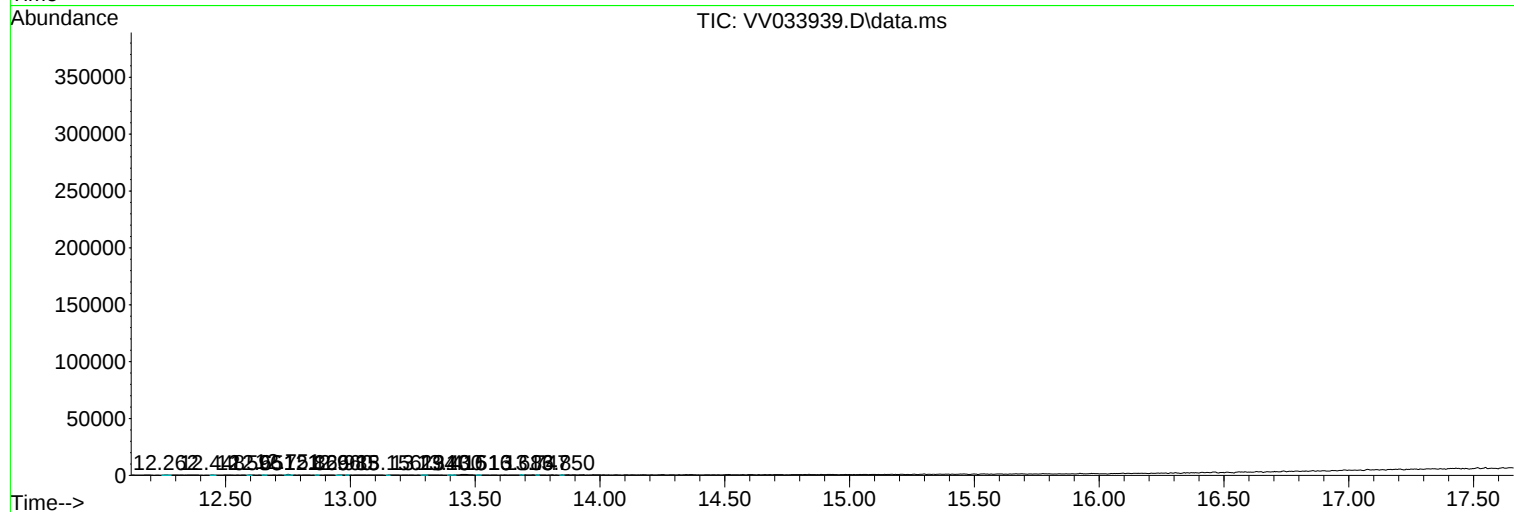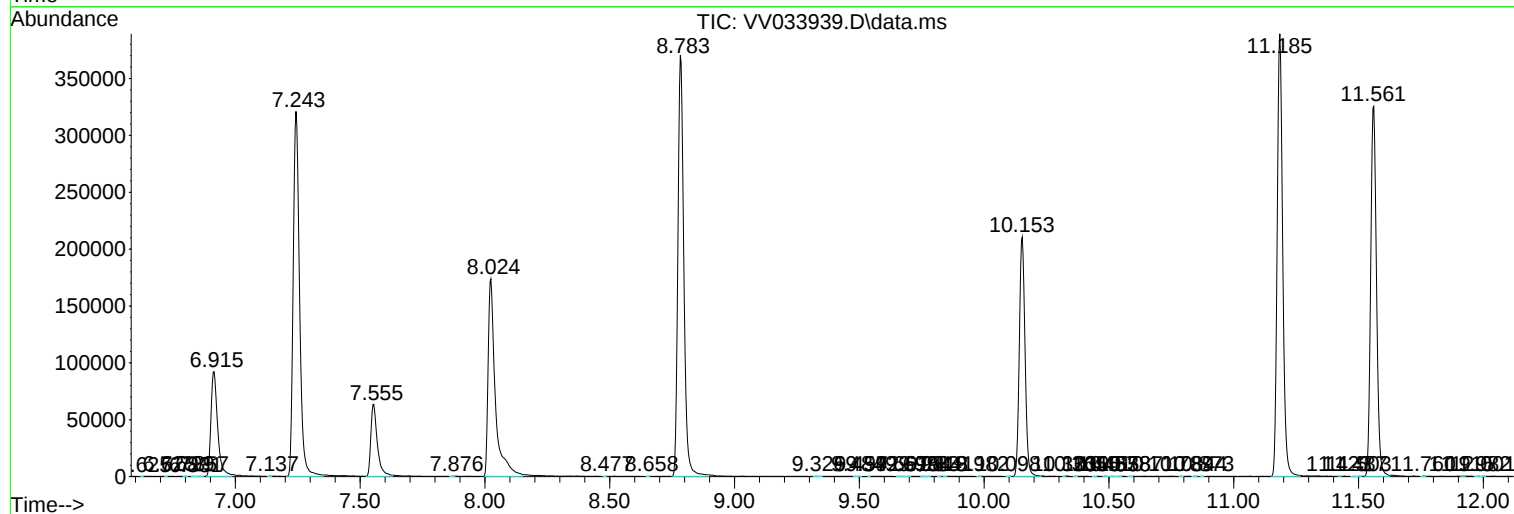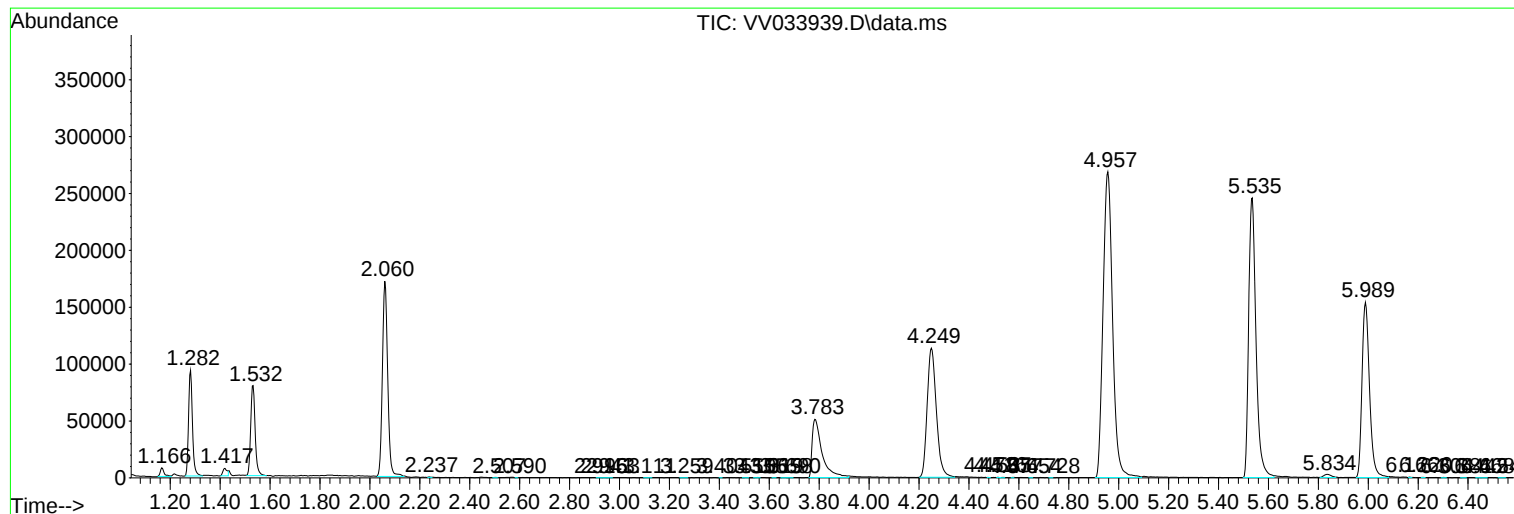

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033939.D
Acq On : 01 Feb 2024 11:26
Operator : SY/MD
Sample : P1309-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033939.D
Acq On : 01 Feb 2024 11:26
Operator : SY/MD
Sample : P1309-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc