

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033942.D
 Acq On : 01 Feb 2024 12:38
 Operator : SY/MD
 Sample : P1310-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	24	rVB	10755	10799	1.57%	0.191%
2	1.166	31	39	43	rBV2	6300	7826	1.14%	0.138%
3	1.278	66	74	87	rBV	90375	100600	14.62%	1.775%
4	1.529	144	152	166	rBV	78252	94346	13.71%	1.665%
5	2.060	307	317	330	rBV	163084	237980	34.58%	4.199%
6	2.230	367	370	372	rBV	283	233	0.03%	0.004%
7	2.298	385	391	395	rBV3	823	1046	0.15%	0.018%
8	2.375	410	415	418	rBV2	225	278	0.04%	0.005%
9	2.429	427	432	433	rBV2	140	142	0.02%	0.003%
10	2.445	433	437	441	rVB	378	325	0.05%	0.006%
11	2.568	470	475	479	rVB2	275	285	0.04%	0.005%
12	2.600	479	485	488	rBV2	198	265	0.04%	0.005%
13	2.690	510	513	516	rBV3	360	202	0.03%	0.004%
14	2.963	594	598	601	rBV2	257	247	0.04%	0.004%
15	3.114	642	645	653	rVB2	249	344	0.05%	0.006%
16	3.159	654	659	660	rBV2	224	189	0.03%	0.003%
17	3.233	672	682	686	rBV2	297	442	0.06%	0.008%
18	3.269	689	693	696	rVB2	184	164	0.02%	0.003%
19	3.365	720	723	726	rBV2	219	174	0.03%	0.003%
20	3.416	735	739	742	rBV2	272	307	0.04%	0.005%
21	3.494	757	763	765	rBV	141	165	0.02%	0.003%
22	3.539	773	777	780	rBV	274	270	0.04%	0.005%
23	3.616	797	801	802	rBV2	256	193	0.03%	0.003%
24	3.664	812	816	819	rBV2	171	156	0.02%	0.003%
25	3.732	833	837	845	rVB2	180	272	0.04%	0.005%
26	3.783	845	853	888	rBV2	51608	136373	19.81%	2.406%
27	4.249	982	998	1040	rBV	109377	278361	40.44%	4.912%
28	4.397	1040	1044	1046	rBV3	232	182	0.03%	0.003%
29	4.487	1067	1072	1076	rBV2	364	342	0.05%	0.006%
30	4.638	1115	1119	1123	rBV2	205	173	0.03%	0.003%
31	4.764	1155	1158	1162	rBV	142	144	0.02%	0.003%
32	4.957	1202	1218	1249	rBV2	258450	688288	100.00%	12.146%
33	5.532	1385	1397	1428	rBV	253861	515883	74.95%	9.103%
34	5.712	1449	1453	1457	rBV3	314	312	0.05%	0.006%
35	5.789	1474	1477	1481	rVB2	218	164	0.02%	0.003%
36	5.834	1483	1491	1503	rVB4	2019	4076	0.59%	0.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020124\
 Data File : VW033942.D
 Acq On : 01 Feb 2024 12:38
 Operator : SY/MD
 Sample : P1310-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1567	rBV	151074	311542	45.26%	5.498%
38	6.146	1585	1588	1591	rVB3	613	452	0.07%	0.008%
39	6.169	1593	1595	1598	rVB2	486	156	0.02%	0.003%
40	6.442	1676	1680	1682	rBV	198	192	0.03%	0.003%
41	6.500	1694	1698	1702	rBV2	125	144	0.02%	0.003%
42	6.616	1730	1734	1736	rBV	193	159	0.02%	0.003%
43	6.757	1775	1778	1781	rVB2	188	163	0.02%	0.003%
44	6.780	1781	1785	1792	rBV2	191	282	0.04%	0.005%
45	6.815	1794	1796	1803	rVB2	265	285	0.04%	0.005%
46	6.857	1803	1809	1810	rBV	161	181	0.03%	0.003%
47	6.915	1817	1827	1846	rBV	89611	165203	24.00%	2.915%
48	7.153	1899	1901	1904	rBV2	265	180	0.03%	0.003%
49	7.175	1906	1908	1911	rVB	265	148	0.02%	0.003%
50	7.243	1917	1929	1958	rBV	310333	545369	79.24%	9.624%
51	7.506	2009	2011	2016	rBV2	470	505	0.07%	0.009%
52	7.555	2016	2026	2057	rVV	60348	110783	16.10%	1.955%
53	7.776	2090	2095	2098	rBV	187	243	0.04%	0.004%
54	7.860	2118	2121	2122	rBV	279	179	0.03%	0.003%
55	7.947	2144	2148	2150	rBV	285	290	0.04%	0.005%
56	8.024	2163	2172	2216	rBV	173559	342996	49.83%	6.053%
57	8.452	2302	2305	2311	rBV2	220	321	0.05%	0.006%
58	8.506	2319	2322	2328	rBV2	168	242	0.04%	0.004%
59	8.712	2381	2386	2389	rBV	173	204	0.03%	0.004%
60	8.783	2397	2408	2444	rBV	379041	627091	91.11%	11.066%
61	8.969	2462	2466	2469	rBV3	380	400	0.06%	0.007%
62	9.635	2670	2673	2676	rBV2	173	163	0.02%	0.003%
63	9.882	2747	2750	2754	rBV	181	201	0.03%	0.004%
64	10.152	2823	2834	2856	rVB	210023	328094	47.67%	5.790%
65	10.320	2881	2886	2888	rBV2	319	292	0.04%	0.005%
66	10.686	2996	3000	3004	rBV	240	220	0.03%	0.004%
67	10.712	3004	3008	3012	rVB2	146	158	0.02%	0.003%
68	10.741	3012	3017	3020	rBV2	149	187	0.03%	0.003%
69	10.879	3057	3060	3062	rBV	195	162	0.02%	0.003%
70	10.953	3080	3083	3089	rVB2	204	196	0.03%	0.003%
71	10.998	3092	3097	3103	rBV2	206	322	0.05%	0.006%
72	11.101	3124	3129	3135	rBV5	1784	2365	0.34%	0.042%
73	11.185	3144	3155	3179	rBV	394473	618713	89.89%	10.918%
74	11.403	3221	3223	3225	rBV	287	160	0.02%	0.003%
75	11.471	3234	3244	3245	rBV2	196	291	0.04%	0.005%
76	11.516	3254	3258	3260	rBV2	221	201	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033942.D
 Acq On : 01 Feb 2024 12:38
 Operator : SY/MD
 Sample : P1310-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.561	3260	3272	3297	rVV	326726	510764	74.21%	9.013%
78	11.693	3311	3313	3318	rVB2	269	164	0.02%	0.003%
79	11.876	3364	3370	3372	rBV2	199	245	0.04%	0.004%
80	12.294	3493	3500	3515	rVB4	5397	9476	1.38%	0.167%
81	12.493	3558	3562	3564	rBV	226	202	0.03%	0.004%
82	12.709	3620	3629	3632	rBV	258	402	0.06%	0.007%
83	12.747	3637	3641	3642	rBV2	539	332	0.05%	0.006%
84	12.934	3696	3699	3704	rBV2	193	263	0.04%	0.005%
85	12.979	3708	3713	3716	rVB2	242	247	0.04%	0.004%
86	13.011	3717	3723	3726	rBV2	174	229	0.03%	0.004%
87	13.075	3740	3743	3749	rVB2	211	266	0.04%	0.005%
88	13.297	3809	3812	3814	rBV2	199	163	0.02%	0.003%
89	13.336	3821	3824	3829	rVB2	201	171	0.02%	0.003%
90	13.969	4017	4021	4023	rBV2	473	428	0.06%	0.008%
91	14.027	4035	4039	4041	rBV2	242	226	0.03%	0.004%
92	14.133	4069	4072	4077	rBV	289	299	0.04%	0.005%
93	14.168	4080	4083	4089	rBV3	305	234	0.03%	0.004%
94	14.207	4093	4095	4098	rBV2	338	251	0.04%	0.004%
95	14.358	4140	4142	4145	rBV2	342	286	0.04%	0.005%
96	14.657	4233	4235	4239	rBV2	192	165	0.02%	0.003%
97	15.172	4393	4395	4397	rBV	295	205	0.03%	0.004%
98	15.249	4417	4419	4421	rBV2	265	146	0.02%	0.003%
99	15.384	4456	4461	4465	rBV3	344	404	0.06%	0.007%
100	15.461	4481	4485	4488	rBV4	516	382	0.06%	0.007%




Sum of corrected areas: 5666933

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033942.D
Acq On : 01 Feb 2024 12:38
Operator : SY/MD
Sample : P1310-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

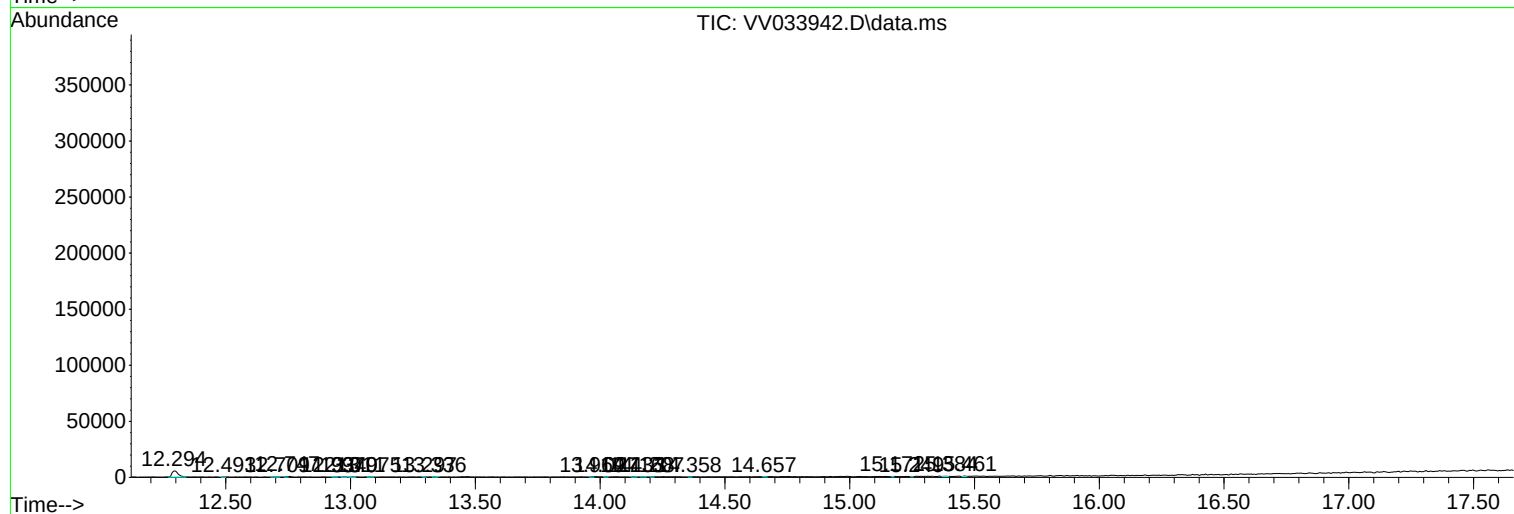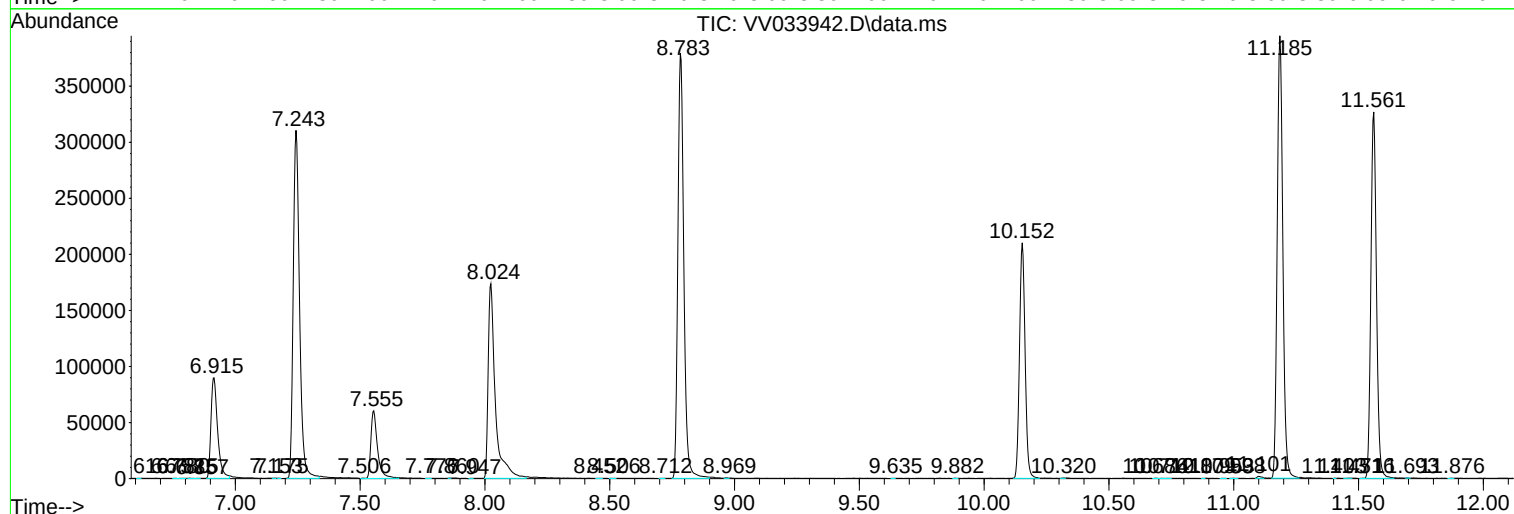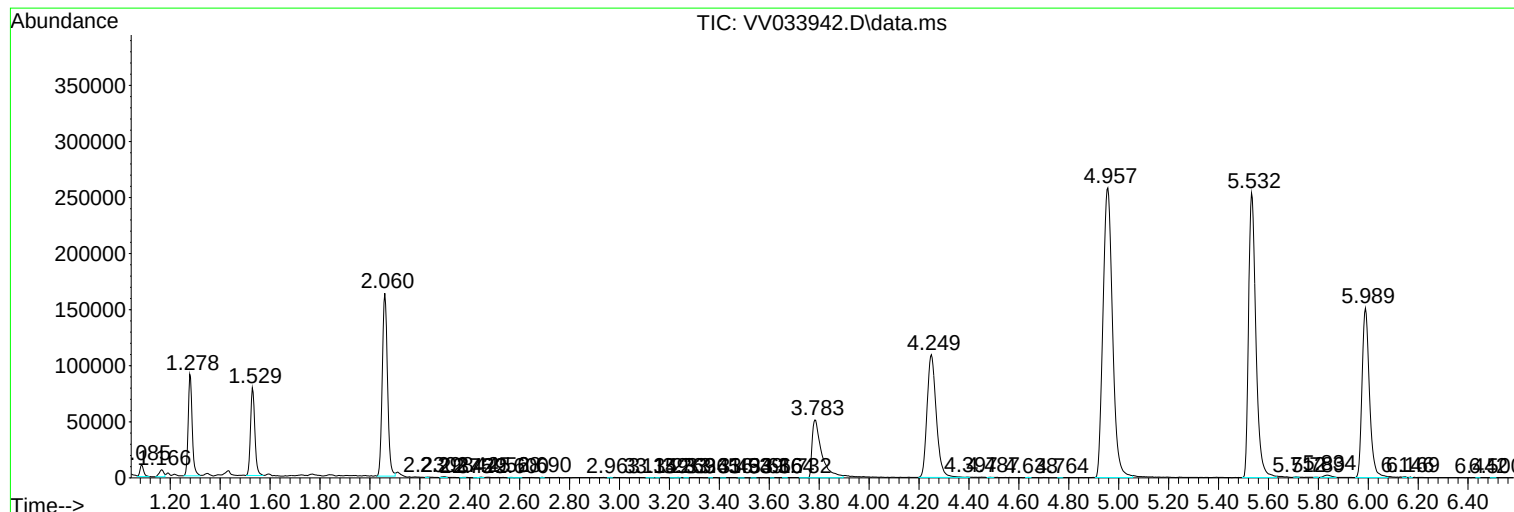

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033942.D
Acq On : 01 Feb 2024 12:38
Operator : SY/MD
Sample : P1310-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033942.D
Acq On : 01 Feb 2024 12:38
Operator : SY/MD
Sample : P1310-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8Z8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc