

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033944.D
 Acq On : 01 Feb 2024 13:26
 Operator : SY/MD
 Sample : P1310-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH900

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	30	rVB	15196	15310	2.25%	0.276%
2	1.166	32	39	44	rBV	6692	7898	1.16%	0.142%
3	1.217	52	55	66	rVB3	1475	1679	0.25%	0.030%
4	1.281	66	75	87	rBV	93983	104177	15.33%	1.880%
5	1.436	113	123	127	rVB7	3678	5574	0.82%	0.101%
6	1.529	145	152	167	rVB	76197	92327	13.59%	1.666%
7	2.060	307	317	332	rBV	162356	237924	35.01%	4.293%
8	2.577	474	478	480	rBV	175	181	0.03%	0.003%
9	2.625	488	493	498	rBV	199	239	0.04%	0.004%
10	2.696	513	515	519	rBV	264	186	0.03%	0.003%
11	2.838	555	559	561	rBV	205	191	0.03%	0.003%
12	2.963	594	598	601	rBV2	239	208	0.03%	0.004%
13	3.031	617	619	625	rBV	118	145	0.02%	0.003%
14	3.079	632	634	639	rVB	185	149	0.02%	0.003%
15	3.114	640	645	649	rBV2	206	281	0.04%	0.005%
16	3.146	651	655	658	rVV	140	138	0.02%	0.002%
17	3.182	664	666	671	rVB	186	162	0.02%	0.003%
18	3.214	671	676	677	rBV	154	143	0.02%	0.003%
19	3.256	686	689	691	rBV2	196	159	0.02%	0.003%
20	3.320	704	709	711	rBV	199	210	0.03%	0.004%
21	3.452	744	750	753	rVV2	243	320	0.05%	0.006%
22	3.629	802	805	809	rVB2	200	134	0.02%	0.002%
23	3.658	810	814	820	rBV2	206	226	0.03%	0.004%
24	3.712	827	831	836	rVB2	211	183	0.03%	0.003%
25	3.783	845	853	898	rBV	51781	139287	20.50%	2.513%
26	4.249	983	998	1032	rBV	107852	278185	40.93%	5.019%
27	4.474	1063	1068	1072	rBV4	433	565	0.08%	0.010%
28	4.539	1084	1088	1089	rBV2	286	188	0.03%	0.003%
29	4.580	1098	1101	1104	rBV	255	233	0.03%	0.004%
30	4.645	1118	1121	1123	rBV	176	145	0.02%	0.003%
31	4.744	1147	1152	1155	rBV	177	205	0.03%	0.004%
32	4.957	1201	1218	1254	rBV2	255559	679582	100.00%	12.261%
33	5.191	1289	1291	1295	rVB2	242	198	0.03%	0.004%
34	5.214	1296	1298	1300	rBV2	343	171	0.03%	0.003%
35	5.413	1356	1360	1363	rVB2	268	206	0.03%	0.004%
36	5.532	1386	1397	1434	rBV	242979	498754	73.39%	8.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033944.D
 Acq On : 01 Feb 2024 13:26
 Operator : SY/MD
 Sample : P1310-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH900

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.838	1483	1492	1506	rVB7	2119	4677	0.69%	0.084%
38	5.989	1526	1539	1567	rBV	148588	306315	45.07%	5.527%
39	6.140	1584	1586	1592	rVB2	486	339	0.05%	0.006%
40	6.169	1592	1595	1598	rBV3	326	216	0.03%	0.004%
41	6.419	1669	1673	1677	rBV2	190	230	0.03%	0.004%
42	6.915	1817	1827	1848	rBV	87588	162598	23.93%	2.934%
43	7.091	1879	1882	1885	rBV2	274	187	0.03%	0.003%
44	7.140	1895	1897	1899	rVB	273	130	0.02%	0.002%
45	7.153	1899	1901	1903	rBV2	301	210	0.03%	0.004%
46	7.185	1908	1911	1917	rBV3	147	137	0.02%	0.002%
47	7.243	1918	1929	1964	rBV	301225	534070	78.59%	9.636%
48	7.554	2016	2026	2050	rBV	59729	107979	15.89%	1.948%
49	7.783	2095	2097	2101	rVB2	327	190	0.03%	0.003%
50	7.879	2121	2127	2129	rBV2	237	272	0.04%	0.005%
51	7.989	2159	2161	2163	rBV2	274	195	0.03%	0.004%
52	8.024	2163	2172	2213	rBV	169654	340850	50.16%	6.150%
53	8.490	2315	2317	2321	rBV	281	189	0.03%	0.003%
54	8.603	2348	2352	2355	rVB2	205	159	0.02%	0.003%
55	8.622	2355	2358	2362	rVB2	182	134	0.02%	0.002%
56	8.654	2362	2368	2377	rVB2	267	522	0.08%	0.009%
57	8.693	2377	2380	2383	rBV2	199	171	0.03%	0.003%
58	8.715	2383	2387	2389	rBV	155	152	0.02%	0.003%
59	8.738	2391	2394	2398	rBV2	138	139	0.02%	0.003%
60	8.783	2398	2408	2434	rBV	361830	595675	87.65%	10.747%
61	9.194	2532	2536	2540	rBV	202	229	0.03%	0.004%
62	9.291	2563	2566	2571	rBV2	277	245	0.04%	0.004%
63	9.693	2686	2691	2692	rBV2	186	183	0.03%	0.003%
64	9.892	2749	2753	2760	rBV	268	377	0.06%	0.007%
65	9.943	2765	2769	2772	rBV2	243	248	0.04%	0.004%
66	10.005	2785	2788	2791	rBV	218	191	0.03%	0.003%
67	10.152	2822	2834	2854	rBV	207172	324875	47.81%	5.861%
68	10.378	2899	2904	2907	rBV2	263	308	0.05%	0.006%
69	10.500	2939	2942	2944	rBV	173	153	0.02%	0.003%
70	10.660	2990	2992	2995	rBV2	170	130	0.02%	0.002%
71	10.792	3028	3033	3037	rVB	239	254	0.04%	0.005%
72	10.866	3051	3056	3058	rBV	333	278	0.04%	0.005%
73	10.914	3068	3071	3074	rBV2	175	161	0.02%	0.003%
74	11.104	3127	3130	3131	rBV	423	169	0.02%	0.003%
75	11.185	3144	3155	3182	rBV	385394	585324	86.13%	10.560%
76	11.345	3202	3205	3207	rBV2	330	212	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033944.D
 Acq On : 01 Feb 2024 13:26
 Operator : SY/MD
 Sample : P1310-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH900

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.455	3236	3239	3243	rBV	210	195	0.03%	0.004%
78	11.561	3260	3272	3293	rBV	314645	497831	73.26%	8.982%
79	11.689	3310	3312	3317	rVB3	400	279	0.04%	0.005%
80	11.728	3321	3324	3326	rVB2	230	131	0.02%	0.002%
81	12.181	3462	3465	3468	rBV	235	218	0.03%	0.004%
82	12.236	3479	3482	3485	rBV2	243	214	0.03%	0.004%
83	12.297	3494	3501	3511	rBV5	3226	4464	0.66%	0.081%
84	12.503	3560	3565	3568	rBV2	216	281	0.04%	0.005%
85	13.545	3886	3889	3892	rVB2	232	180	0.03%	0.003%
86	13.654	3917	3923	3928	rBV	274	407	0.06%	0.007%
87	13.721	3940	3944	3947	rBV	180	184	0.03%	0.003%
88	13.818	3970	3974	3977	rBV2	219	190	0.03%	0.003%
89	13.853	3981	3985	3989	rBV2	264	298	0.04%	0.005%
90	13.963	4015	4019	4021	rBV2	341	242	0.04%	0.004%
91	14.123	4066	4069	4070	rBV	340	173	0.03%	0.003%
92	14.149	4075	4077	4081	rVB2	323	237	0.03%	0.004%
93	14.229	4099	4102	4105	rBV2	339	258	0.04%	0.005%
94	14.352	4137	4140	4143	rBV	249	182	0.03%	0.003%
95	14.387	4147	4151	4156	rBV2	338	286	0.04%	0.005%
96	14.541	4196	4199	4205	rBB3	284	246	0.04%	0.004%
97	14.741	4258	4261	4263	rBV2	302	212	0.03%	0.004%
98	14.889	4304	4307	4312	rVB3	356	353	0.05%	0.006%
99	15.101	4370	4373	4375	rBV2	422	304	0.04%	0.005%
100	15.281	4426	4429	4432	rVB2	508	296	0.04%	0.005%




Sum of corrected areas: 5542597

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033944.D
Acq On : 01 Feb 2024 13:26
Operator : SY/MD
Sample : P1310-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH900

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

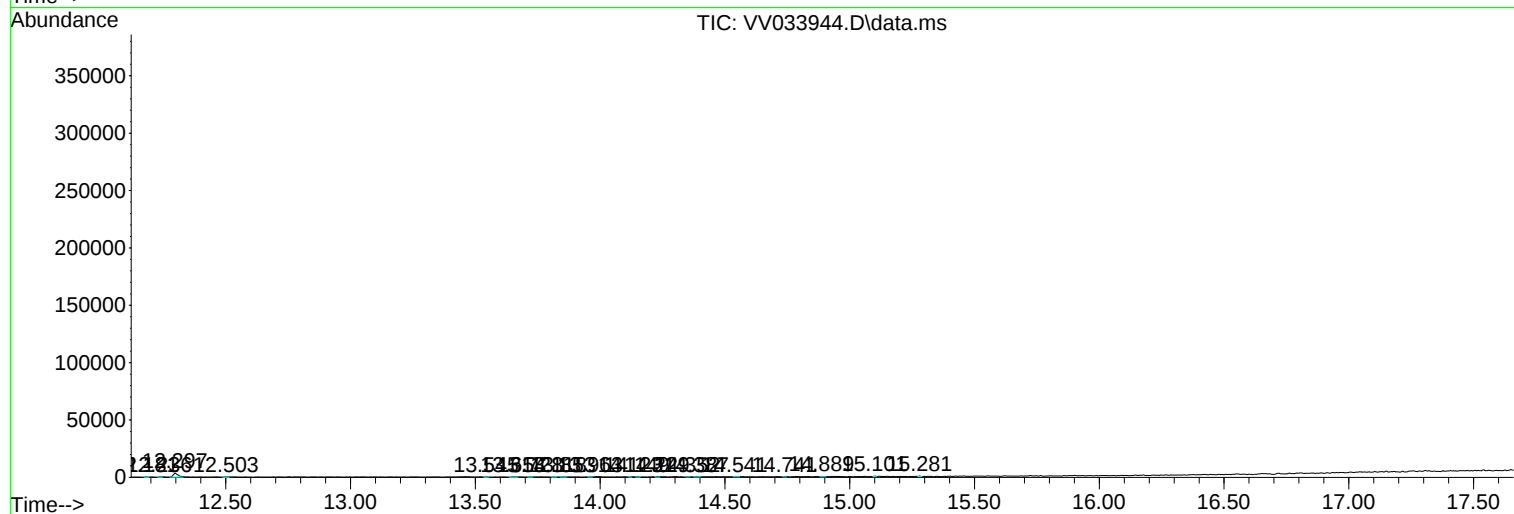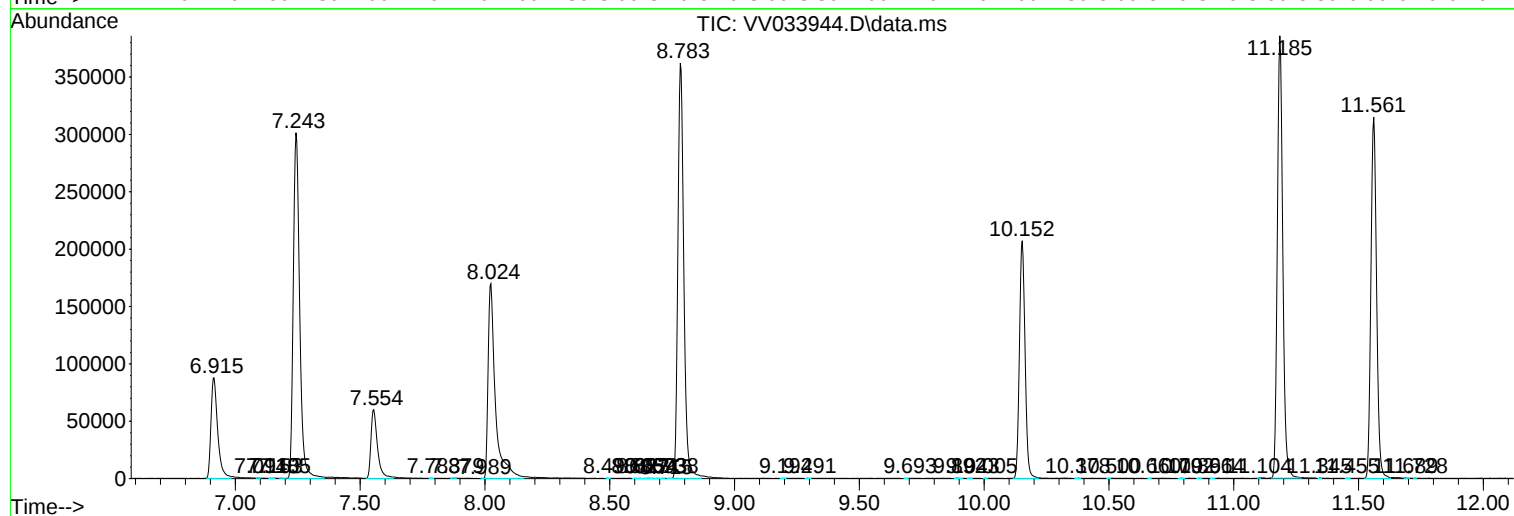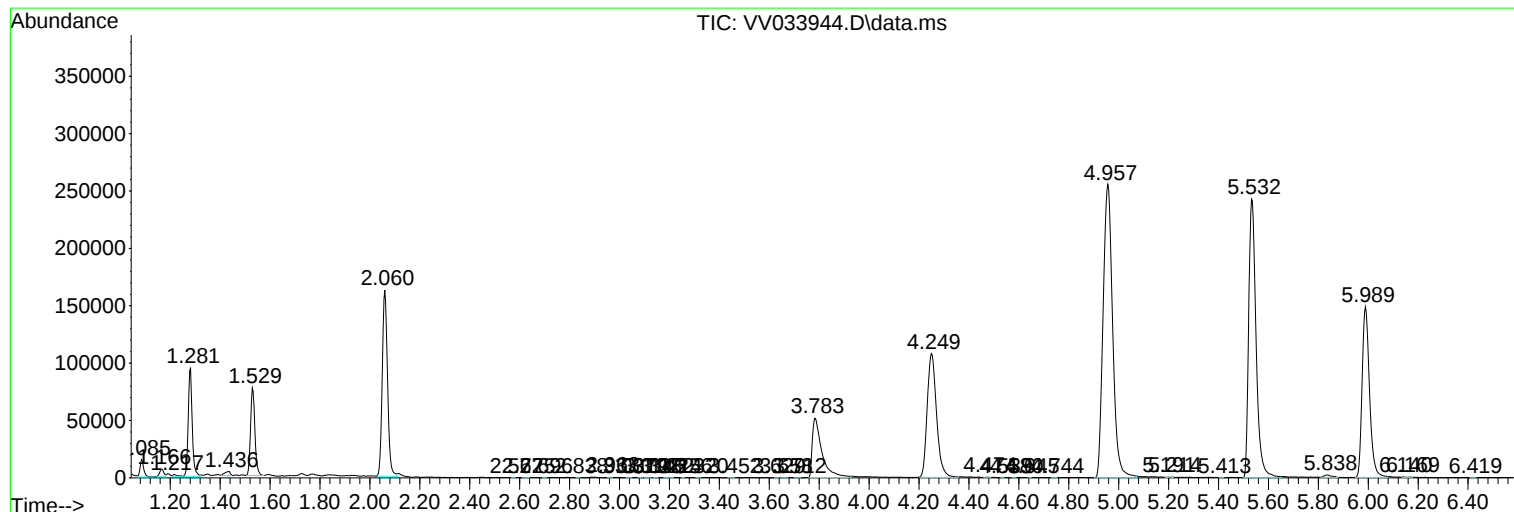

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033944.D
Acq On : 01 Feb 2024 13:26
Operator : SY/MD
Sample : P1310-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH900

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033944.D
Acq On : 01 Feb 2024 13:26
Operator : SY/MD
Sample : P1310-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH900

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc