

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033948.D
 Acq On : 01 Feb 2024 15:02
 Operator : SY/MD
 Sample : P1310-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH917

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	6185	7588	1.15%	0.140%
2	1.278	68	74	88	rBV	82644	89050	13.48%	1.641%
3	1.416	112	117	120	rBV2	4788	5066	0.77%	0.093%
4	1.529	145	152	166	rVB	74864	90171	13.65%	1.661%
5	2.059	306	317	331	rBV	157371	230624	34.91%	4.249%
6	2.182	353	355	361	rVB2	353	338	0.05%	0.006%
7	2.294	385	390	396	rBV2	175	280	0.04%	0.005%
8	2.352	402	408	413	rVB2	229	318	0.05%	0.006%
9	2.391	413	420	424	rBV2	240	360	0.05%	0.007%
10	2.442	433	436	443	rVB2	361	454	0.07%	0.008%
11	2.474	443	446	450	rBV	175	194	0.03%	0.004%
12	2.555	466	471	472	rBV2	473	393	0.06%	0.007%
13	2.699	508	516	522	rBV2	216	458	0.07%	0.008%
14	2.934	584	589	592	rBV	196	221	0.03%	0.004%
15	2.992	602	607	610	rBV	158	182	0.03%	0.003%
16	3.027	614	618	620	rVB	220	178	0.03%	0.003%
17	3.047	620	624	627	rBV2	249	182	0.03%	0.003%
18	3.172	656	663	664	rBV	193	174	0.03%	0.003%
19	3.185	664	667	669	rVV2	217	172	0.03%	0.003%
20	3.339	709	715	718	rBV2	168	159	0.02%	0.003%
21	3.400	731	734	736	rBV2	193	155	0.02%	0.003%
22	3.455	748	751	755	rBV2	171	178	0.03%	0.003%
23	3.481	755	759	763	rVB2	218	182	0.03%	0.003%
24	3.696	823	826	828	rVV2	227	154	0.02%	0.003%
25	3.728	833	836	839	rVB	201	178	0.03%	0.003%
26	3.783	845	853	892	rBV	49723	134831	20.41%	2.484%
27	4.249	982	998	1028	rBV	106500	271086	41.03%	4.995%
28	4.387	1038	1041	1044	rBV2	224	201	0.03%	0.004%
29	4.641	1115	1120	1124	rVB2	214	247	0.04%	0.005%
30	4.674	1124	1130	1131	rBV2	209	240	0.04%	0.004%
31	4.767	1157	1159	1165	rVB	236	237	0.04%	0.004%
32	4.796	1165	1168	1173	rBV	148	169	0.03%	0.003%
33	4.956	1202	1218	1246	rBV2	249147	660700	100.00%	12.174%
34	5.329	1331	1334	1337	rVB2	262	170	0.03%	0.003%
35	5.407	1356	1358	1362	rVB2	365	210	0.03%	0.004%
36	5.429	1362	1365	1369	rBV2	157	158	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033948.D
 Acq On : 01 Feb 2024 15:02
 Operator : SY/MD
 Sample : P1310-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH917

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1427	rBV	237618	488428	73.93%	9.000%
38	5.831	1484	1490	1505	rVB4	2383	5304	0.80%	0.098%
39	5.989	1525	1539	1563	rBV2	147281	303946	46.00%	5.601%
40	6.162	1591	1593	1600	rVB3	512	417	0.06%	0.008%
41	6.313	1635	1640	1643	rBV	295	333	0.05%	0.006%
42	6.329	1643	1645	1650	rVB	242	229	0.03%	0.004%
43	6.471	1682	1689	1691	rBV2	233	294	0.04%	0.005%
44	6.632	1736	1739	1744	rVB3	249	214	0.03%	0.004%
45	6.722	1763	1767	1769	rBV	182	169	0.03%	0.003%
46	6.815	1793	1796	1799	rBV	219	173	0.03%	0.003%
47	6.915	1816	1827	1845	rBV	85653	158435	23.98%	2.919%
48	7.040	1861	1866	1870	rBV3	432	545	0.08%	0.010%
49	7.136	1894	1896	1900	rVB2	336	247	0.04%	0.005%
50	7.165	1900	1905	1914	rVB3	519	831	0.13%	0.015%
51	7.243	1914	1929	1953	rBV	300513	524766	79.43%	9.669%
52	7.554	2016	2026	2047	rBV	58518	105420	15.96%	1.942%
53	7.818	2103	2108	2111	rBV2	212	255	0.04%	0.005%
54	7.879	2120	2127	2130	rBV	480	624	0.09%	0.011%
55	8.024	2163	2172	2214	rBV	167464	333182	50.43%	6.139%
56	8.406	2288	2291	2293	rBV3	254	207	0.03%	0.004%
57	8.513	2320	2324	2327	rBV2	166	184	0.03%	0.003%
58	8.561	2335	2339	2342	rVB	152	150	0.02%	0.003%
59	8.783	2397	2408	2447	rBV	360566	595942	90.20%	10.981%
60	9.255	2551	2555	2558	rBV2	228	264	0.04%	0.005%
61	9.490	2625	2628	2630	rBV2	184	166	0.03%	0.003%
62	9.696	2688	2692	2699	rBV2	241	328	0.05%	0.006%
63	9.914	2758	2760	2766	rBV2	149	169	0.03%	0.003%
64	10.043	2795	2800	2802	rVB	185	151	0.02%	0.003%
65	10.152	2823	2834	2854	rBV	205282	320948	48.58%	5.914%
66	10.326	2881	2888	2893	rBV2	675	839	0.13%	0.015%
67	10.413	2911	2915	2918	rBV2	226	213	0.03%	0.004%
68	10.451	2924	2927	2929	rBV2	187	156	0.02%	0.003%
69	10.567	2960	2963	2966	rBV2	179	160	0.02%	0.003%
70	10.680	2995	2998	3001	rBV	151	150	0.02%	0.003%
71	10.815	3038	3040	3044	rBV	175	159	0.02%	0.003%
72	10.840	3044	3048	3051	rVB2	168	155	0.02%	0.003%
73	10.876	3052	3059	3066	rBV2	205	357	0.05%	0.007%
74	10.969	3083	3088	3091	rBV	201	228	0.03%	0.004%
75	11.185	3144	3155	3179	rBV	383306	582917	88.23%	10.741%
76	11.561	3260	3272	3298	rBV	311725	497302	75.27%	9.163%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033948.D
 Acq On : 01 Feb 2024 15:02
 Operator : SY/MD
 Sample : P1310-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH917

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.979	3395	3402	3408	rBV	284	401	0.06%	0.007%
78	12.056	3420	3426	3430	rBV2	244	354	0.05%	0.007%
79	12.181	3463	3465	3469	rVB2	339	208	0.03%	0.004%
80	12.207	3469	3473	3477	rBV2	220	182	0.03%	0.003%
81	12.310	3496	3505	3510	rBV4	868	1402	0.21%	0.026%
82	12.345	3514	3516	3520	rBV2	174	149	0.02%	0.003%
83	12.429	3538	3542	3545	rBV2	159	153	0.02%	0.003%
84	12.660	3611	3614	3617	rBV	259	215	0.03%	0.004%
85	12.940	3697	3701	3703	rBV2	165	152	0.02%	0.003%
86	13.197	3774	3781	3784	rBV2	211	300	0.05%	0.006%
87	13.416	3843	3849	3852	rBV2	238	318	0.05%	0.006%
88	13.554	3889	3892	3894	rBV	327	195	0.03%	0.004%
89	13.673	3926	3929	3932	rBV3	225	148	0.02%	0.003%
90	13.712	3936	3941	3944	rBV2	219	250	0.04%	0.005%
91	13.754	3949	3954	3955	rBV2	177	163	0.02%	0.003%
92	13.895	3993	3998	4002	rBV2	405	332	0.05%	0.006%
93	13.969	4018	4021	4022	rBV2	290	171	0.03%	0.003%
94	14.168	4080	4083	4085	rBV	255	160	0.02%	0.003%
95	14.184	4085	4088	4091	rVV	300	205	0.03%	0.004%
96	14.236	4101	4104	4106	rBV	207	158	0.02%	0.003%
97	14.609	4217	4220	4224	rBV2	197	179	0.03%	0.003%
98	14.667	4235	4238	4240	rVB2	293	182	0.03%	0.003%
99	14.686	4240	4244	4245	rBV	302	228	0.03%	0.004%
100	15.483	4490	4492	4497	rVB3	395	281	0.04%	0.005%




Sum of corrected areas: 5427101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033948.D
Acq On : 01 Feb 2024 15:02
Operator : SY/MD
Sample : P1310-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

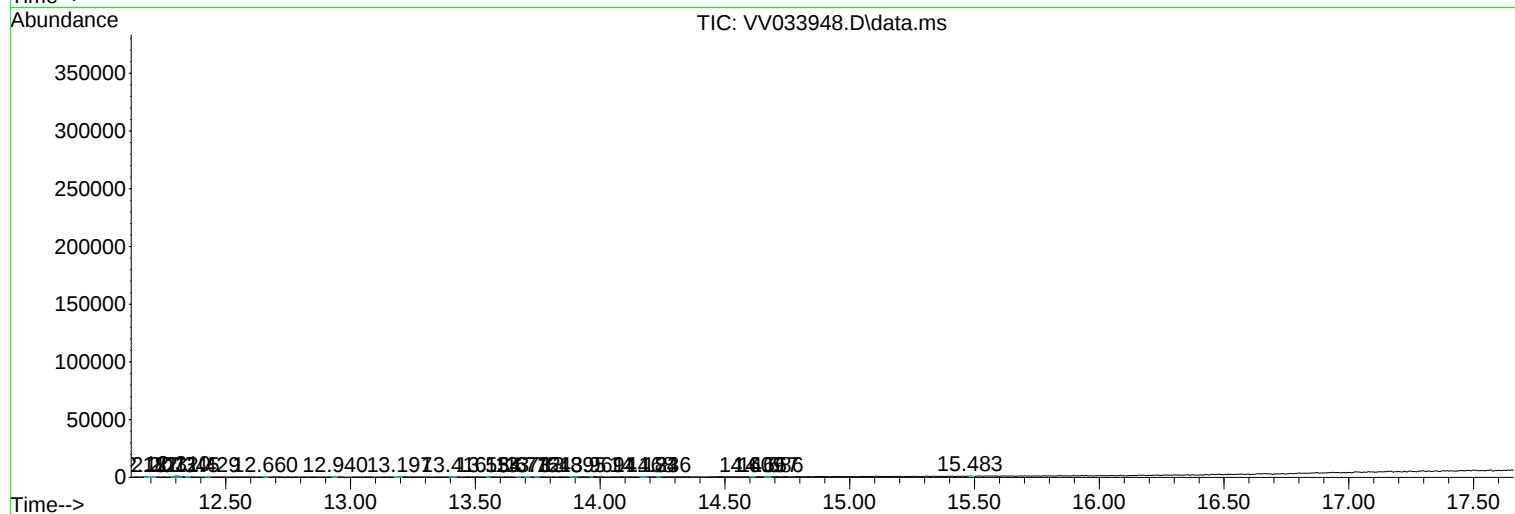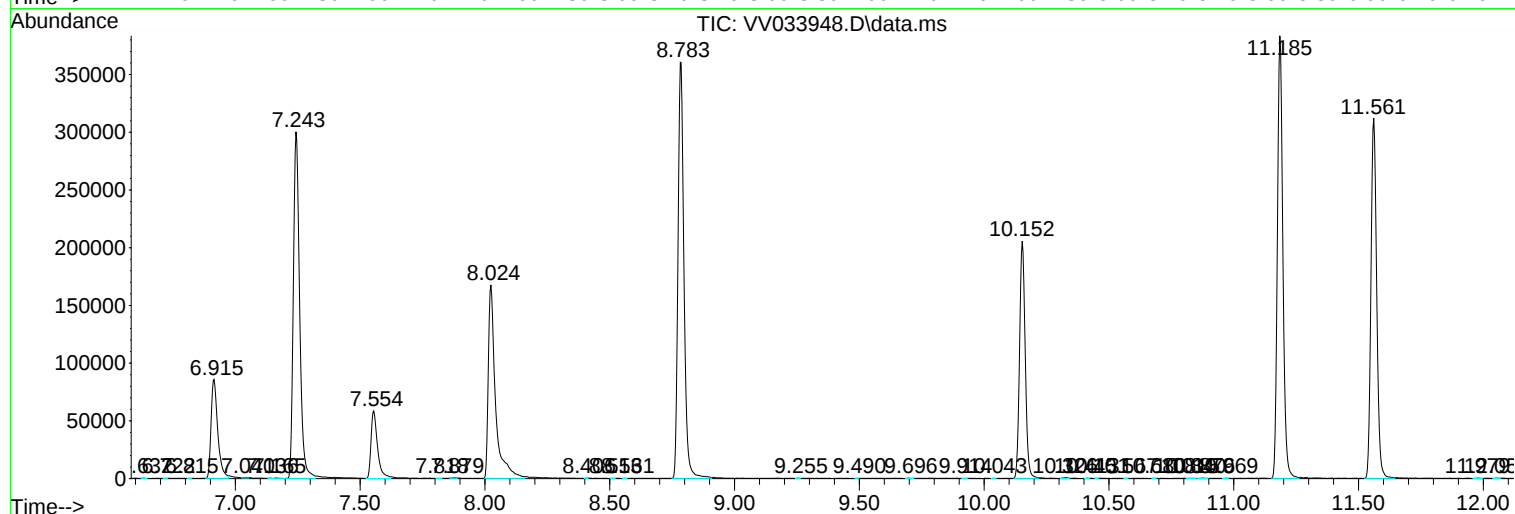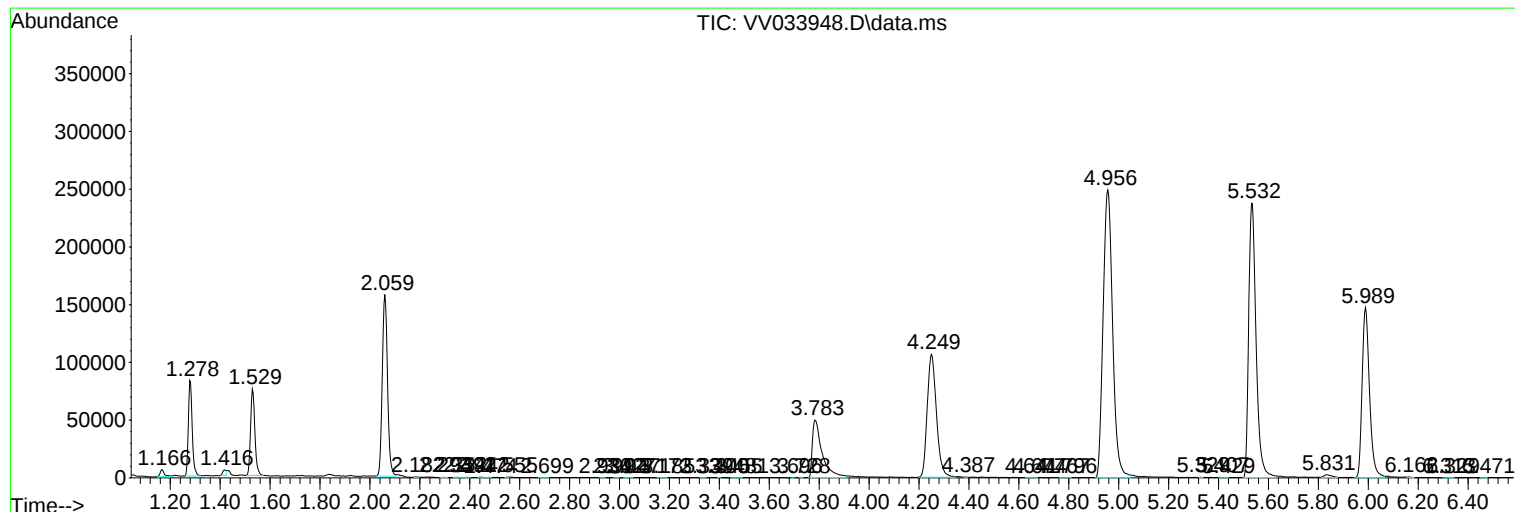

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033948.D
Acq On : 01 Feb 2024 15:02
Operator : SY/MD
Sample : P1310-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033948.D
Acq On : 01 Feb 2024 15:02
Operator : SY/MD
Sample : P1310-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc