

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033949.D
 Acq On : 01 Feb 2024 15:26
 Operator : SY/MD
 Sample : P1310-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH920

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	45	rBV	3938	4358	0.67%	0.080%
2	1.278	67	74	90	rBV	81382	89393	13.75%	1.650%
3	1.417	111	117	129	rBV2	22935	24594	3.78%	0.454%
4	1.529	144	152	167	rBV	73093	88110	13.56%	1.626%
5	2.060	307	317	341	rVB	154699	227436	35.00%	4.197%
6	2.230	362	370	388	rVB3	1859	3760	0.58%	0.069%
7	2.320	395	398	403	rBV2	207	231	0.04%	0.004%
8	2.439	429	435	436	rBV2	401	286	0.04%	0.005%
9	2.552	465	470	473	rBV3	478	539	0.08%	0.010%
10	2.642	495	498	502	rVB	206	174	0.03%	0.003%
11	2.921	583	585	591	rVB	190	198	0.03%	0.004%
12	2.973	596	601	604	rBB	170	153	0.02%	0.003%
13	3.137	647	652	657	rBV	196	249	0.04%	0.005%
14	3.298	695	702	704	rBV	196	266	0.04%	0.005%
15	3.359	718	721	726	rBV	194	203	0.03%	0.004%
16	3.388	726	730	734	rVB2	176	198	0.03%	0.004%
17	3.439	742	746	750	rBV2	216	206	0.03%	0.004%
18	3.465	750	754	761	rVB2	172	207	0.03%	0.004%
19	3.507	762	767	771	rVB	274	305	0.05%	0.006%
20	3.532	771	775	780	rBV	192	216	0.03%	0.004%
21	3.613	796	800	804	rBV	199	176	0.03%	0.003%
22	3.725	830	835	837	rBV	210	219	0.03%	0.004%
23	3.783	845	853	889	rBV	51682	138532	21.32%	2.556%
24	4.249	983	998	1031	rBV	104175	265291	40.82%	4.896%
25	4.532	1083	1086	1091	rVB2	408	390	0.06%	0.007%
26	4.574	1094	1099	1102	rVB2	285	259	0.04%	0.005%
27	4.590	1102	1104	1110	rBV2	142	143	0.02%	0.003%
28	4.696	1132	1137	1139	rBV2	279	264	0.04%	0.005%
29	4.957	1202	1218	1246	rBV2	248402	649907	100.00%	11.993%
30	5.532	1382	1397	1428	rBV	241842	494762	76.13%	9.130%
31	5.834	1483	1491	1509	rVB4	2557	5708	0.88%	0.105%
32	5.931	1517	1521	1524	rBV2	311	335	0.05%	0.006%
33	5.989	1526	1539	1565	rBV	146178	296731	45.66%	5.476%
34	6.233	1613	1615	1620	rVB	337	244	0.04%	0.005%
35	6.262	1621	1624	1629	rBV2	331	272	0.04%	0.005%
36	6.307	1634	1638	1641	rBV	264	234	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033949.D
 Acq On : 01 Feb 2024 15:26
 Operator : SY/MD
 Sample : P1310-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH920

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.506	1697	1700	1703	rBV	209	198	0.03%	0.004%
38	6.580	1720	1723	1725	rBV2	196	164	0.03%	0.003%
39	6.674	1749	1752	1756	rVB	205	162	0.02%	0.003%
40	6.712	1760	1764	1767	rBV	142	150	0.02%	0.003%
41	6.812	1791	1795	1799	rBV2	157	173	0.03%	0.003%
42	6.915	1816	1827	1854	rBV2	84983	160538	24.70%	2.963%
43	7.088	1878	1881	1884	rBV2	235	208	0.03%	0.004%
44	7.243	1918	1929	1954	rBV	293231	512318	78.83%	9.454%
45	7.555	2013	2026	2055	rBV	56963	106580	16.40%	1.967%
46	7.789	2096	2099	2103	rBV2	321	267	0.04%	0.005%
47	7.931	2140	2143	2147	rVB	241	233	0.04%	0.004%
48	8.024	2163	2172	2213	rVV	171161	339823	52.29%	6.271%
49	8.288	2252	2254	2260	rBV2	300	279	0.04%	0.005%
50	8.317	2260	2263	2268	rVB2	238	207	0.03%	0.004%
51	8.448	2298	2304	2309	rVB3	253	264	0.04%	0.005%
52	8.500	2316	2320	2323	rBV2	149	154	0.02%	0.003%
53	8.612	2350	2355	2358	rBV2	177	172	0.03%	0.003%
54	8.731	2388	2392	2396	rVB2	184	156	0.02%	0.003%
55	8.783	2397	2408	2444	rBV	360770	601595	92.57%	11.102%
56	9.252	2550	2554	2559	rBV2	277	328	0.05%	0.006%
57	9.329	2575	2578	2580	rBV2	175	150	0.02%	0.003%
58	9.461	2613	2619	2624	rBV2	223	330	0.05%	0.006%
59	9.516	2632	2636	2638	rBV2	190	163	0.03%	0.003%
60	9.725	2698	2701	2702	rBV	227	155	0.02%	0.003%
61	9.979	2774	2780	2783	rBV	281	350	0.05%	0.006%
62	10.153	2823	2834	2860	rVV	204292	318716	49.04%	5.882%
63	10.548	2954	2957	2964	rBV2	178	186	0.03%	0.003%
64	10.664	2989	2993	2995	rBV	161	153	0.02%	0.003%
65	10.728	3007	3013	3015	rBV2	202	228	0.04%	0.004%
66	10.834	3042	3046	3049	rBV2	212	246	0.04%	0.005%
67	11.040	3106	3110	3113	rBV2	179	208	0.03%	0.004%
68	11.185	3144	3155	3184	rBV	385640	588621	90.57%	10.862%
69	11.300	3189	3191	3195	rVB2	386	264	0.04%	0.005%
70	11.365	3206	3211	3213	rBV2	161	142	0.02%	0.003%
71	11.561	3261	3272	3294	rBV	306698	482278	74.21%	8.900%
72	11.834	3351	3357	3359	rBV	158	197	0.03%	0.004%
73	11.866	3364	3367	3372	rBV2	240	245	0.04%	0.005%
74	11.898	3372	3377	3378	rBV2	220	152	0.02%	0.003%
75	11.995	3404	3407	3411	rVB	158	155	0.02%	0.003%
76	12.101	3435	3440	3442	rBV	216	211	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020124\
 Data File : VW033949.D
 Acq On : 01 Feb 2024 15:26
 Operator : SY/MD
 Sample : P1310-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH920

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.249	3482	3486	3489	rBV2	297	286	0.04%	0.005%
78	12.786	3648	3653	3656	rBV2	174	217	0.03%	0.004%
79	12.908	3688	3691	3695	rBV	170	147	0.02%	0.003%
80	13.040	3729	3732	3738	rBV	206	240	0.04%	0.004%
81	13.088	3743	3747	3753	rBV2	250	305	0.05%	0.006%
82	13.204	3781	3783	3786	rVB2	235	150	0.02%	0.003%
83	13.233	3786	3792	3794	rBV2	260	308	0.05%	0.006%
84	13.468	3860	3865	3869	rBV	359	346	0.05%	0.006%
85	13.599	3903	3906	3912	rBV2	318	290	0.04%	0.005%
86	13.744	3947	3951	3955	rVB2	304	240	0.04%	0.004%
87	13.795	3962	3967	3968	rBV	269	185	0.03%	0.003%
88	13.850	3981	3984	3989	rBV2	222	248	0.04%	0.005%
89	13.988	4024	4027	4033	rVB3	457	514	0.08%	0.009%
90	14.033	4033	4041	4043	rBV2	321	402	0.06%	0.007%
91	14.098	4056	4061	4067	rVB3	380	527	0.08%	0.010%
92	14.130	4067	4071	4073	rBV	298	259	0.04%	0.005%
93	14.165	4078	4082	4085	rBV2	220	218	0.03%	0.004%
94	14.246	4105	4107	4111	rBV2	261	210	0.03%	0.004%
95	14.455	4169	4172	4176	rBV2	448	357	0.05%	0.007%
96	14.574	4206	4209	4211	rBV2	264	184	0.03%	0.003%
97	15.101	4370	4373	4375	rBV2	212	168	0.03%	0.003%
98	15.223	4409	4411	4415	rBV2	481	293	0.05%	0.005%
99	15.287	4428	4431	4435	rBV3	389	420	0.06%	0.008%
100	15.413	4464	4470	4473	rBV2	597	767	0.12%	0.014%




Sum of corrected areas: 5418949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033949.D
Acq On : 01 Feb 2024 15:26
Operator : SY/MD
Sample : P1310-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

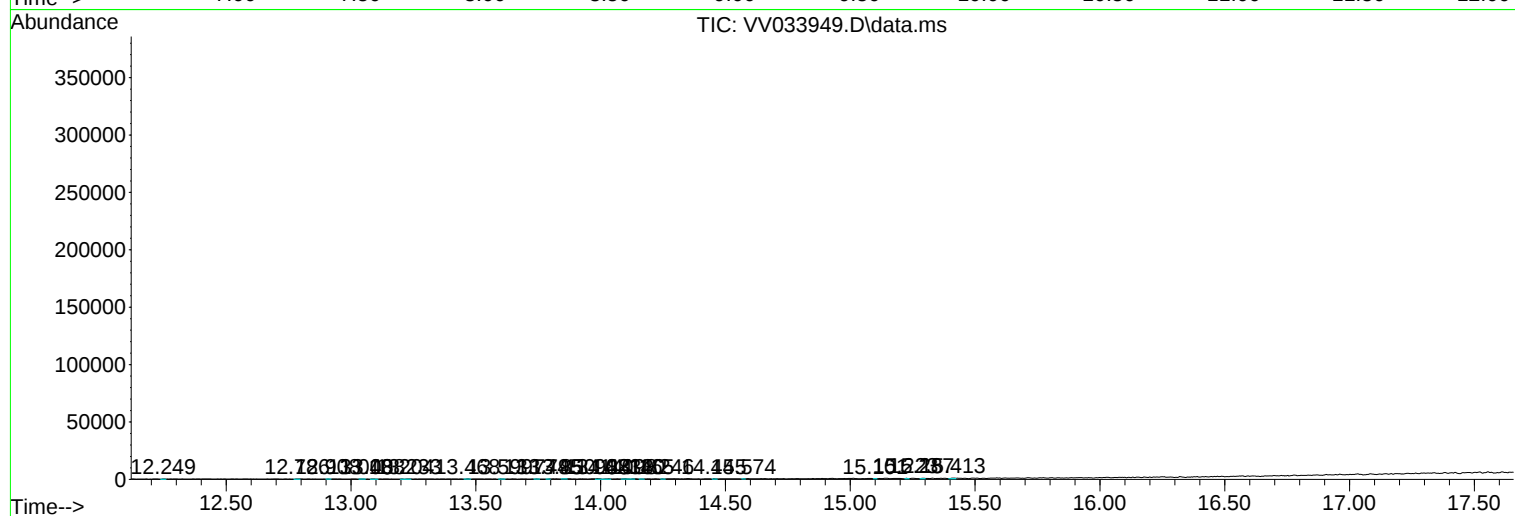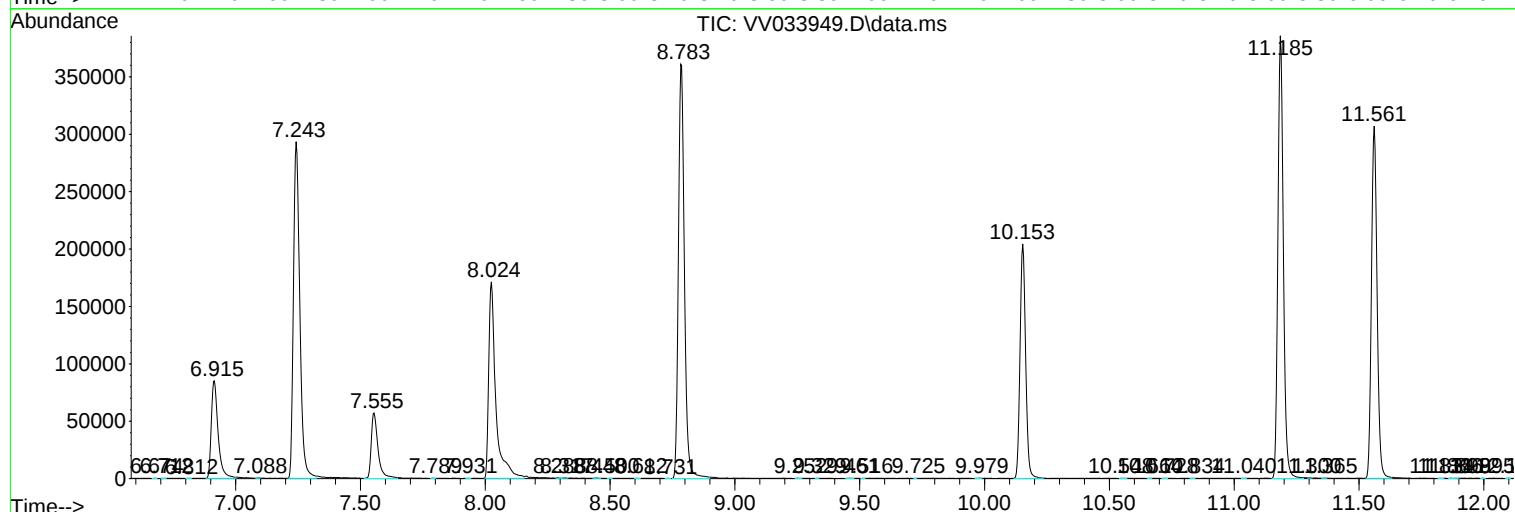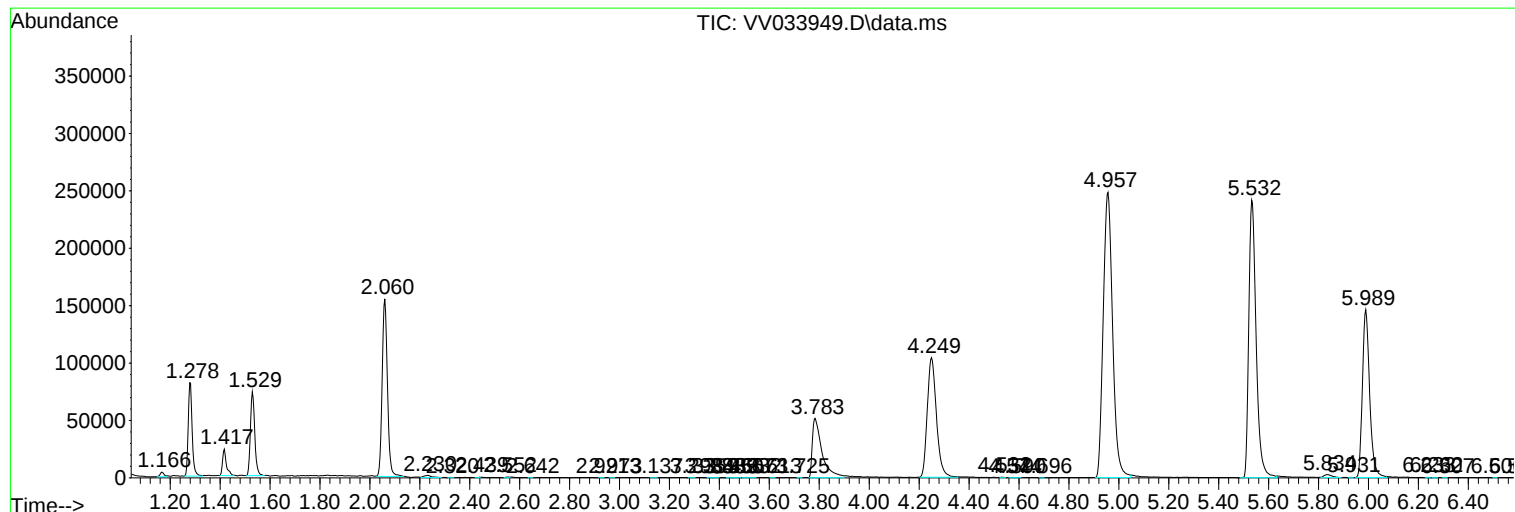

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033949.D
Acq On : 01 Feb 2024 15:26
Operator : SY/MD
Sample : P1310-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033949.D
Acq On : 01 Feb 2024 15:26
Operator : SY/MD
Sample : P1310-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
