

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033950.D
 Acq On : 01 Feb 2024 15:50
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	32	39	45	rBV	5847	6528	1.00%	0.119%
2	1.281	67	75	89	rBV	81067	86422	13.25%	1.571%
3	1.436	113	123	129	rVB7	4691	6488	0.99%	0.118%
4	1.529	144	152	172	rVB	74107	91007	13.95%	1.654%
5	2.060	307	317	335	rVB	153801	221794	34.01%	4.031%
6	2.240	370	373	375	rVB2	286	171	0.03%	0.003%
7	2.397	419	422	427	rVB2	245	286	0.04%	0.005%
8	2.452	427	439	449	rBV3	2284	3900	0.60%	0.071%
9	2.551	468	470	472	rBV	275	190	0.03%	0.003%
10	2.706	515	518	526	rBV	132	182	0.03%	0.003%
11	2.854	560	564	566	rBV	202	149	0.02%	0.003%
12	2.973	597	601	603	rBV2	166	171	0.03%	0.003%
13	3.098	636	640	644	rBV2	300	327	0.05%	0.006%
14	3.124	644	648	651	rVV	196	183	0.03%	0.003%
15	3.169	658	662	665	rVB	163	159	0.02%	0.003%
16	3.233	679	682	685	rBV2	209	161	0.02%	0.003%
17	3.310	700	706	708	rBV2	193	198	0.03%	0.004%
18	3.349	714	718	720	rBV	158	159	0.02%	0.003%
19	3.481	755	759	762	rBV2	182	205	0.03%	0.004%
20	3.519	769	771	773	rVB	280	149	0.02%	0.003%
21	3.542	774	778	780	rBV2	289	277	0.04%	0.005%
22	3.667	816	817	821	rVB2	273	149	0.02%	0.003%
23	3.690	821	824	826	rBV	257	171	0.03%	0.003%
24	3.706	826	829	832	rVB	339	269	0.04%	0.005%
25	3.735	832	838	842	rBB2	235	258	0.04%	0.005%
26	3.783	843	853	890	rBV	54759	144996	22.23%	2.635%
27	4.249	983	998	1027	rBV	105986	269221	41.28%	4.893%
28	4.535	1084	1087	1093	rBV2	218	268	0.04%	0.005%
29	4.748	1147	1153	1156	rBV	161	214	0.03%	0.004%
30	4.957	1201	1218	1248	rBV2	248201	652181	100.00%	11.854%
31	5.259	1310	1312	1317	rBV3	247	154	0.02%	0.003%
32	5.333	1329	1335	1338	rBV2	278	298	0.05%	0.005%
33	5.394	1350	1354	1359	rVB3	173	150	0.02%	0.003%
34	5.532	1385	1397	1428	rBV	253329	514259	78.85%	9.347%
35	5.834	1480	1491	1495	rBV4	2848	4620	0.71%	0.084%
36	5.924	1515	1519	1523	rBV3	217	236	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033950.D
 Acq On : 01 Feb 2024 15:50
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1566	rBV	143902	298823	45.82%	5.431%
38	6.146	1585	1588	1591	rVB3	419	245	0.04%	0.004%
39	6.207	1602	1607	1611	rVB2	405	486	0.07%	0.009%
40	6.233	1611	1615	1616	rBV2	306	214	0.03%	0.004%
41	6.313	1636	1640	1644	rBV2	207	203	0.03%	0.004%
42	6.336	1644	1647	1650	rBV2	220	210	0.03%	0.004%
43	6.426	1672	1675	1679	rBV2	213	232	0.04%	0.004%
44	6.519	1698	1704	1709	rBV2	190	347	0.05%	0.006%
45	6.767	1778	1781	1785	rVB2	186	149	0.02%	0.003%
46	6.792	1785	1789	1791	rBV2	180	183	0.03%	0.003%
47	6.854	1805	1808	1812	rBV2	283	255	0.04%	0.005%
48	6.915	1816	1827	1860	rVV	84324	160844	24.66%	2.924%
49	7.120	1889	1891	1894	rBV2	259	155	0.02%	0.003%
50	7.140	1894	1897	1900	rBV3	263	205	0.03%	0.004%
51	7.243	1918	1929	1957	rBV	289234	509850	78.18%	9.267%
52	7.554	2017	2026	2050	rBV	58191	104374	16.00%	1.897%
53	7.905	2130	2135	2138	rBV2	247	288	0.04%	0.005%
54	8.024	2163	2172	2204	rBV	175348	346005	53.05%	6.289%
55	8.300	2254	2258	2261	rVB	227	162	0.02%	0.003%
56	8.365	2275	2278	2281	rBV2	343	229	0.04%	0.004%
57	8.407	2289	2291	2297	rVB2	308	280	0.04%	0.005%
58	8.689	2376	2379	2381	rBV	184	153	0.02%	0.003%
59	8.783	2397	2408	2439	rBV	378270	622808	95.50%	11.320%
60	9.082	2496	2501	2504	rBV2	382	460	0.07%	0.008%
61	9.133	2512	2517	2518	rBV	212	186	0.03%	0.003%
62	9.320	2570	2575	2577	rBV	201	204	0.03%	0.004%
63	9.471	2618	2622	2625	rBV2	211	225	0.03%	0.004%
64	9.513	2631	2635	2637	rBV	202	171	0.03%	0.003%
65	9.599	2659	2662	2666	rBV2	145	156	0.02%	0.003%
66	9.686	2684	2689	2694	rBV2	175	262	0.04%	0.005%
67	9.751	2705	2709	2713	rBV2	176	201	0.03%	0.004%
68	9.831	2730	2734	2736	rBV	157	151	0.02%	0.003%
69	10.152	2822	2834	2858	rVV	209587	328116	50.31%	5.964%
70	10.741	3014	3017	3020	rBV2	205	170	0.03%	0.003%
71	10.844	3043	3049	3052	rBV	170	222	0.03%	0.004%
72	11.072	3115	3120	3122	rBV2	207	228	0.03%	0.004%
73	11.185	3145	3155	3180	rBV	390952	615075	94.31%	11.180%
74	11.377	3213	3215	3219	rVB2	271	165	0.03%	0.003%
75	11.561	3260	3272	3296	rBV	317622	495632	76.00%	9.009%
76	11.831	3351	3356	3357	rBV	352	224	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033950.D
 Acq On : 01 Feb 2024 15:50
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.969	3396	3399	3403	rVB2	230	175	0.03%	0.003%
78	12.008	3408	3411	3416	rVB	240	277	0.04%	0.005%
79	12.062	3422	3428	3434	rBV2	275	427	0.07%	0.008%
80	12.159	3454	3458	3462	rBV2	238	273	0.04%	0.005%
81	12.455	3547	3550	3553	rBV	244	223	0.03%	0.004%
82	12.574	3580	3587	3591	rVB2	247	353	0.05%	0.006%
83	12.606	3591	3597	3599	rBV2	208	263	0.04%	0.005%
84	12.721	3626	3633	3637	rBV2	186	298	0.05%	0.005%
85	12.776	3647	3650	3653	rBV2	205	158	0.02%	0.003%
86	12.799	3653	3657	3661	rBV2	241	295	0.05%	0.005%
87	13.130	3757	3760	3763	rBV	219	162	0.02%	0.003%
88	13.590	3899	3903	3907	rBV2	199	240	0.04%	0.004%
89	13.802	3966	3969	3975	rVB2	336	291	0.04%	0.005%
90	13.937	4009	4011	4014	rBV	227	179	0.03%	0.003%
91	14.053	4045	4047	4053	rVB3	396	326	0.05%	0.006%
92	14.085	4053	4057	4059	rBV3	320	295	0.05%	0.005%
93	14.278	4111	4117	4125	rBV2	392	775	0.12%	0.014%
94	14.355	4137	4141	4145	rBV2	308	336	0.05%	0.006%
95	14.413	4156	4159	4161	rBV2	270	172	0.03%	0.003%
96	14.712	4249	4252	4257	rVB3	269	188	0.03%	0.003%
97	14.737	4257	4260	4263	rBV	257	152	0.02%	0.003%
98	15.014	4345	4346	4348	rBV	310	151	0.02%	0.003%
99	15.528	4504	4506	4510	rBV3	324	205	0.03%	0.004%
100	15.921	4626	4628	4632	rVB3	633	386	0.06%	0.007%




Sum of corrected areas: 5501698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033950.D
Acq On : 01 Feb 2024 15:50
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

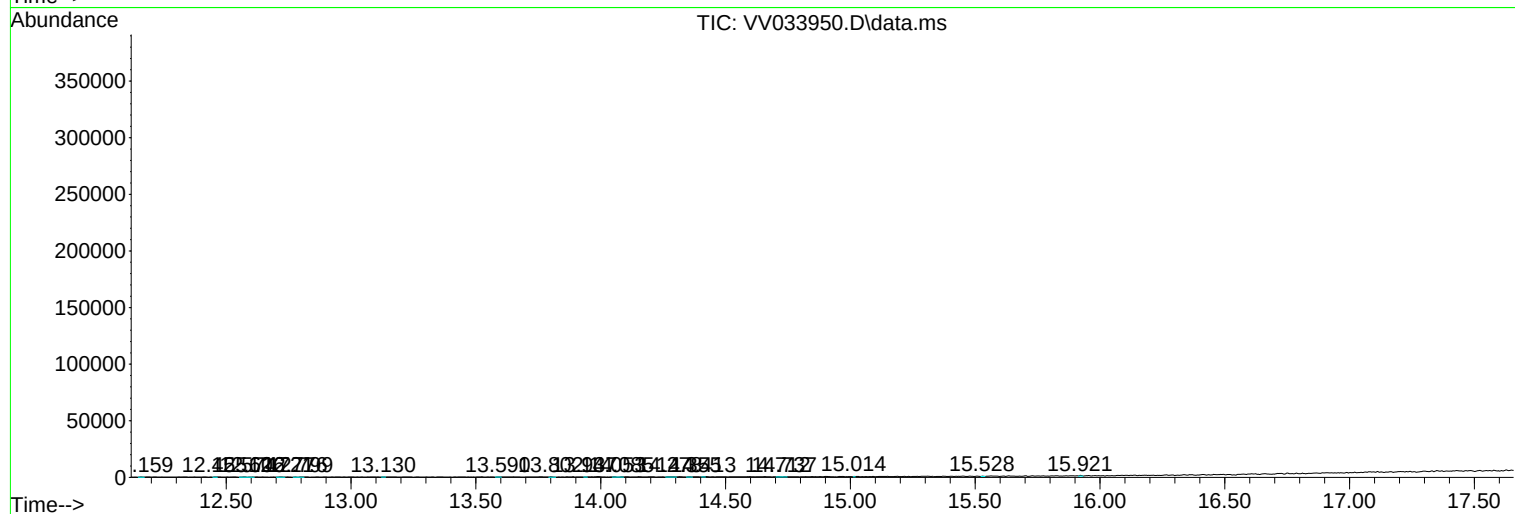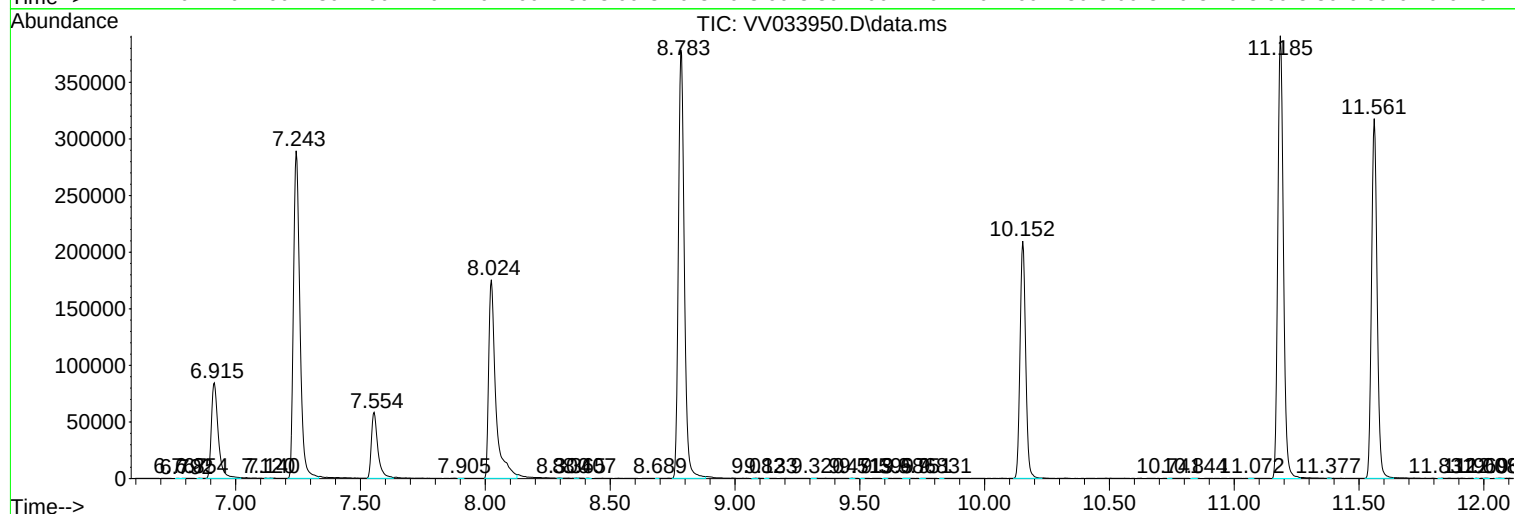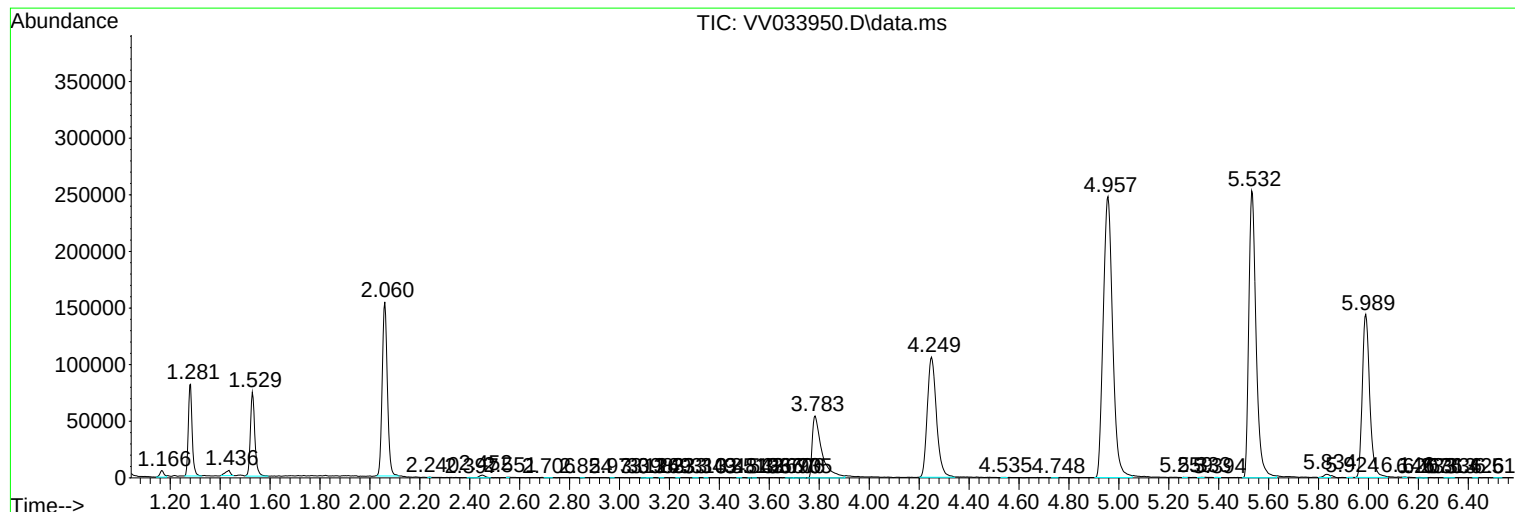

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033950.D
Acq On : 01 Feb 2024 15:50
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033950.D
Acq On : 01 Feb 2024 15:50
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc