

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033951.D
 Acq On : 01 Feb 2024 16:14
 Operator : SY/MD
 Sample : VIBLK268
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	45	rBV	4782	5255	0.82%	0.098%
2	1.282	67	75	92	rBV	77635	84271	13.19%	1.565%
3	1.529	144	152	166	rVB	70061	84652	13.25%	1.572%
4	2.060	307	317	334	rVB	147933	214973	33.65%	3.992%
5	2.240	369	373	376	rBV2	475	364	0.06%	0.007%
6	2.449	430	438	447	rBV3	2223	3491	0.55%	0.065%
7	2.494	449	452	458	rBV2	225	254	0.04%	0.005%
8	2.558	468	472	474	rBV3	389	307	0.05%	0.006%
9	2.622	485	492	495	rBV2	180	286	0.04%	0.005%
10	2.674	505	508	511	rBV	217	163	0.03%	0.003%
11	2.729	522	525	528	rBV2	206	177	0.03%	0.003%
12	2.799	543	547	550	rBV2	197	190	0.03%	0.004%
13	2.886	569	574	576	rBV2	188	192	0.03%	0.004%
14	3.073	627	632	634	rBV	205	183	0.03%	0.003%
15	3.137	647	652	662	rVB2	192	350	0.05%	0.006%
16	3.179	662	665	671	rBV2	226	282	0.04%	0.005%
17	3.368	720	724	728	rBV2	223	221	0.03%	0.004%
18	3.619	797	802	805	rVV2	150	180	0.03%	0.003%
19	3.783	842	853	884	rBV	55830	145852	22.83%	2.708%
20	4.018	923	926	929	rBV2	378	286	0.04%	0.005%
21	4.249	982	998	1032	rBV	104166	265311	41.53%	4.927%
22	4.452	1057	1061	1062	rBV	312	259	0.04%	0.005%
23	4.500	1074	1076	1080	rVB2	477	302	0.05%	0.006%
24	4.536	1084	1087	1091	rVB3	413	346	0.05%	0.006%
25	4.574	1096	1099	1101	rBV2	276	246	0.04%	0.005%
26	4.603	1105	1108	1110	rBV	306	233	0.04%	0.004%
27	4.626	1111	1115	1117	rBV2	234	170	0.03%	0.003%
28	4.738	1143	1150	1152	rBV2	175	243	0.04%	0.005%
29	4.847	1181	1184	1187	rVB2	295	265	0.04%	0.005%
30	4.873	1188	1192	1196	rBV2	297	360	0.06%	0.007%
31	4.957	1202	1218	1258	rBV2	239346	638771	100.00%	11.862%
32	5.426	1360	1364	1366	rBV	370	301	0.05%	0.006%
33	5.468	1373	1377	1380	rBV2	279	240	0.04%	0.004%
34	5.532	1386	1397	1435	rBV	243663	501256	78.47%	9.308%
35	5.728	1455	1458	1462	rVB3	355	302	0.05%	0.006%
36	5.831	1482	1490	1501	rBV6	2334	5059	0.79%	0.094%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033951.D
 Acq On : 01 Feb 2024 16:14
 Operator : SY/MD
 Sample : VIBLK268
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1569	rVV	140402	293008	45.87%	5.441%
38	6.153	1586	1590	1591	rBV3	563	396	0.06%	0.007%
39	6.246	1616	1619	1622	rBV	153	156	0.02%	0.003%
40	6.278	1624	1629	1632	rBV2	147	149	0.02%	0.003%
41	6.375	1656	1659	1664	rBV2	191	222	0.03%	0.004%
42	6.568	1712	1719	1723	rBV2	176	285	0.04%	0.005%
43	6.670	1749	1751	1756	rBV2	194	206	0.03%	0.004%
44	6.825	1795	1799	1802	rVB	210	144	0.02%	0.003%
45	6.915	1816	1827	1849	rBV	83058	156228	24.46%	2.901%
46	7.243	1918	1929	1955	rBV	281634	492024	77.03%	9.137%
47	7.555	2016	2026	2054	rBV	57299	103768	16.24%	1.927%
48	7.728	2078	2080	2083	rBV	190	148	0.02%	0.003%
49	7.760	2087	2090	2094	rBV2	184	182	0.03%	0.003%
50	7.879	2124	2127	2130	rVB2	241	207	0.03%	0.004%
51	8.024	2163	2172	2218	rBV	175999	353942	55.41%	6.573%
52	8.268	2245	2248	2255	rVB3	323	350	0.05%	0.006%
53	8.426	2292	2297	2300	rBV2	283	261	0.04%	0.005%
54	8.542	2330	2333	2336	rBV2	156	146	0.02%	0.003%
55	8.783	2397	2408	2444	rBV	368538	606831	95.00%	11.269%
56	9.233	2542	2548	2550	rBV	141	187	0.03%	0.003%
57	9.355	2583	2586	2591	rVB2	194	184	0.03%	0.003%
58	9.641	2670	2675	2683	rVB2	252	364	0.06%	0.007%
59	9.706	2692	2695	2701	rVB2	240	304	0.05%	0.006%
60	9.857	2738	2742	2745	rBV	152	173	0.03%	0.003%
61	9.918	2755	2761	2763	rBV2	156	176	0.03%	0.003%
62	9.985	2777	2782	2787	rVB2	171	205	0.03%	0.004%
63	10.053	2798	2803	2805	rBV	148	162	0.03%	0.003%
64	10.153	2823	2834	2859	rVV	204743	326999	51.19%	6.072%
65	10.326	2884	2888	2890	rBV	286	206	0.03%	0.004%
66	10.394	2901	2909	2913	rVV2	154	293	0.05%	0.005%
67	10.445	2920	2925	2926	rBV2	164	164	0.03%	0.003%
68	10.680	2994	2998	3000	rBV2	153	155	0.02%	0.003%
69	10.767	3022	3025	3028	rBV2	226	189	0.03%	0.004%
70	11.024	3100	3105	3107	rBV2	301	210	0.03%	0.004%
71	11.185	3144	3155	3179	rBV	375434	594551	93.08%	11.041%
72	11.313	3193	3195	3200	rVB3	380	268	0.04%	0.005%
73	11.468	3240	3243	3246	rBV2	225	168	0.03%	0.003%
74	11.561	3260	3272	3297	rBV	313127	489858	76.69%	9.096%
75	11.757	3332	3333	3340	rVB2	236	212	0.03%	0.004%
76	11.825	3346	3354	3355	rBV2	209	260	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033951.D
 Acq On : 01 Feb 2024 16:14
 Operator : SY/MD
 Sample : VIBLK268
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.953	3390	3394	3398	rVB2	162	170	0.03%	0.003%
78	11.985	3398	3404	3406	rBV2	188	238	0.04%	0.004%
79	12.088	3434	3436	3440	rBV2	172	150	0.02%	0.003%
80	12.278	3491	3495	3499	rBV	151	196	0.03%	0.004%
81	12.323	3506	3509	3513	rBV	190	218	0.03%	0.004%
82	12.374	3523	3525	3530	rBV2	128	146	0.02%	0.003%
83	12.464	3550	3553	3559	rBV2	141	175	0.03%	0.003%
84	12.535	3571	3575	3577	rBV	141	154	0.02%	0.003%
85	12.661	3610	3614	3618	rBV	174	183	0.03%	0.003%
86	12.805	3657	3659	3663	rBV2	157	148	0.02%	0.003%
87	13.056	3732	3737	3741	rBV2	244	275	0.04%	0.005%
88	13.127	3755	3759	3761	rBV2	173	163	0.03%	0.003%
89	13.272	3802	3804	3812	rVB2	187	220	0.03%	0.004%
90	13.362	3828	3832	3835	rBV	233	223	0.03%	0.004%
91	13.805	3968	3970	3977	rVB2	274	283	0.04%	0.005%
92	13.844	3977	3982	3987	rBV2	340	373	0.06%	0.007%
93	14.040	4040	4043	4045	rBV	293	188	0.03%	0.003%
94	14.053	4045	4047	4052	rVV2	269	200	0.03%	0.004%
95	14.098	4056	4061	4064	rBV2	353	291	0.05%	0.005%
96	14.432	4163	4165	4169	rVB	336	199	0.03%	0.004%
97	14.503	4184	4187	4191	rBV3	256	226	0.04%	0.004%
98	14.574	4206	4209	4213	rBV2	355	344	0.05%	0.006%
99	15.519	4499	4503	4507	rBV4	625	645	0.10%	0.012%
100	15.542	4508	4510	4513	rVV3	398	209	0.03%	0.004%



Sum of corrected areas: 5385151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033951.D
Acq On : 01 Feb 2024 16:14
Operator : SY/MD
Sample : VIBLK268
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

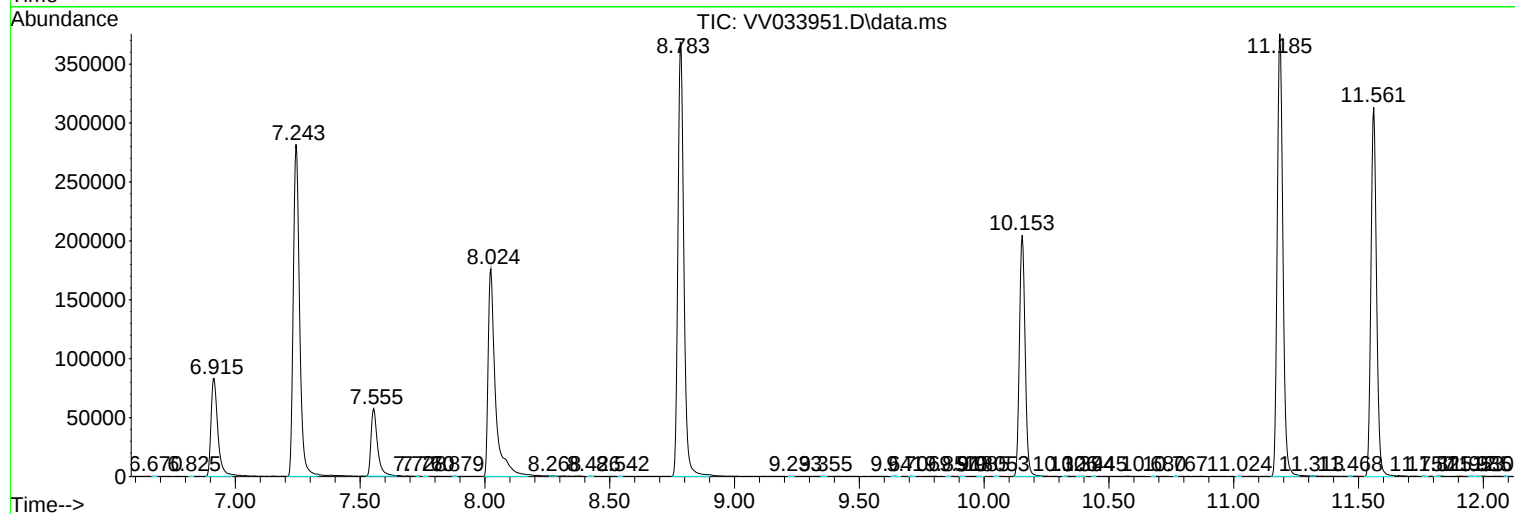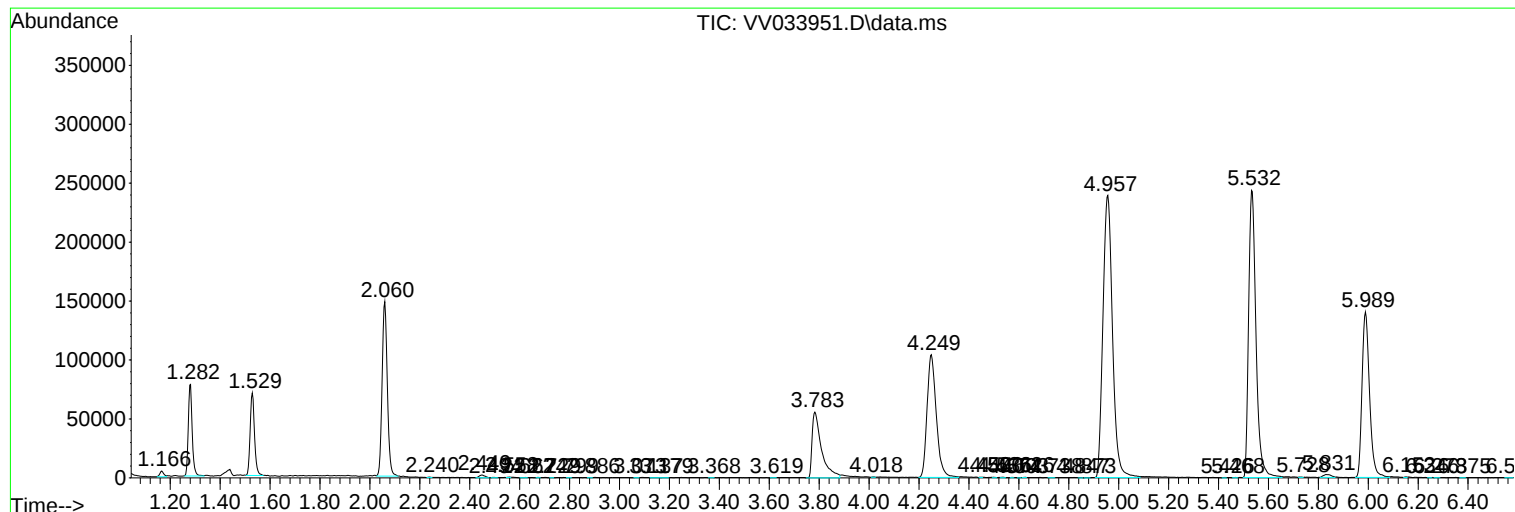

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033951.D
Acq On : 01 Feb 2024 16:14
Operator : SY/MD
Sample : VIBLK268
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033951.D
Acq On : 01 Feb 2024 16:14
Operator : SY/MD
Sample : VIBLK268
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc