

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033953.D
 Acq On : 01 Feb 2024 17:02
 Operator : SY/MD
 Sample : P1300-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	5282	6632	1.13%	0.136%
2	1.214	51	54	58	rBV2	753	660	0.11%	0.014%
3	1.278	68	74	91	rVB	61186	66349	11.33%	1.359%
4	1.442	112	125	132	rBV5	7348	12761	2.18%	0.261%
5	1.526	144	151	169	rVB	60188	74125	12.66%	1.518%
6	2.056	306	316	345	rVB	116720	177045	30.23%	3.626%
7	2.490	448	451	455	rBV	176	174	0.03%	0.004%
8	2.568	466	475	489	rBV3	3247	7339	1.25%	0.150%
9	2.690	509	513	516	rVB2	161	140	0.02%	0.003%
10	2.818	549	553	555	rBV	146	140	0.02%	0.003%
11	2.886	571	574	577	rBV	188	169	0.03%	0.003%
12	2.905	577	580	584	rVV2	233	252	0.04%	0.005%
13	2.947	588	593	598	rBV2	179	186	0.03%	0.004%
14	3.053	623	626	630	rBV2	184	154	0.03%	0.003%
15	3.117	642	646	648	rBV	183	162	0.03%	0.003%
16	3.169	658	662	664	rBV2	240	171	0.03%	0.004%
17	3.191	665	669	673	rVV	198	193	0.03%	0.004%
18	3.246	683	686	689	rBV2	142	149	0.03%	0.003%
19	3.417	734	739	742	rBV	190	211	0.04%	0.004%
20	3.503	763	766	769	rBV	171	157	0.03%	0.003%
21	3.552	778	781	785	rBV2	144	172	0.03%	0.004%
22	3.580	787	790	793	rBV	193	144	0.02%	0.003%
23	3.680	818	821	823	rBV2	259	212	0.04%	0.004%
24	3.748	839	842	845	rBV2	152	155	0.03%	0.003%
25	3.783	845	853	887	rBV	52602	139156	23.76%	2.850%
26	4.159	964	970	973	rVB3	273	325	0.06%	0.007%
27	4.249	982	998	1025	rBV	96144	241920	41.31%	4.954%
28	4.455	1058	1062	1067	rBV3	545	565	0.10%	0.012%
29	4.555	1091	1093	1097	rVB	327	191	0.03%	0.004%
30	4.735	1147	1149	1152	rBV	273	164	0.03%	0.003%
31	4.786	1161	1165	1168	rBV	192	198	0.03%	0.004%
32	4.957	1201	1218	1246	rBV2	218690	585600	100.00%	11.992%
33	5.317	1328	1330	1333	rBV2	298	175	0.03%	0.004%
34	5.368	1344	1346	1351	rVB2	242	175	0.03%	0.004%
35	5.478	1377	1380	1383	rBV2	245	168	0.03%	0.003%
36	5.535	1387	1398	1428	rBV	209602	433908	74.10%	8.886%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033953.D
 Acq On : 01 Feb 2024 17:02
 Operator : SY/MD
 Sample : P1300-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.841	1483	1493	1503	rVV5	2215	4689	0.80%	0.096%
38	5.989	1527	1539	1564	rBV	132893	272726	46.57%	5.585%
39	6.108	1575	1576	1579	rVB	307	145	0.02%	0.003%
40	6.133	1582	1584	1587	rVB3	295	171	0.03%	0.004%
41	6.307	1634	1638	1639	rBV	189	154	0.03%	0.003%
42	6.330	1644	1645	1651	rBV2	232	204	0.03%	0.004%
43	6.381	1657	1661	1667	rBV2	144	147	0.03%	0.003%
44	6.510	1693	1701	1705	rBV3	1481	2137	0.36%	0.044%
45	6.651	1742	1745	1749	rVB2	186	177	0.03%	0.004%
46	6.677	1749	1753	1754	rBV	193	159	0.03%	0.003%
47	6.709	1759	1763	1771	rBV2	222	370	0.06%	0.008%
48	6.915	1816	1827	1852	rBV	77459	144295	24.64%	2.955%
49	7.111	1885	1888	1889	rBV	240	140	0.02%	0.003%
50	7.127	1889	1893	1900	rVB2	258	309	0.05%	0.006%
51	7.159	1900	1903	1906	rBV2	273	161	0.03%	0.003%
52	7.191	1908	1913	1914	rBV2	280	205	0.04%	0.004%
53	7.243	1919	1929	1968	rBV	247626	440969	75.30%	9.030%
54	7.555	2017	2026	2060	rBV	53270	98479	16.82%	2.017%
55	7.796	2097	2101	2105	rBV3	302	282	0.05%	0.006%
56	7.876	2121	2126	2130	rVB2	324	367	0.06%	0.008%
57	8.024	2162	2172	2211	rBV	178391	347819	59.40%	7.123%
58	8.262	2243	2246	2247	rBV2	275	151	0.03%	0.003%
59	8.484	2310	2315	2318	rBV	330	421	0.07%	0.009%
60	8.580	2340	2345	2347	rBV2	231	259	0.04%	0.005%
61	8.677	2373	2375	2378	rBV	173	135	0.02%	0.003%
62	8.786	2397	2409	2431	rBV	329292	538175	91.90%	11.021%
63	9.002	2472	2476	2477	rBV2	198	161	0.03%	0.003%
64	9.272	2556	2560	2567	rBV	271	385	0.07%	0.008%
65	9.346	2579	2583	2585	rBV2	195	155	0.03%	0.003%
66	9.574	2651	2654	2659	rVB2	193	182	0.03%	0.004%
67	9.596	2659	2661	2665	rBV	145	146	0.02%	0.003%
68	9.702	2689	2694	2696	rBV2	190	223	0.04%	0.005%
69	9.780	2712	2718	2722	rBV2	210	321	0.05%	0.007%
70	9.882	2745	2750	2752	rBV2	168	208	0.04%	0.004%
71	9.931	2762	2765	2772	rVB2	192	214	0.04%	0.004%
72	10.111	2818	2821	2822	rBV	303	150	0.03%	0.003%
73	10.153	2823	2834	2852	rVV	201009	311855	53.25%	6.386%
74	10.323	2883	2887	2891	rVB2	257	248	0.04%	0.005%
75	10.805	3032	3037	3043	rBV2	321	385	0.07%	0.008%
76	11.185	3144	3155	3181	rBV	333227	518251	88.50%	10.613%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033953.D
 Acq On : 01 Feb 2024 17:02
 Operator : SY/MD
 Sample : P1300-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH6Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.471	3236	3244	3248	rBV2	271	396	0.07%	0.008%
78	11.561	3257	3272	3309	rBV	276599	440226	75.18%	9.015%
79	11.944	3388	3391	3393	rBV	194	147	0.03%	0.003%
80	12.008	3408	3411	3412	rBV2	197	132	0.02%	0.003%
81	12.628	3598	3604	3606	rBV2	223	258	0.04%	0.005%
82	12.702	3624	3627	3633	rBV	268	300	0.05%	0.006%
83	12.911	3687	3692	3694	rBV	202	203	0.03%	0.004%
84	12.940	3698	3701	3703	rVB	216	140	0.02%	0.003%
85	13.181	3771	3776	3784	rBV2	203	312	0.05%	0.006%
86	13.300	3809	3813	3818	rBV2	267	256	0.04%	0.005%
87	13.471	3861	3866	3870	rBV2	376	382	0.07%	0.008%
88	13.519	3877	3881	3884	rBV2	205	225	0.04%	0.005%
89	13.693	3931	3935	3939	rVB4	459	417	0.07%	0.009%
90	13.886	3992	3995	3998	rBV	194	165	0.03%	0.003%
91	14.014	4033	4035	4038	rVB2	340	230	0.04%	0.005%
92	14.053	4045	4047	4053	rVB2	215	198	0.03%	0.004%
93	14.104	4060	4063	4066	rBV2	202	173	0.03%	0.004%
94	14.259	4106	4111	4121	rBV3	305	553	0.09%	0.011%
95	14.580	4207	4211	4214	rBV2	339	282	0.05%	0.006%
96	14.956	4325	4328	4334	rBV2	381	285	0.05%	0.006%
97	15.120	4376	4379	4383	rBV3	341	341	0.06%	0.007%
98	15.493	4493	4495	4498	rBV2	325	173	0.03%	0.004%
99	15.509	4498	4500	4502	rVV2	387	216	0.04%	0.004%
100	15.770	4575	4581	4584	rBV4	550	701	0.12%	0.014%




Sum of corrected areas: 4883238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033953.D
Acq On : 01 Feb 2024 17:02
Operator : SY/MD
Sample : P1300-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

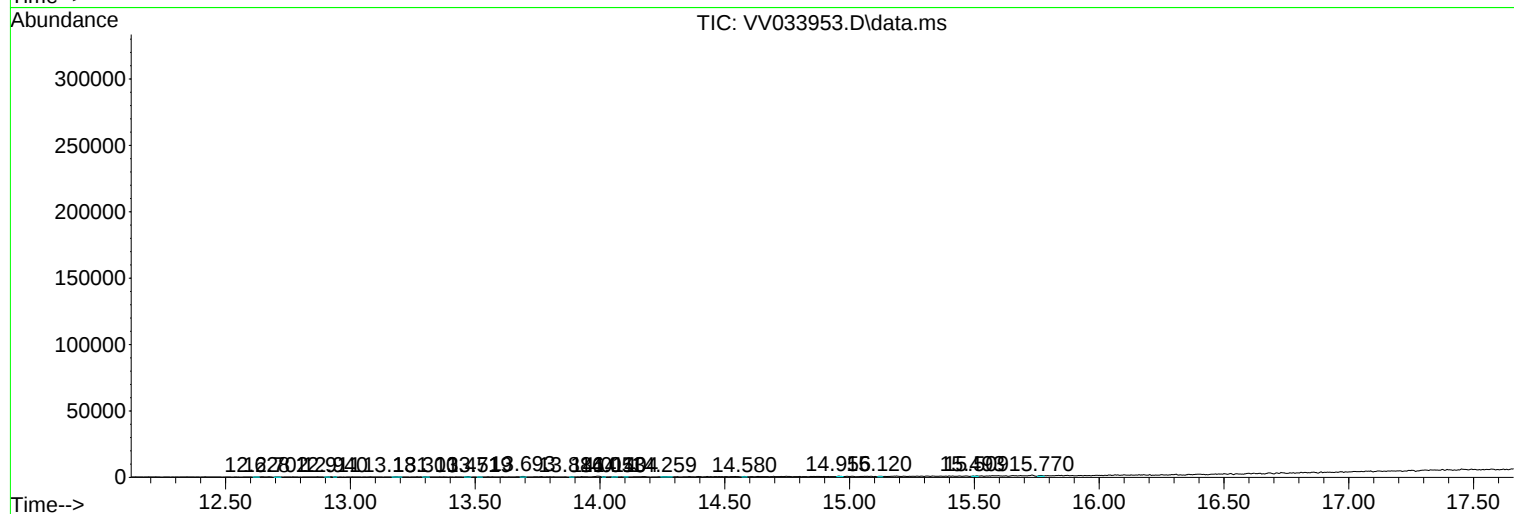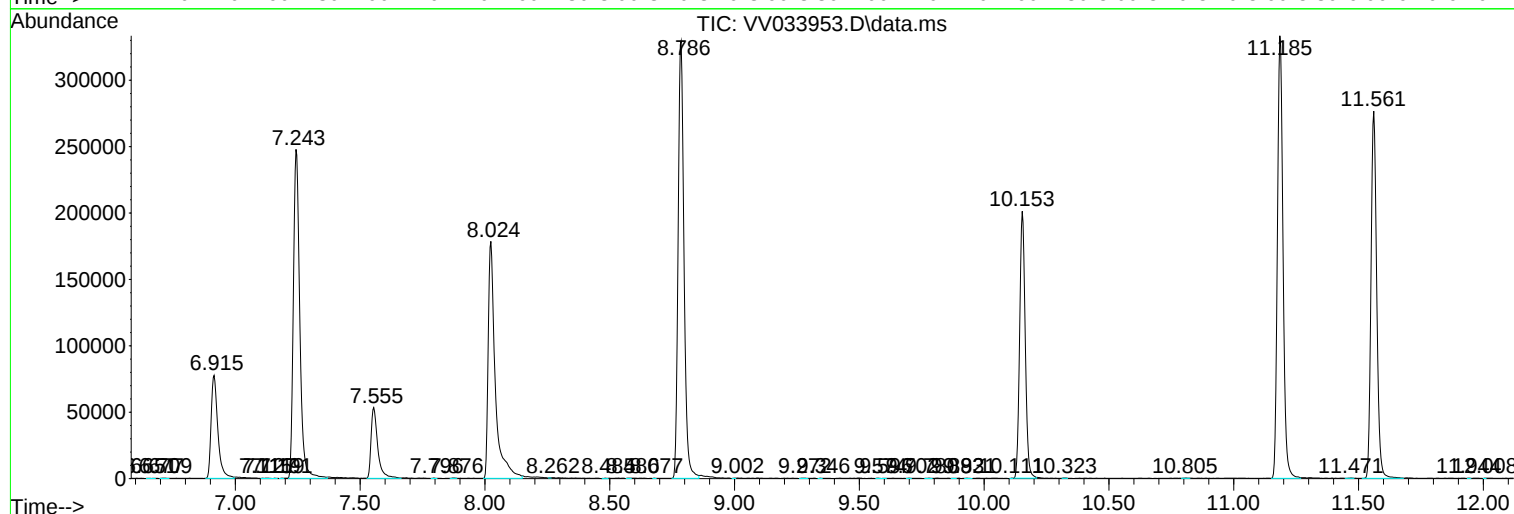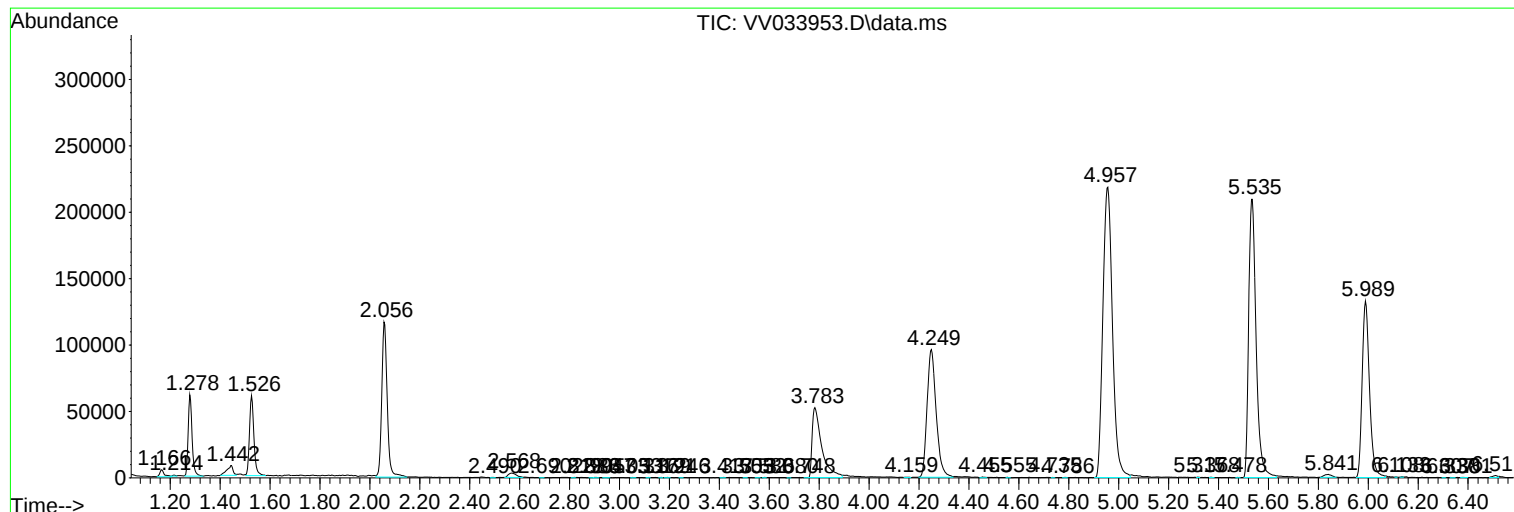

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033953.D
Acq On : 01 Feb 2024 17:02
Operator : SY/MD
Sample : P1300-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033953.D
Acq On : 01 Feb 2024 17:02
Operator : SY/MD
Sample : P1300-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH6Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc