

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033954.D
 Acq On : 01 Feb 2024 17:26
 Operator : SY/MD
 Sample : P1300-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	45	rBV	5204	5395	0.85%	0.102%
2	1.278	67	74	89	rBV	79757	86429	13.66%	1.631%
3	1.529	144	152	167	rVB	70122	85269	13.48%	1.609%
4	1.722	210	212	214	rBV3	616	309	0.05%	0.006%
5	2.060	307	317	329	rBV	147130	211831	33.49%	3.997%
6	2.224	365	368	369	rBV	316	168	0.03%	0.003%
7	2.317	394	397	400	rVV2	202	160	0.03%	0.003%
8	2.564	466	474	487	rBV2	3282	6677	1.06%	0.126%
9	2.870	563	569	576	rVB2	234	390	0.06%	0.007%
10	2.915	576	583	586	rBV2	203	312	0.05%	0.006%
11	3.285	695	698	701	rBV2	180	148	0.02%	0.003%
12	3.355	715	720	722	rVB	189	173	0.03%	0.003%
13	3.378	722	727	730	rVB2	277	337	0.05%	0.006%
14	3.413	733	738	740	rBV2	173	164	0.03%	0.003%
15	3.445	746	748	750	rBV	280	171	0.03%	0.003%
16	3.535	773	776	782	rVB	196	150	0.02%	0.003%
17	3.674	815	819	824	rVB2	218	226	0.04%	0.004%
18	3.703	824	828	831	rBV	167	177	0.03%	0.003%
19	3.728	831	836	839	rVB	222	187	0.03%	0.004%
20	3.744	839	841	845	rBV	181	168	0.03%	0.003%
21	3.783	845	853	893	rBV	50721	137327	21.71%	2.591%
22	4.249	983	998	1031	rVB	101895	261546	41.35%	4.935%
23	4.439	1054	1057	1065	rVB2	420	417	0.07%	0.008%
24	4.474	1065	1068	1071	rBV4	248	175	0.03%	0.003%
25	4.825	1172	1177	1179	rBV	141	145	0.02%	0.003%
26	4.902	1198	1201	1202	rBV	226	148	0.02%	0.003%
27	4.957	1202	1218	1253	rVV2	237605	632521	100.00%	11.936%
28	5.166	1280	1283	1285	rBV2	257	198	0.03%	0.004%
29	5.355	1340	1342	1348	rVB	227	172	0.03%	0.003%
30	5.391	1352	1353	1358	rVB	302	229	0.04%	0.004%
31	5.532	1385	1397	1422	rBV	243918	495445	78.33%	9.349%
32	5.741	1460	1462	1465	rVB2	331	193	0.03%	0.004%
33	5.838	1483	1492	1507	rVB5	2673	5851	0.93%	0.110%
34	5.902	1509	1512	1517	rBV2	188	229	0.04%	0.004%
35	5.989	1525	1539	1568	rBV	142401	290842	45.98%	5.488%
36	6.207	1602	1607	1610	rBV2	183	161	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033954.D
 Acq On : 01 Feb 2024 17:26
 Operator : SY/MD
 Sample : P1300-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.275	1626	1628	1632	rBV2	164	154	0.02%	0.003%
38	6.423	1669	1674	1676	rBV	152	155	0.02%	0.003%
39	6.513	1693	1702	1713	rBV5	1414	3190	0.50%	0.060%
40	6.558	1713	1716	1720	rVB	277	172	0.03%	0.003%
41	6.577	1720	1722	1727	rBV2	169	146	0.02%	0.003%
42	6.645	1739	1743	1745	rBV	207	153	0.02%	0.003%
43	6.915	1817	1827	1862	rVV	81521	153364	24.25%	2.894%
44	7.185	1907	1911	1914	rBV2	325	284	0.04%	0.005%
45	7.243	1918	1929	1960	rBV	275024	488899	77.29%	9.226%
46	7.554	2017	2026	2058	rBV	54431	100340	15.86%	1.893%
47	7.796	2098	2101	2105	rVB2	258	203	0.03%	0.004%
48	7.879	2117	2127	2135	rVB3	682	1266	0.20%	0.024%
49	7.969	2151	2155	2157	rBV	199	157	0.02%	0.003%
50	8.024	2163	2172	2212	rBV	177444	342991	54.23%	6.472%
51	8.313	2260	2262	2266	rVB	288	153	0.02%	0.003%
52	8.342	2269	2271	2276	rVB2	306	191	0.03%	0.004%
53	8.403	2285	2290	2292	rBV2	230	228	0.04%	0.004%
54	8.535	2330	2331	2338	rVB2	248	204	0.03%	0.004%
55	8.564	2338	2340	2343	rBV	195	150	0.02%	0.003%
56	8.783	2398	2408	2442	rBV	361905	602240	95.21%	11.364%
57	9.008	2475	2478	2480	rBV2	224	149	0.02%	0.003%
58	9.059	2490	2494	2499	rVB	306	239	0.04%	0.005%
59	9.400	2597	2600	2602	rBV2	216	149	0.02%	0.003%
60	9.458	2615	2618	2621	rBV	175	149	0.02%	0.003%
61	9.500	2627	2631	2636	rBV2	185	239	0.04%	0.005%
62	10.037	2794	2798	2800	rBV	178	158	0.02%	0.003%
63	10.152	2822	2834	2855	rVV	199526	316809	50.09%	5.978%
64	10.323	2877	2887	2895	rBV4	1028	1701	0.27%	0.032%
65	10.487	2931	2938	2942	rBV2	229	369	0.06%	0.007%
66	10.564	2959	2962	2967	rBV2	187	161	0.03%	0.003%
67	10.587	2967	2969	2973	rVV2	182	183	0.03%	0.003%
68	10.660	2984	2992	2995	rBV2	231	354	0.06%	0.007%
69	10.750	3015	3020	3023	rBV	207	233	0.04%	0.004%
70	10.892	3060	3064	3070	rBV2	142	189	0.03%	0.004%
71	10.969	3084	3088	3092	rBV	195	209	0.03%	0.004%
72	10.992	3092	3095	3099	rVB	173	156	0.02%	0.003%
73	11.075	3118	3121	3127	rVB	193	215	0.03%	0.004%
74	11.185	3144	3155	3182	rVV	373146	580446	91.77%	10.953%
75	11.561	3261	3272	3299	rBV	299389	470900	74.45%	8.886%
76	11.805	3343	3348	3350	rBV	170	163	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
 Data File : VV033954.D
 Acq On : 01 Feb 2024 17:26
 Operator : SY/MD
 Sample : P1300-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.857	3359	3364	3365	rBV	160	163	0.03%	0.003%
78	12.021	3409	3415	3417	rBV	179	200	0.03%	0.004%
79	12.094	3434	3438	3443	rBV	202	221	0.03%	0.004%
80	12.162	3452	3459	3461	rBV2	343	407	0.06%	0.008%
81	12.278	3492	3495	3500	rBV	161	185	0.03%	0.003%
82	12.657	3609	3613	3618	rVB2	222	256	0.04%	0.005%
83	12.734	3634	3637	3639	rBV	195	166	0.03%	0.003%
84	12.889	3682	3685	3688	rBV	222	190	0.03%	0.004%
85	12.953	3703	3705	3709	rVB	262	178	0.03%	0.003%
86	12.975	3709	3712	3716	rBV2	190	238	0.04%	0.004%
87	13.162	3768	3770	3775	rBV	247	204	0.03%	0.004%
88	13.619	3908	3912	3914	rBV2	252	220	0.03%	0.004%
89	13.692	3932	3935	3939	rBV2	549	526	0.08%	0.010%
90	13.924	4003	4007	4008	rBV2	212	168	0.03%	0.003%
91	13.982	4020	4025	4036	rVB3	590	1004	0.16%	0.019%
92	14.078	4051	4055	4058	rVB2	343	244	0.04%	0.005%
93	14.149	4073	4077	4081	rBV3	403	362	0.06%	0.007%
94	14.281	4115	4118	4123	rBV3	241	259	0.04%	0.005%
95	14.545	4196	4200	4202	rBV3	322	285	0.05%	0.005%
96	14.921	4315	4317	4321	rBV2	288	234	0.04%	0.004%
97	15.127	4376	4381	4384	rBV2	373	396	0.06%	0.007%
98	15.348	4447	4450	4453	rBV3	359	190	0.03%	0.004%
99	15.409	4466	4469	4471	rBV4	375	252	0.04%	0.005%
100	16.136	4692	4695	4698	rBV3	709	571	0.09%	0.011%




Sum of corrected areas: 5299370

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033954.D
Acq On : 01 Feb 2024 17:26
Operator : SY/MD
Sample : P1300-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

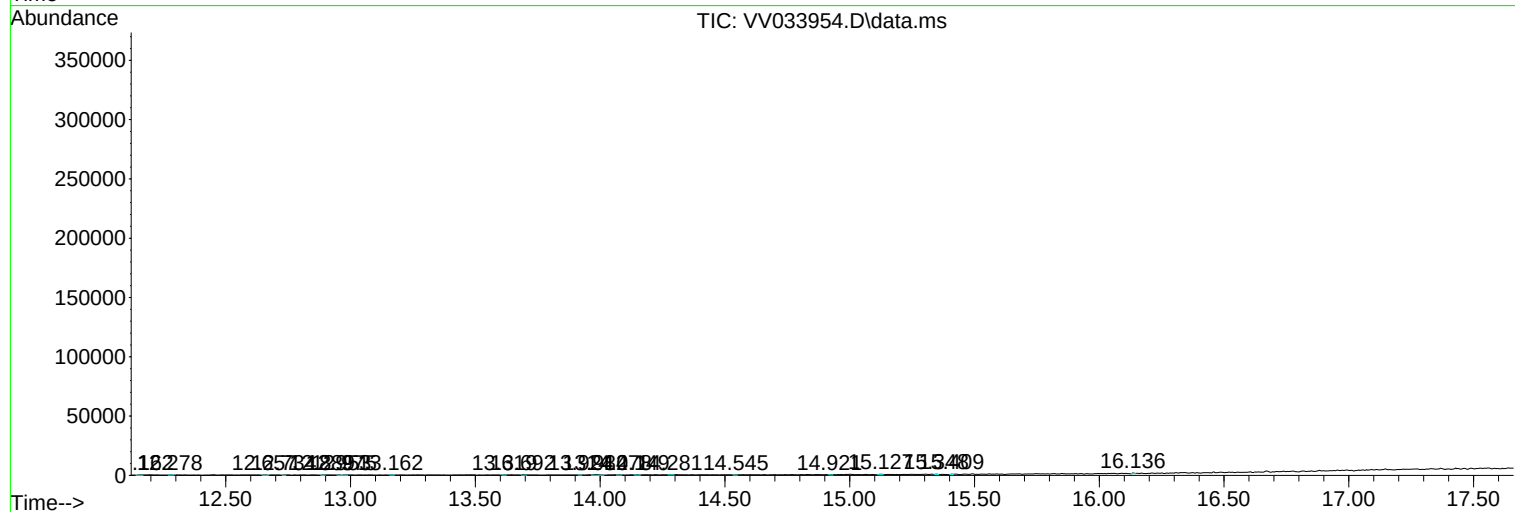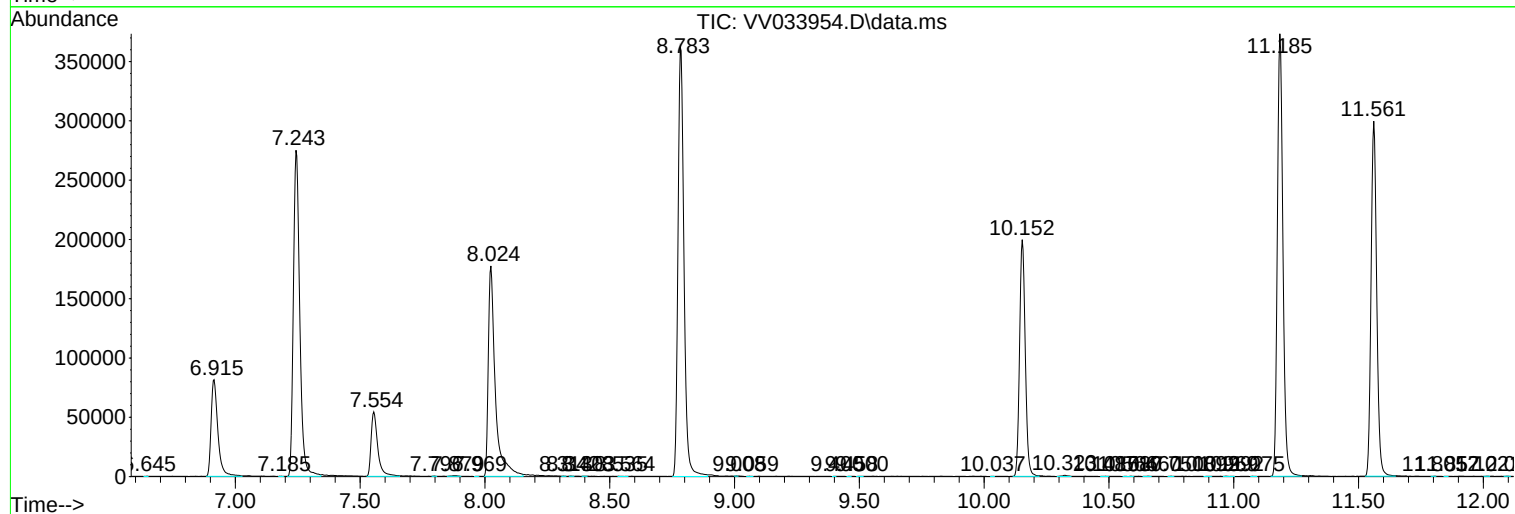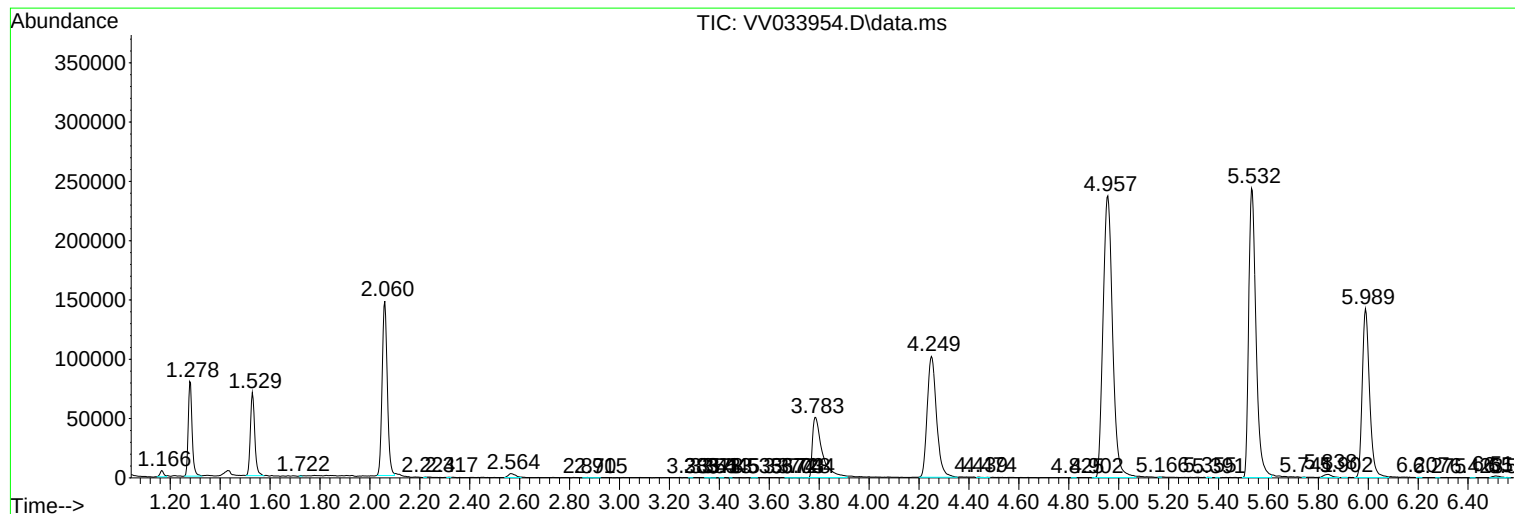

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033954.D
Acq On : 01 Feb 2024 17:26
Operator : SY/MD
Sample : P1300-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033954.D
Acq On : 01 Feb 2024 17:26
Operator : SY/MD
Sample : P1300-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc