
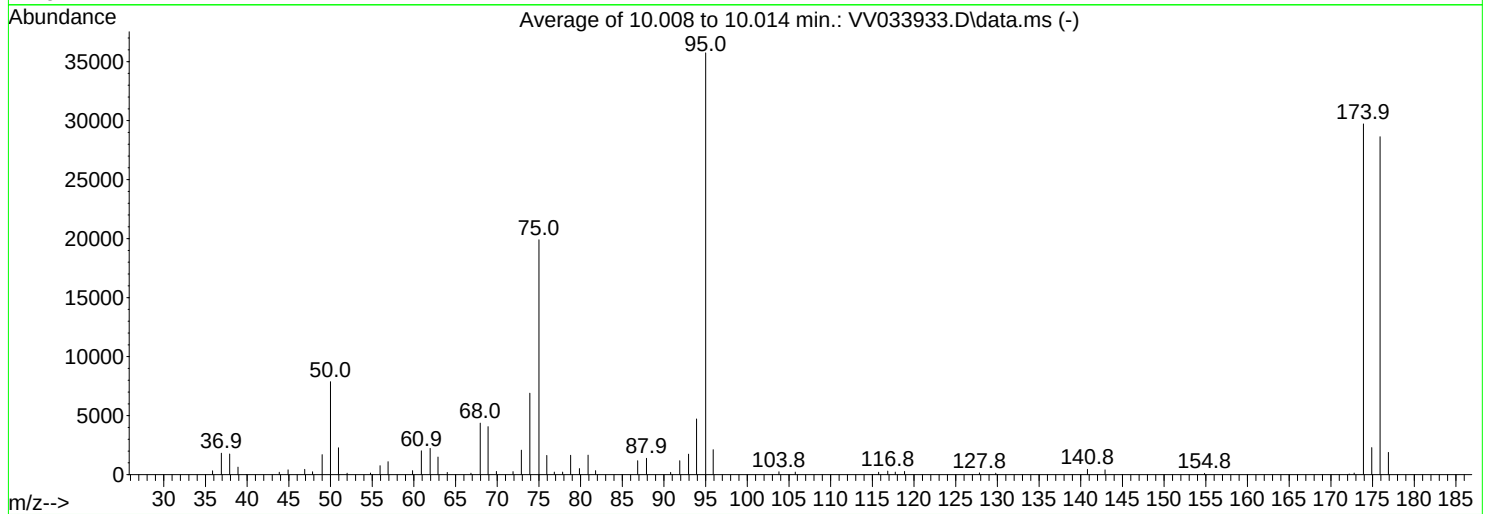


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020124\
Data File : VV033933.D
Acq On : 01 Feb 2024 08:39
Operator : SY/MD
Sample : BFB260
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB260

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Sat Feb 03 01:42:15 2024

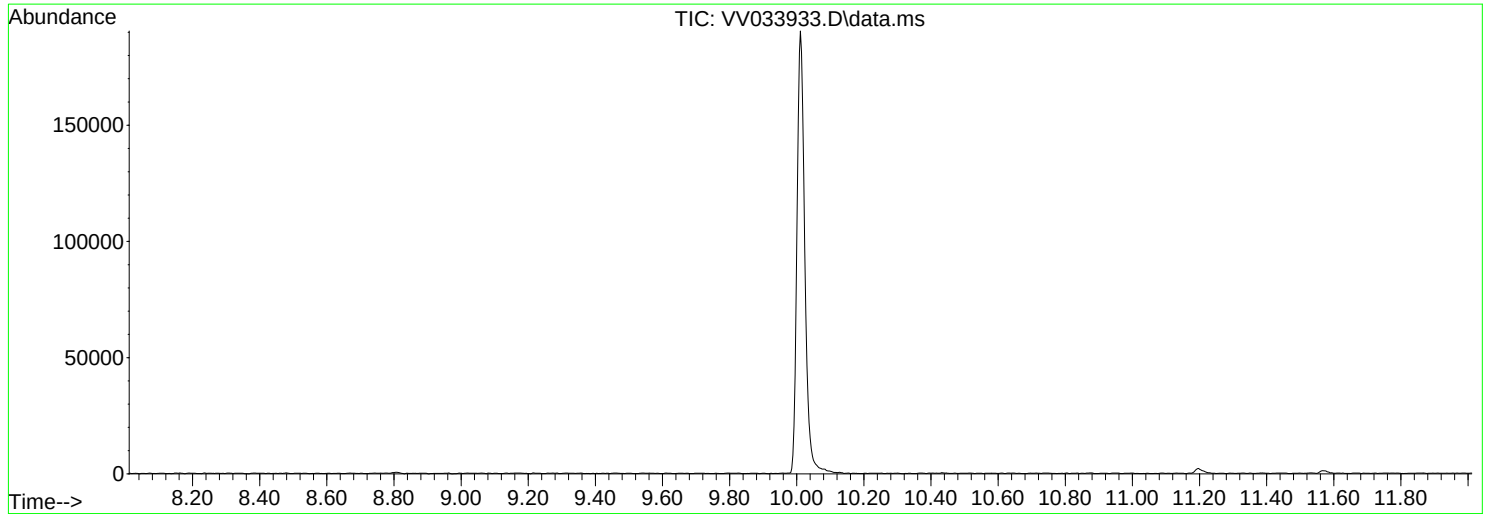

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	7878	PASS
75	95	30	80	55.7	19904	PASS
95	95	100	100	100.0	35744	PASS
96	95	5	9	5.9	2117	PASS
173	174	0.00	2	0.5	136	PASS
174	95	50	120	83.1	29717	PASS
175	174	5	9	7.7	2292	PASS
176	174	95	105	96.4	28637	PASS
177	176	5	10	6.6	1888	PASS

m/z	Abundance
39.90	131.0
43.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.90	330.0
36.90	1795.0
37.90	1717.0
38.90	690.0
40.00	152.0
43.90	435.0
44.90	390.0
46.90	481.0
47.80	217.0
49.00	1647.0
50.00	7963.0
51.00	2264.0
52.00	126.0
54.80	120.0
55.90	733.0
56.90	1147.0
59.90	338.0
60.90	2130.0
61.90	2290.0
62.90	1525.0
64.00	210.0
66.90	106.0
67.90	4381.0
68.90	3977.0
69.90	265.0
71.90	238.0
72.90	2057.0
73.90	6904.0
75.00	19664.0
76.00	1599.0
76.90	244.0
77.80	224.0
78.80	1640.0
79.80	491.0
80.90	1723.0
81.80	322.0
86.90	1171.0
87.90	1398.0
90.80	205.0
91.90	1303.0
92.90	1578.0
93.90	4748.0
95.00	34744.0
95.90	2161.0
103.80	238.0
105.80	185.0
115.70	182.0
116.80	258.0
117.70	230.0
118.80	245.0
127.90	116.0
129.80	137.0
140.70	424.0
142.90	382.0
154.90	101.0
172.80	407.0
173.90	28568.0
174.90	2351.0
175.90	27672.0
176.90	1840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.90	330.0
36.90	1835.0
37.90	1813.0
38.90	654.0
39.90	151.0
43.90	421.0
44.90	418.0
46.90	476.0
47.90	250.0
49.00	1731.0
50.00	8266.0
51.00	2356.0
52.00	127.0
54.80	142.0
55.90	799.0
56.90	1113.0
59.90	351.0
60.90	2074.0
61.90	2321.0
62.90	1534.0
64.00	188.0
66.90	128.0
68.00	4544.0
68.90	4199.0
69.90	287.0
71.90	259.0
72.90	2177.0
73.90	7084.0
75.00	20520.0
76.00	1718.0
76.90	219.0
77.80	252.0
78.80	1720.0
79.90	543.0
80.90	1704.0
81.80	347.0
86.80	1203.0
87.90	1397.0
90.80	197.0
91.90	1195.0
92.90	1799.0
93.90	4859.0
95.00	37016.0
95.90	2147.0
103.80	265.0
105.70	234.0
115.80	224.0
116.90	323.0
117.70	219.0
118.90	280.0
127.90	165.0
129.80	136.0
140.80	444.0
142.90	406.0
154.80	118.0
173.90	30800.0
174.90	2368.0
175.90	29736.0
176.90	1953.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.90	300.0
36.90	1826.0
37.90	1704.0
38.90	588.0
39.90	146.0
43.90	364.0
44.90	405.0
46.90	401.0
47.90	266.0
49.00	1721.0
50.00	7404.0
50.90	2232.0
52.00	110.0
54.80	148.0
56.00	730.0
56.90	1041.0
59.80	348.0
60.90	1874.0
62.00	2080.0
62.90	1422.0
64.00	161.0
66.80	120.0
68.00	4190.0
68.90	4040.0
69.90	279.0
71.90	276.0
72.90	2000.0
73.90	6716.0
75.00	19528.0
75.90	1579.0
76.80	180.0
77.90	197.0
78.80	1579.0
79.90	502.0
80.90	1537.0
81.80	353.0
86.90	1170.0
87.90	1378.0
90.80	178.0
91.90	1042.0
93.00	1836.0
93.90	4535.0
95.00	35472.0
95.90	2044.0
103.80	231.0
105.70	248.0
115.80	211.0
116.90	311.0
117.80	188.0
118.90	283.0
127.80	182.0
129.80	107.0
140.90	481.0
142.90	417.0
154.80	120.0
172.20	182.0
173.90	29784.0
174.90	2158.0
175.90	28504.0
176.90	1871.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260