

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020223\
 Data File : VW030017.D
 Acq On : 02 Feb 2023 12:39
 Operator : SY/MD
 Sample : 01393-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Quant Time: Feb 03 01:12:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 03 01:11:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	231948	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	217882	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	108333	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	79349	4.510	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.200%	
7) Chloroethane-d5	1.561	69	73990	5.073	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.400%	
11) 1,1-Dichloroethene-d2	2.101	63	109804	3.424	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	3.886	46	159764	51.235	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.480%	
24) Chloroform-d	4.333	84	142513	4.416	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	5.021	65	62807	4.595	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.000%	
32) Benzene-d6	5.037	84	298633	4.621	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	6.059	67	94579	5.000	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.304	98	250725	4.190	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.612	79	29628	4.289	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.800%	
46) 2-Hexanone-d5	8.082	63	141474	50.304	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.600%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	66361	4.787	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.800%	
66) 1,2-Dichlorobenzene-d4	11.612	152	92150	4.679	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.600%	
Target Compounds					Qvalue	
13) Acetone	2.182	43	14703	6.606	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030017.D
Acq On : 02 Feb 2023 12:39
Operator : SY/MD
Sample : 01393-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B60


Quant Time: Feb 03 01:12:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 03 01:11:57 2023
Response via : Initial Calibration

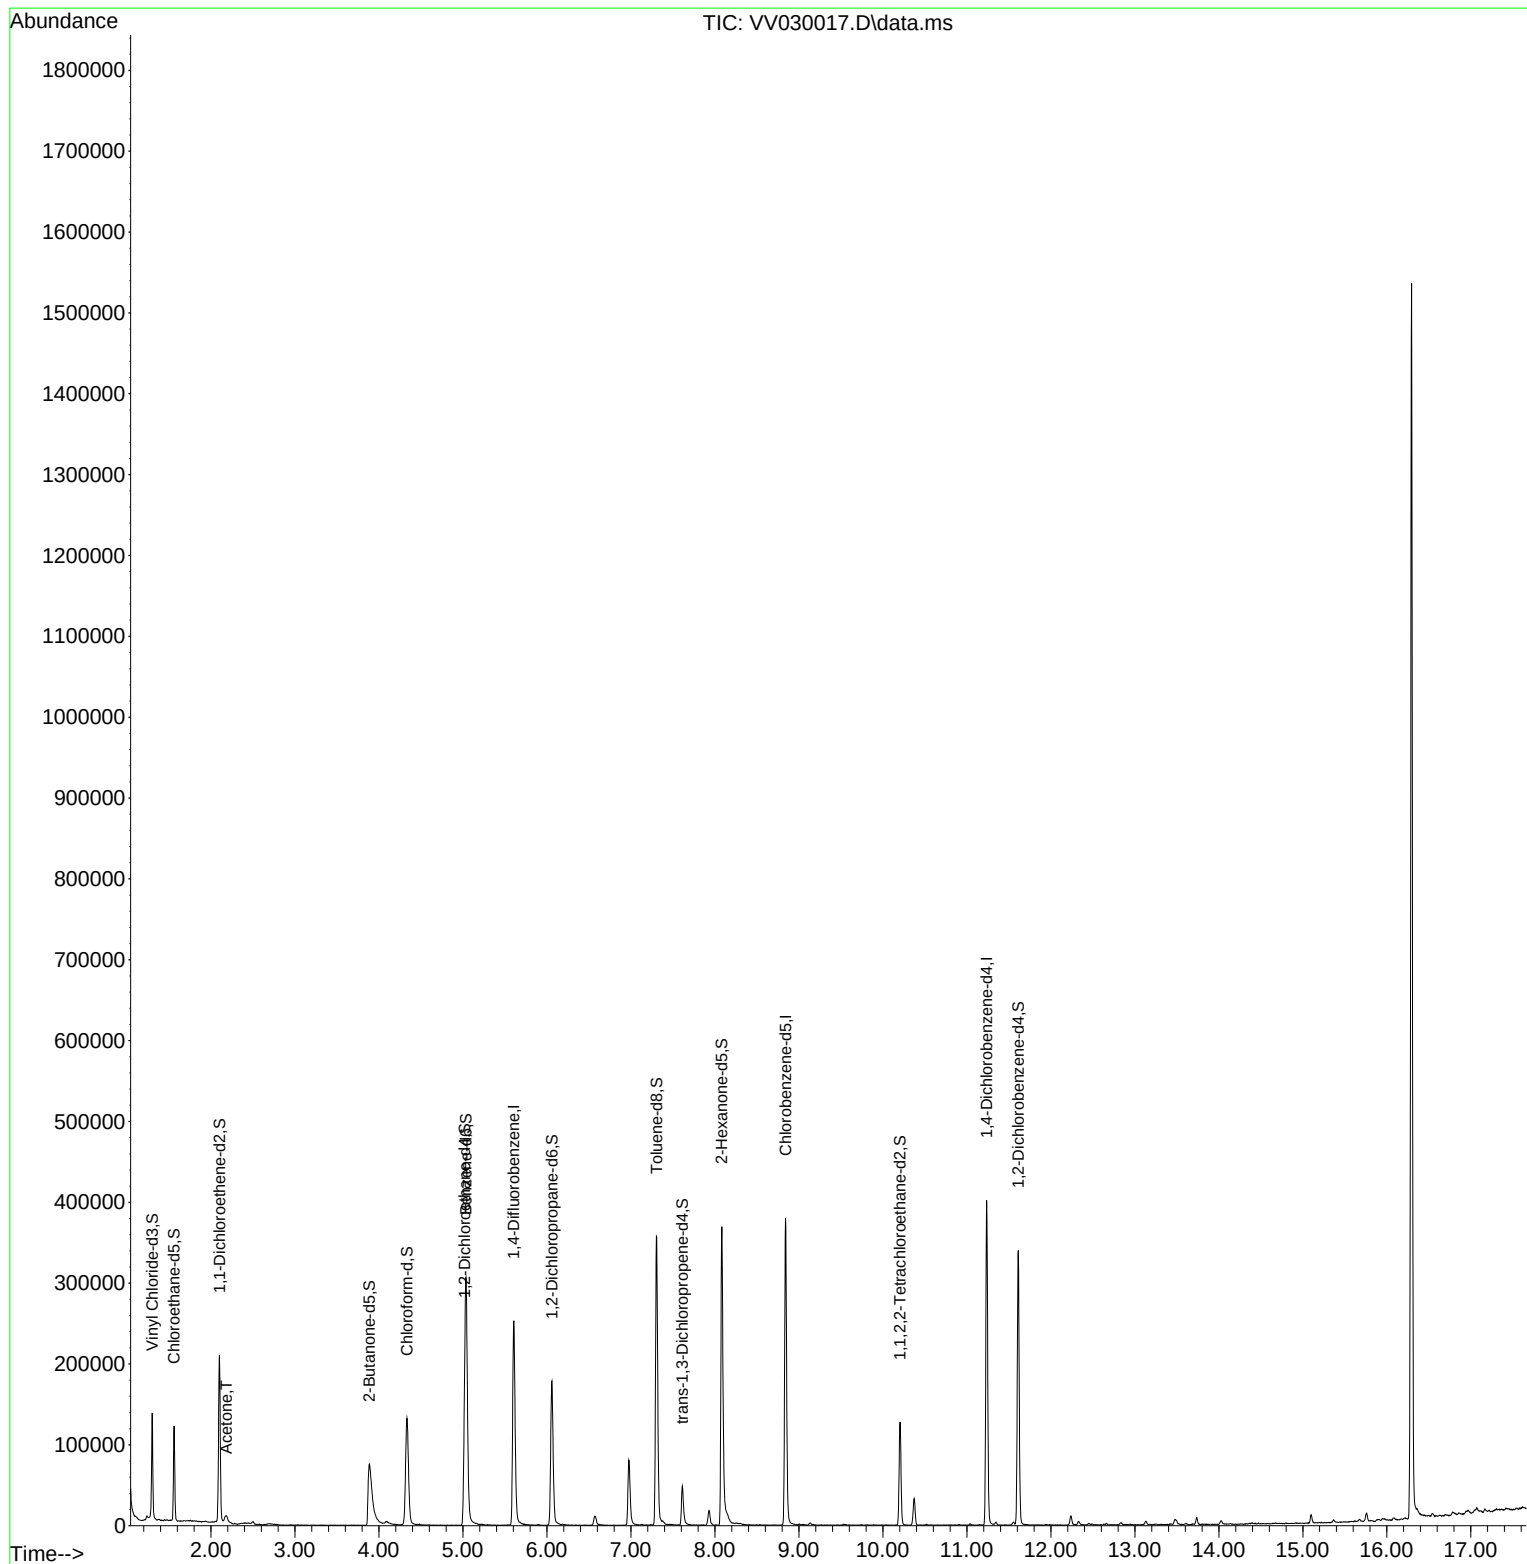

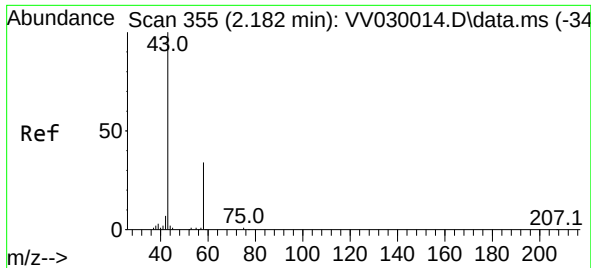

#13
 Acetone
 Concen: 6.606 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV030017.D
 Acq: 02 Feb 2023 12:39

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

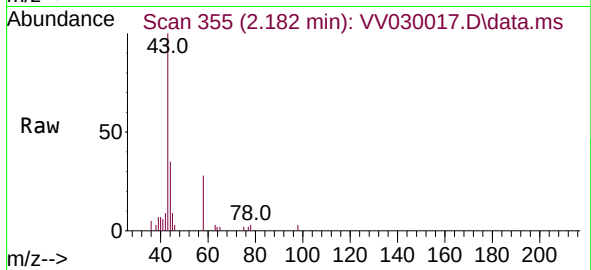

Tgt Ion: 43 Resp: 14703
 Ion Ratio Lower Upper
 43 100
 58 36.1 0.0 68.8

