

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020223\
 Data File : VW030019.D
 Acq On : 02 Feb 2023 13:26
 Operator : SY/MD
 Sample : 01393-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59

Quant Time: Feb 03 01:13:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 03 01:11:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	255642	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	238919	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	117996	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	80715	4.163	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.200%
7) Chloroethane-d5	1.564	69	76599	4.766	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.400%
11) 1,1-Dichloroethene-d2	2.105	63	111586	3.157	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	3.889	46	167618	48.772	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.540%
24) Chloroform-d	4.336	84	146913	4.130	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	5.021	65	64429	4.277	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
32) Benzene-d6	5.040	84	311365	4.393	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	6.059	67	100808	4.860	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.307	98	262857	4.006	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	7.616	79	31958	4.219	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%
46) 2-Hexanone-d5	8.082	63	147203	47.732	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.460%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	67377	4.433	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	96595	4.503	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.000%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	27811	11.338	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030019.D
Acq On : 02 Feb 2023 13:26
Operator : SY/MD
Sample : 01393-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59


Quant Time: Feb 03 01:13:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 03 01:11:57 2023
Response via : Initial Calibration

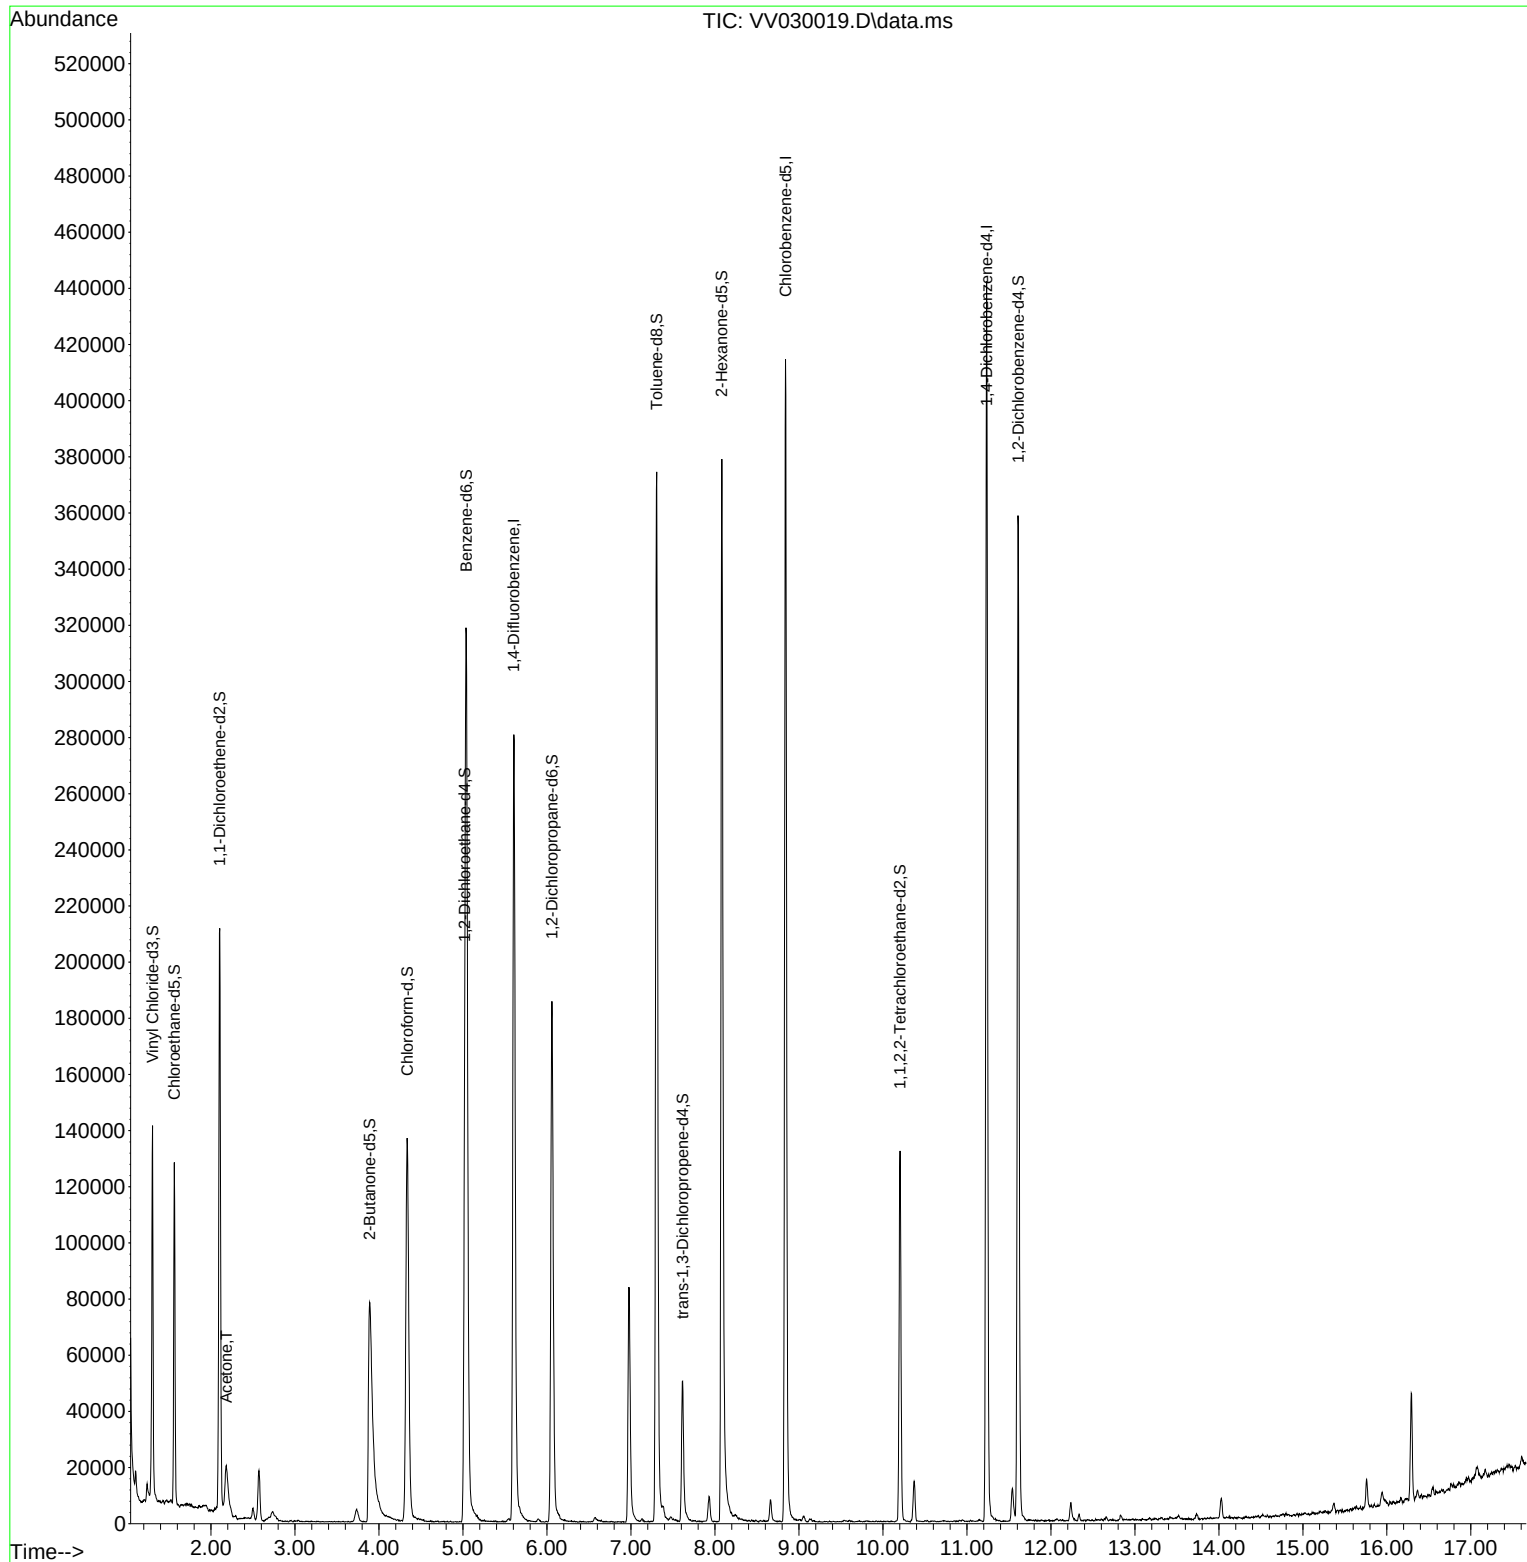

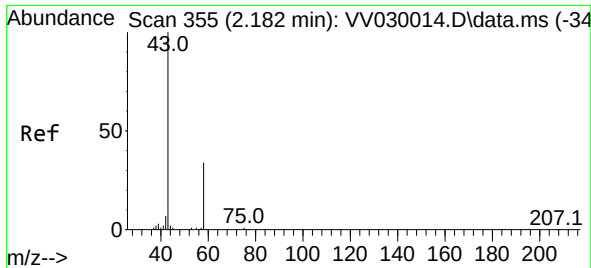

#13
 Acetone
 Concen: 11.338 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV030019.D
 Acq: 02 Feb 2023 13:26

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59

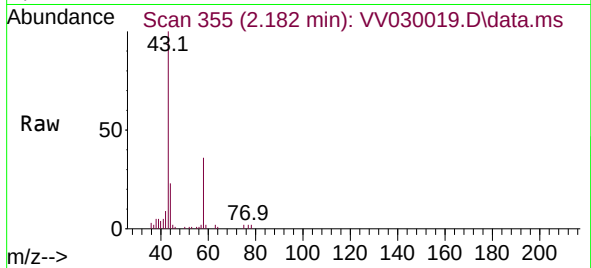

Tgt Ion: 43 Resp: 27811
 Ion Ratio Lower Upper
 43 100
 58 37.1 0.0 68.8

