

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020223\
 Data File : VW030022.D
 Acq On : 02 Feb 2023 14:45
 Operator : SY/MD
 Sample : 01393-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Quant Time: Feb 03 01:14:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 03 01:11:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	229102	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	214052	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	104472	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	82915	4.772	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.400%
7) Chloroethane-d5	1.564	69	77371	5.371	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.400%
11) 1,1-Dichloroethene-d2	2.105	63	111810	3.530	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	3.886	46	171661	55.735	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.460%
24) Chloroform-d	4.336	84	151391	4.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.021	65	67084	4.969	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.040	84	317514	5.001	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
36) 1,2-Dichloropropane-d6	6.059	67	101252	5.449	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.000%
41) Toluene-d8	7.307	98	269449	4.584	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	7.612	79	31658	4.665	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.200%
46) 2-Hexanone-d5	8.082	63	150134	54.338	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.680%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	69658	5.115	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%
66) 1,2-Dichlorobenzene-d4	11.612	152	94708	4.986	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	13192	6.001	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030022.D
Acq On : 02 Feb 2023 14:45
Operator : SY/MD
Sample : 01393-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Time: Feb 03 01:14:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 03 01:11:57 2023
Response via : Initial Calibration

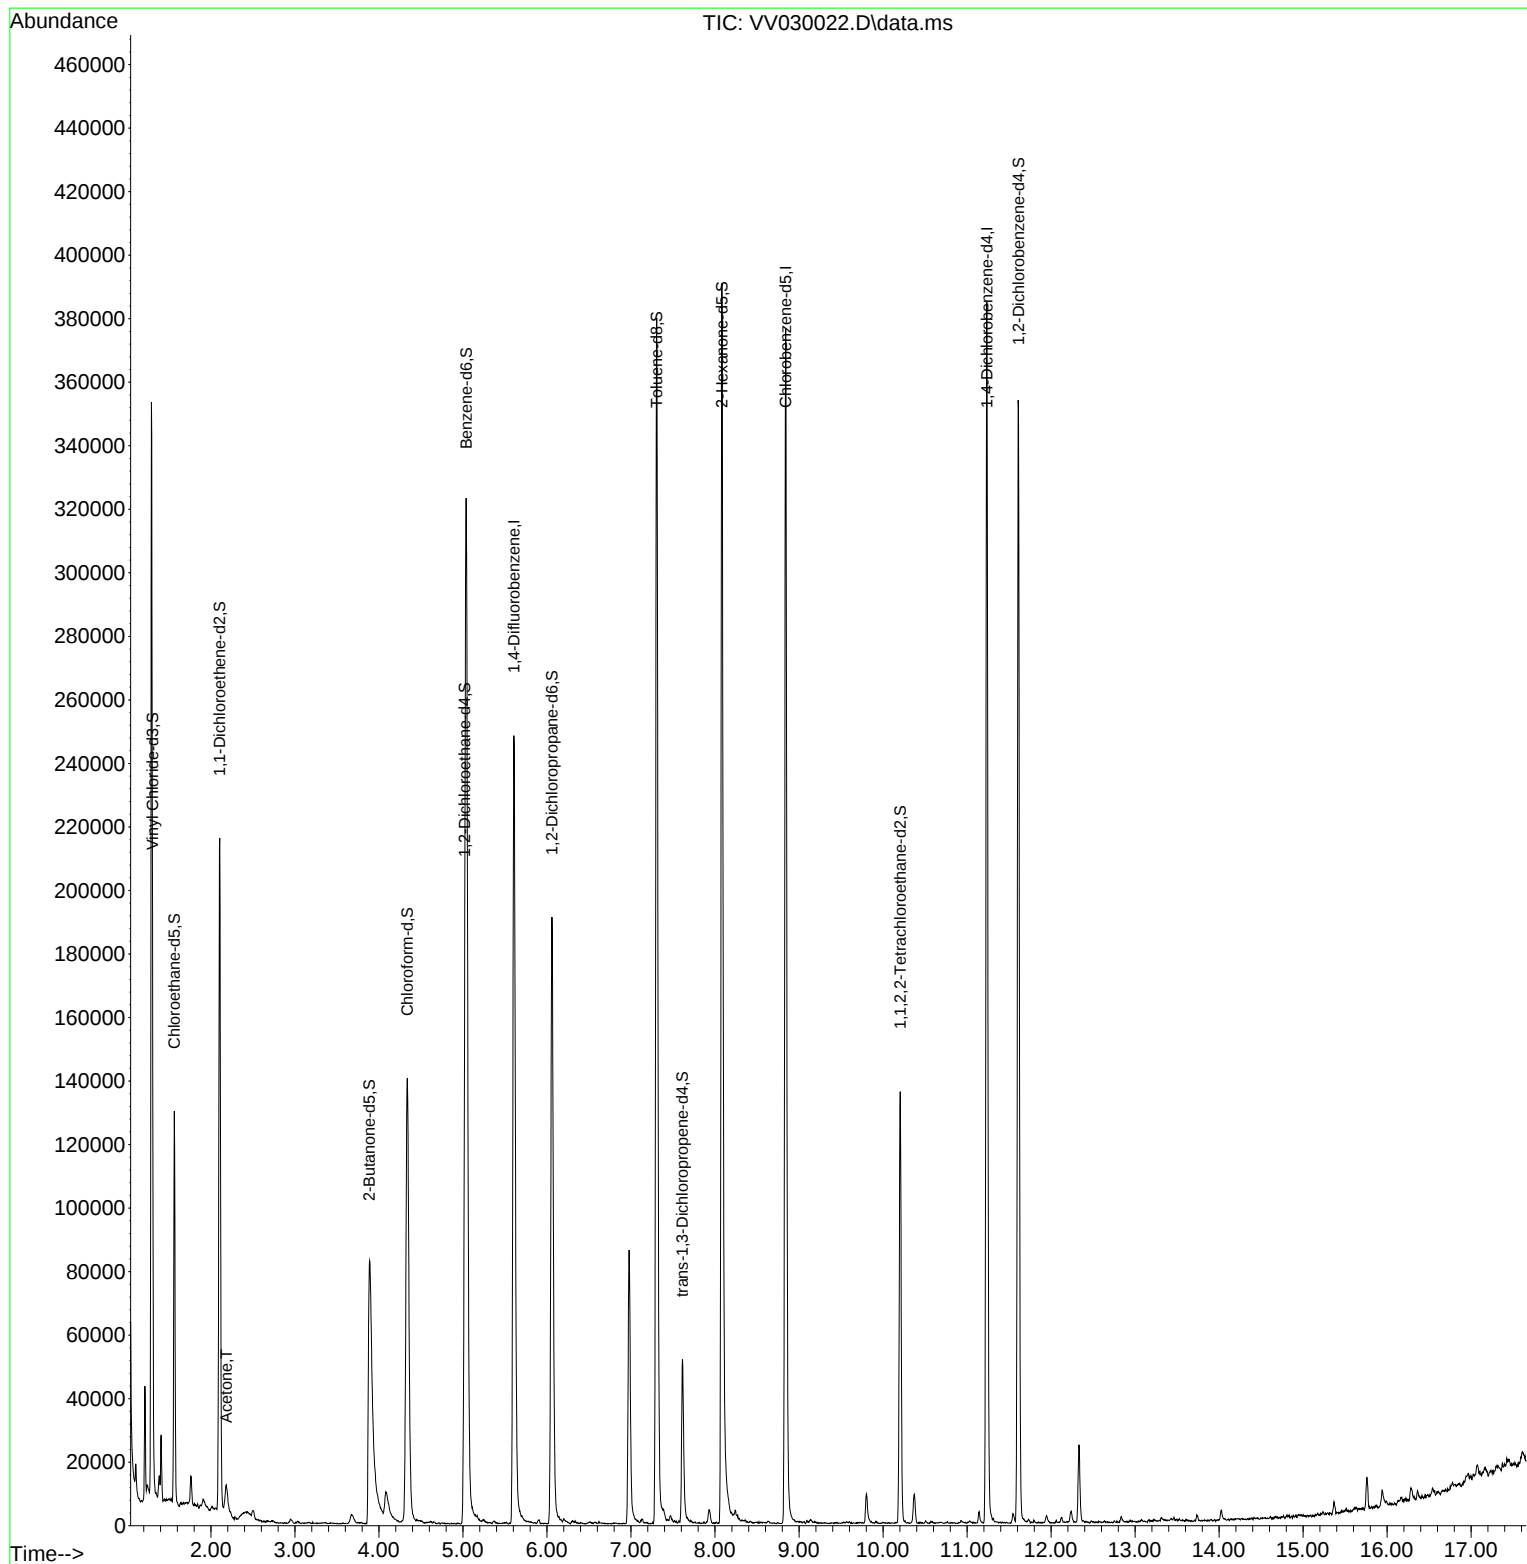

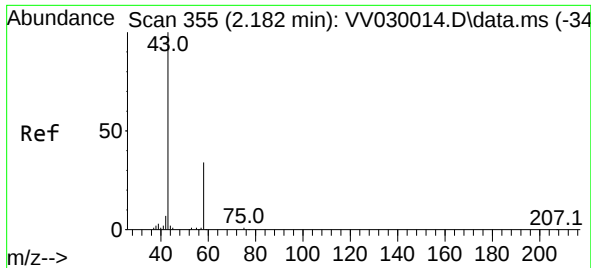

#13
 Acetone
 Concen: 6.001 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV030022.D
 Acq: 02 Feb 2023 14:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Tgt Ion: 43 Resp: 13192
 Ion Ratio Lower Upper
 43 100
 58 41.4 0.0 68.8

