

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
 Data File : VV030015.D
 Acq On : 02 Feb 2023 11:26
 Operator : SY/MD
 Sample : VV0202WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK301

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	73	81	96	rVB	137192	151790	17.97%	2.238%
2	1.564	155	163	176	rVB	129985	145665	17.25%	2.148%
3	2.101	320	330	345	rVB	225227	320247	37.92%	4.722%
4	2.500	443	454	468	rBV	35432	59703	7.07%	0.880%
5	3.892	875	887	937	rBV	73276	280491	33.21%	4.136%
6	4.336	1008	1025	1050	rBV	142485	355156	42.05%	5.236%
7	5.037	1226	1243	1273	rBV2	337881	844579	100.00%	12.453%
8	5.606	1406	1420	1447	rBV	246976	505177	59.81%	7.448%
9	6.059	1547	1561	1578	rBV	194880	397828	47.10%	5.866%
10	6.976	1834	1846	1861	rBV	87821	162510	19.24%	2.396%
11	7.307	1935	1949	1973	rBV	396638	700922	82.99%	10.334%
12	7.612	2033	2044	2066	rBV2	51832	95861	11.35%	1.413%
13	8.082	2179	2190	2233	rBV	386101	708130	83.84%	10.441%
14	8.413	2283	2293	2305	rVB2	5955	9508	1.13%	0.140%
15	8.841	2415	2426	2455	rBV	365183	607875	71.97%	8.963%
16	10.204	2839	2850	2867	rVB	140353	219613	26.00%	3.238%
17	11.236	3159	3171	3191	rBV	394364	605188	71.66%	8.923%
18	11.612	3275	3288	3310	rBV	373744	589397	69.79%	8.690%
19	14.027	4028	4039	4048	rBV2	5072	9080	1.08%	0.134%
20	15.760	4570	4578	4587	rVB7	9178	13634	1.61%	0.201%




Sum of corrected areas: 6782354

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030015.D
Acq On : 02 Feb 2023 11:26
Operator : SY/MD
Sample : VV0202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

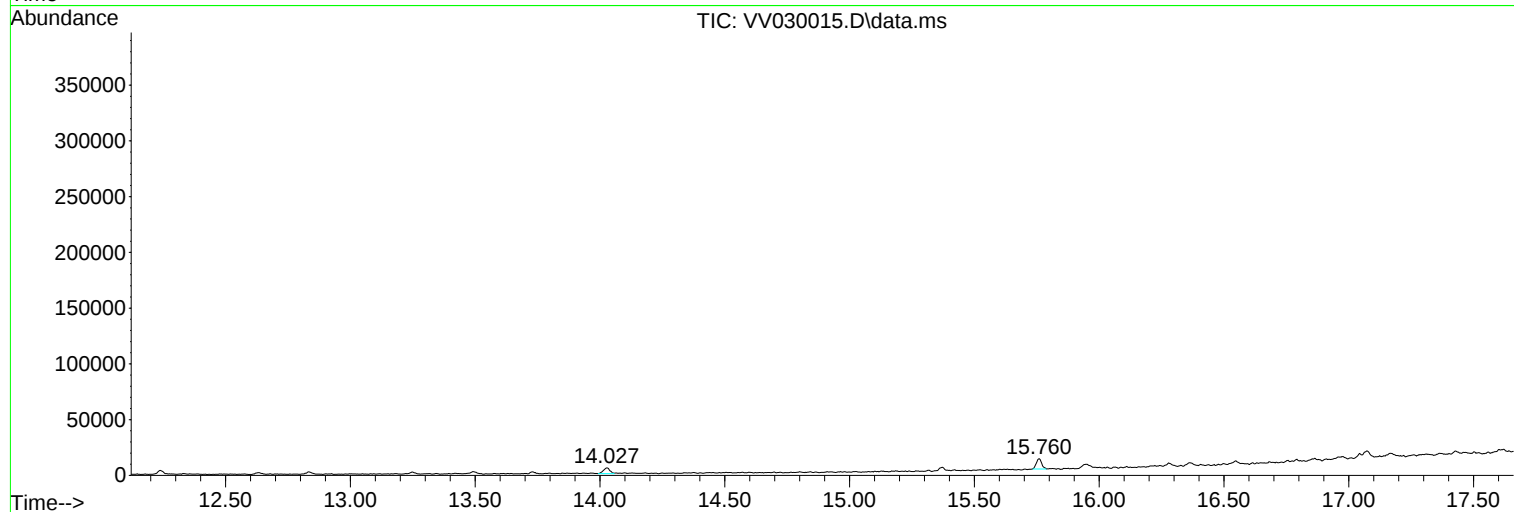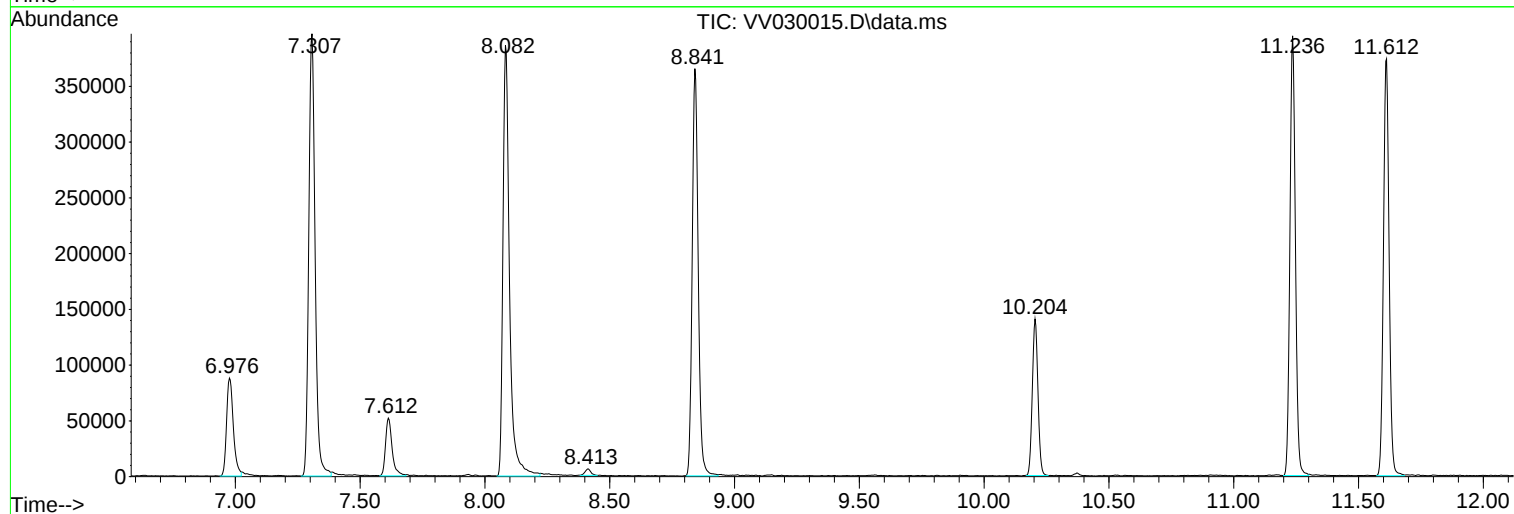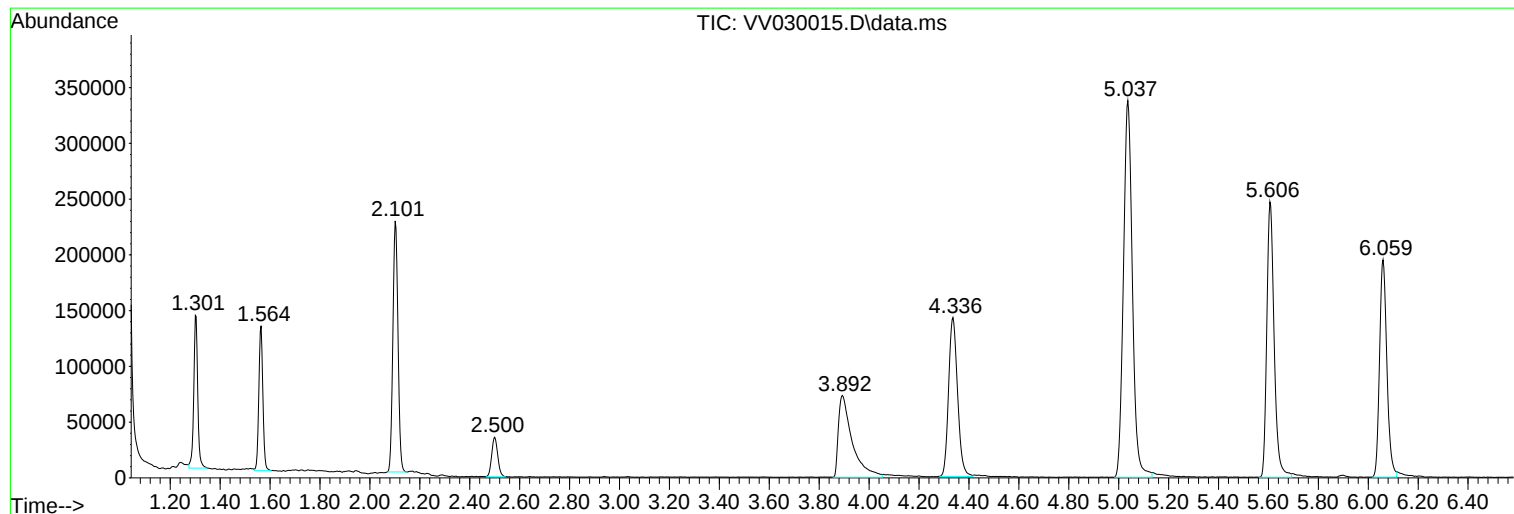

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030015.D
Acq On : 02 Feb 2023 11:26
Operator : SY/MD
Sample : VV0202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030015.D
Acq On : 02 Feb 2023 11:26
Operator : SY/MD
Sample : VV0202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------