

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
 Data File : VV030019.D
 Acq On : 02 Feb 2023 13:26
 Operator : SY/MD
 Sample : 01393-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.101	16	19	29	rVB3	9076	10166	1.26%	0.145%
2	1.240	57	62	71	rBV2	6074	9157	1.14%	0.131%
3	1.304	72	82	100	rVB	133916	153971	19.15%	2.197%
4	1.564	155	163	174	rVB	122055	135434	16.84%	1.933%
5	2.105	320	331	343	rBV	206586	298076	37.07%	4.253%
6	2.182	346	355	380	rVB2	18293	53294	6.63%	0.760%
7	2.571	464	476	489	rVB	17797	32232	4.01%	0.460%
8	3.735	822	838	857	rVB3	4459	11439	1.42%	0.163%
9	3.889	874	886	934	rBV	78218	293918	36.55%	4.194%
10	4.336	1008	1025	1047	rBV	136349	338624	42.11%	4.832%
11	5.037	1226	1243	1281	rBV2	318494	804086	100.00%	11.474%
12	5.606	1407	1420	1461	rBV	279827	569730	70.85%	8.130%
13	6.059	1545	1561	1587	rBV	185453	387252	48.16%	5.526%
14	6.976	1835	1846	1877	rBV	83711	159664	19.86%	2.278%
15	7.307	1934	1949	1968	rBV	373799	661709	82.29%	9.442%
16	7.616	2033	2045	2069	rBV	50021	93413	11.62%	1.333%
17	7.931	2133	2143	2158	rVB2	9064	16924	2.10%	0.241%
18	8.082	2177	2190	2225	rBV	378492	684357	85.11%	9.765%
19	8.664	2361	2371	2388	rVB3	7678	12682	1.58%	0.181%
20	8.841	2411	2426	2447	rBV	414039	682656	84.90%	9.741%
21	10.204	2837	2850	2864	rBV	131787	206046	25.62%	2.940%
22	10.371	2889	2902	2912	rBV3	14433	24634	3.06%	0.352%
23	11.236	3159	3171	3189	rBV	441643	676781	84.17%	9.657%
24	11.542	3256	3266	3276	rBV4	11588	21597	2.69%	0.308%
25	11.609	3276	3287	3313	rVB	357707	572889	71.25%	8.175%
26	12.239	3472	3483	3494	rBV	6515	11319	1.41%	0.162%
27	14.030	4031	4040	4049	rVB	6995	11374	1.41%	0.162%
28	15.760	4570	4578	4588	rBV6	9850	14265	1.77%	0.204%
29	16.291	4734	4743	4755	rVB2	38247	60301	7.50%	0.860%




Sum of corrected areas: 7007990

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030019.D
Acq On : 02 Feb 2023 13:26
Operator : SY/MD
Sample : 01393-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

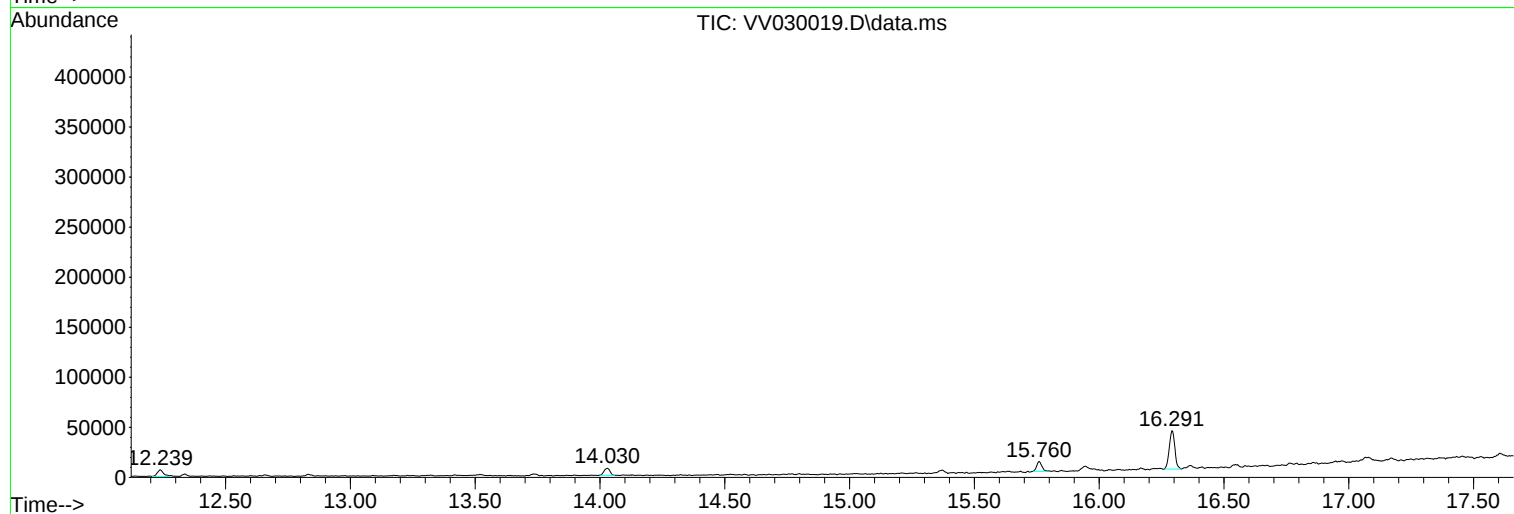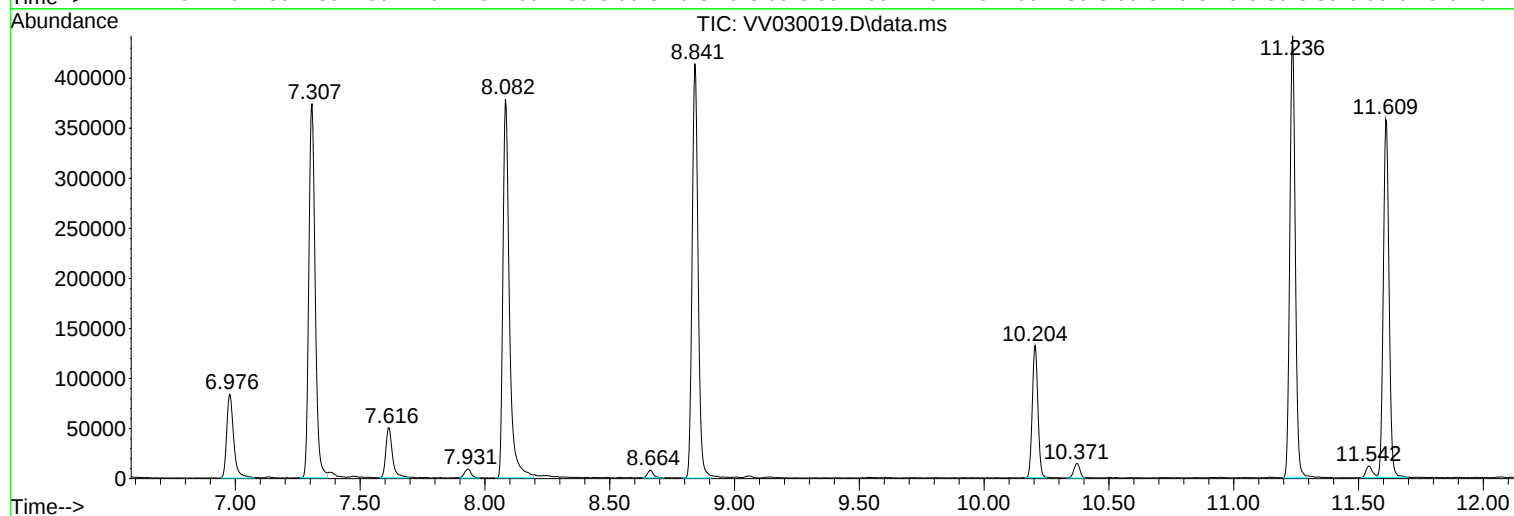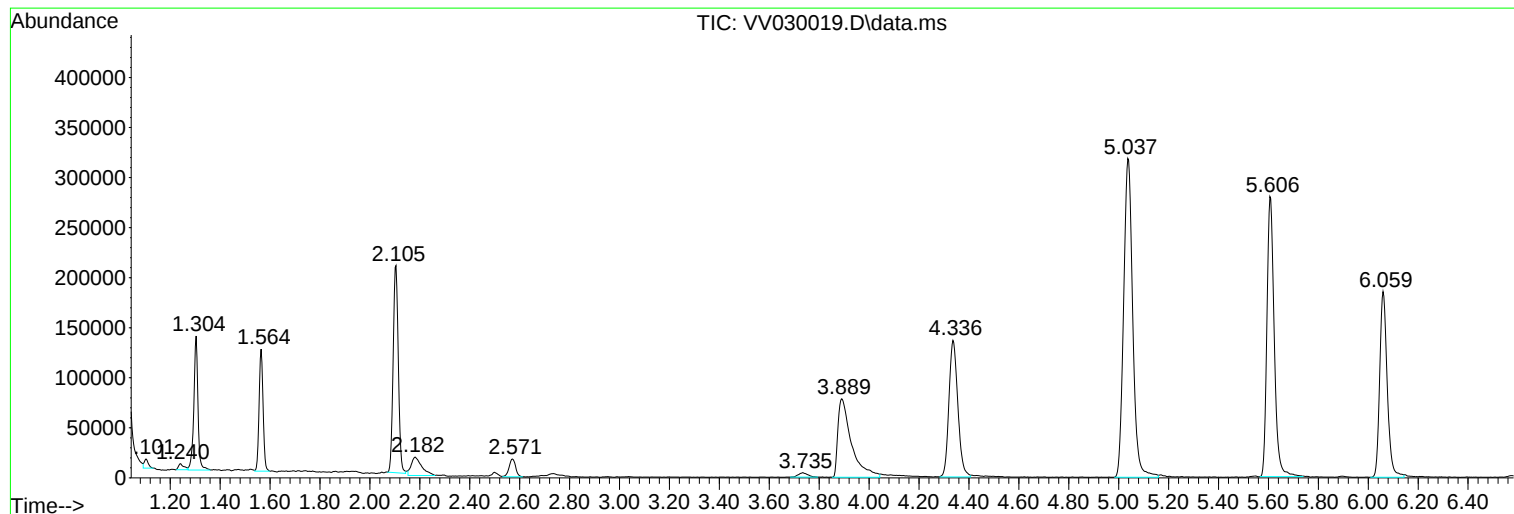

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030019.D
Acq On : 02 Feb 2023 13:26
Operator : SY/MD
Sample : 01393-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030019.D
Acq On : 02 Feb 2023 13:26
Operator : SY/MD
Sample : 01393-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------