

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
 Data File : VV030022.D
 Acq On : 02 Feb 2023 14:45
 Operator : SY/MD
 Sample : 01393-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	31	rVB2	10913	11406	1.40%	0.160%
2	1.214	48	54	59	rBV	35796	31913	3.91%	0.449%
3	1.291	71	78	94	rVB2	343489	442281	54.26%	6.223%
4	1.384	101	107	110	rBV	6872	8265	1.01%	0.116%
5	1.407	110	114	121	rVB	20892	18868	2.31%	0.265%
6	1.564	155	163	181	rVB	124523	140968	17.29%	1.983%
7	1.761	219	224	234	rVB2	9215	11808	1.45%	0.166%
8	2.105	320	331	345	rBV	211561	304353	37.34%	4.282%
9	2.182	346	355	379	rVB3	10448	29062	3.57%	0.409%
10	3.674	806	819	839	rBV3	2849	8578	1.05%	0.121%
11	3.889	875	886	926	rBV	82737	297815	36.53%	4.190%
12	4.082	937	946	971	rVB3	7945	24348	2.99%	0.343%
13	4.336	1008	1025	1057	rVB2	139343	351997	43.18%	4.952%
14	5.037	1222	1243	1276	rBV2	323065	815170	100.00%	11.469%
15	5.606	1406	1420	1447	rBV	248112	510301	62.60%	7.180%
16	6.059	1547	1561	1584	rBV	190922	390771	47.94%	5.498%
17	6.979	1834	1847	1869	rBV	86148	159970	19.62%	2.251%
18	7.307	1936	1949	1971	rBV	379539	674045	82.69%	9.483%
19	7.612	2034	2044	2061	rBV	51264	89738	11.01%	1.263%
20	7.931	2129	2143	2157	rVB3	4435	8621	1.06%	0.121%
21	8.082	2179	2190	2223	rBV	390366	700378	85.92%	9.854%
22	8.841	2409	2426	2458	rBV	376353	619338	75.98%	8.714%
23	9.802	2715	2725	2741	rBV5	9240	16776	2.06%	0.236%
24	10.204	2839	2850	2864	rBV	135692	215331	26.42%	3.030%
25	10.371	2885	2902	2913	rBV2	9144	15837	1.94%	0.223%
26	11.236	3159	3171	3192	rBV	384516	592567	72.69%	8.337%
27	11.609	3276	3287	3306	rVV	352979	557247	68.36%	7.840%
28	12.333	3502	3512	3524	rBV2	24392	37361	4.58%	0.526%
29	15.760	4571	4578	4585	rBV4	9298	13215	1.62%	0.186%
30	15.940	4627	4634	4647	rBV10	4880	9258	1.14%	0.130%




Sum of corrected areas: 7107586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030022.D
Acq On : 02 Feb 2023 14:45
Operator : SY/MD
Sample : 01393-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

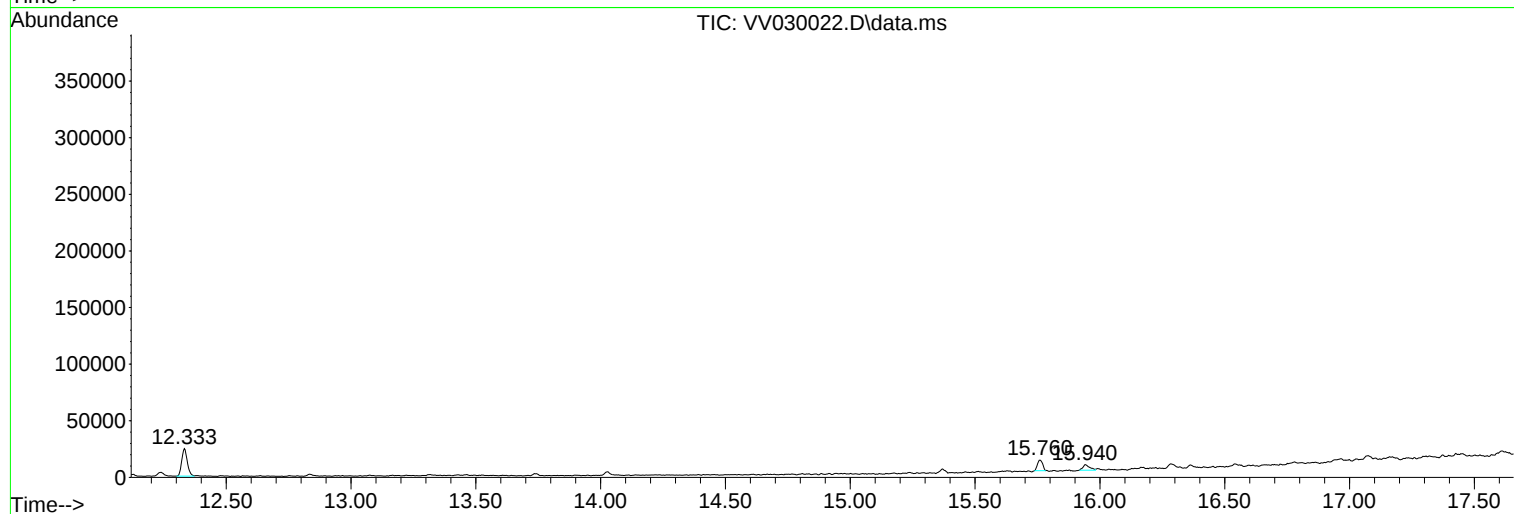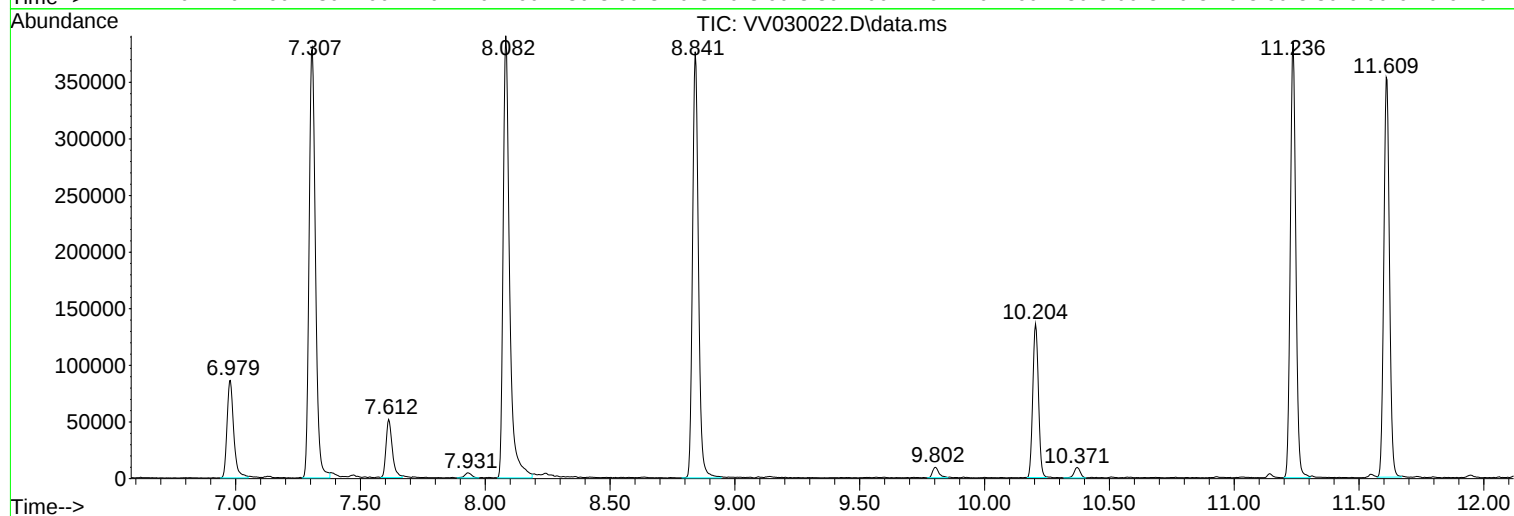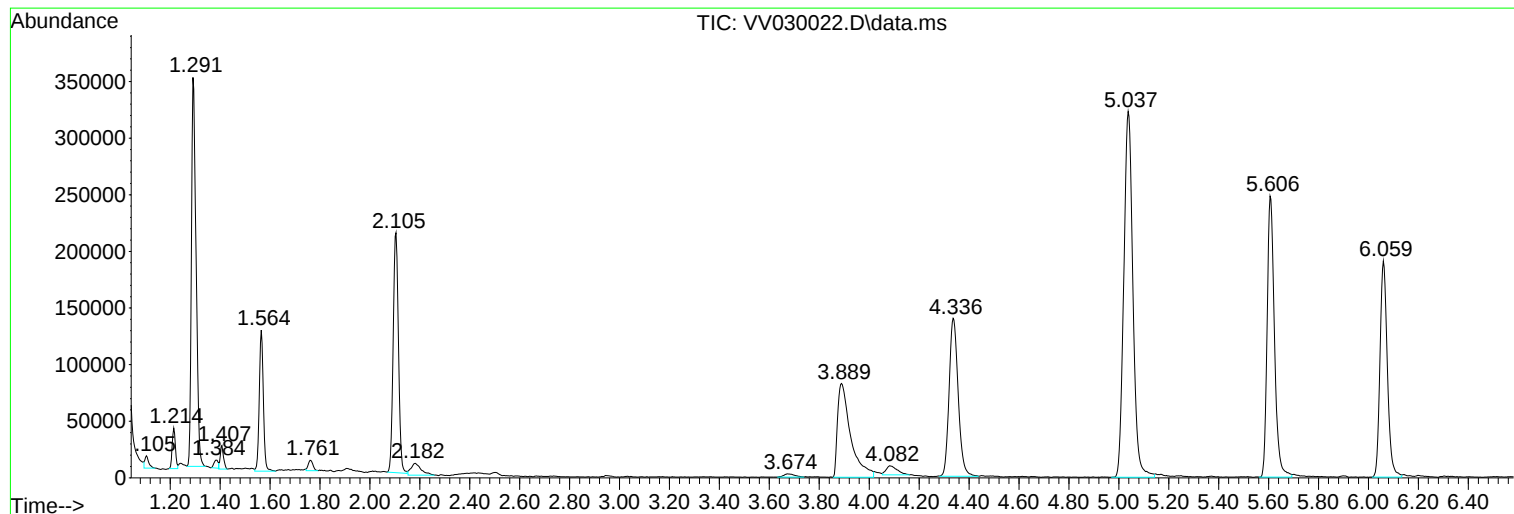

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030022.D
Acq On : 02 Feb 2023 14:45
Operator : SY/MD
Sample : 01393-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030022.D
Acq On : 02 Feb 2023 14:45
Operator : SY/MD
Sample : 01393-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------