

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
 Data File : VV030023.D
 Acq On : 02 Feb 2023 15:08
 Operator : SY/MD
 Sample : 01408-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1156

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	71	rBV3	5517	8836	1.08%	0.130%
2	1.304	73	82	96	rVB	127065	140752	17.20%	2.074%
3	1.564	155	163	177	rVB	121335	136287	16.65%	2.008%
4	2.105	320	331	346	rBV	209031	303006	37.02%	4.465%
5	2.500	445	454	466	rVB2	13851	22785	2.78%	0.336%
6	3.034	609	620	632	rBV2	4788	9826	1.20%	0.145%
7	3.889	874	886	928	rBV	81096	278917	34.08%	4.110%
8	4.339	1006	1026	1050	rBV	141965	365177	44.62%	5.381%
9	5.040	1225	1244	1288	rBV2	318101	818471	100.00%	12.060%
10	5.609	1409	1421	1450	rBV	246267	505100	61.71%	7.443%
11	6.059	1546	1561	1597	rBV	187632	391721	47.86%	5.772%
12	6.979	1831	1847	1877	rBV	83203	159050	19.43%	2.344%
13	7.307	1936	1949	1971	rBV	384520	671198	82.01%	9.890%
14	7.612	2033	2044	2066	rBV	50083	90929	11.11%	1.340%
15	7.934	2131	2144	2154	rBV3	5001	9235	1.13%	0.136%
16	8.082	2179	2190	2229	rBV	382127	688755	84.15%	10.149%
17	8.243	2230	2240	2251	rVB7	4288	8903	1.09%	0.131%
18	8.844	2414	2427	2454	rBV	363419	611372	74.70%	9.009%
19	10.204	2839	2850	2865	rBV	137314	213001	26.02%	3.139%
20	10.374	2891	2903	2918	rVB2	11786	19070	2.33%	0.281%
21	11.143	3131	3142	3150	rBV5	5705	9770	1.19%	0.144%
22	11.236	3157	3171	3189	rBV	397237	610287	74.56%	8.993%
23	11.535	3253	3264	3277	rBV2	22692	44119	5.39%	0.650%
24	11.612	3277	3288	3310	rVB	369760	584885	71.46%	8.618%
25	12.236	3470	3482	3492	rBV3	7116	13284	1.62%	0.196%
26	12.332	3504	3512	3528	rVB3	25508	39941	4.88%	0.589%
27	13.368	3825	3834	3844	rBV	5524	8290	1.01%	0.122%
28	15.760	4568	4578	4587	rBV4	9081	15381	1.88%	0.227%
29	15.943	4628	4635	4644	rBV9	4101	8211	1.00%	0.121%




Sum of corrected areas: 6786559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030023.D
Acq On : 02 Feb 2023 15:08
Operator : SY/MD
Sample : 01408-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1156

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

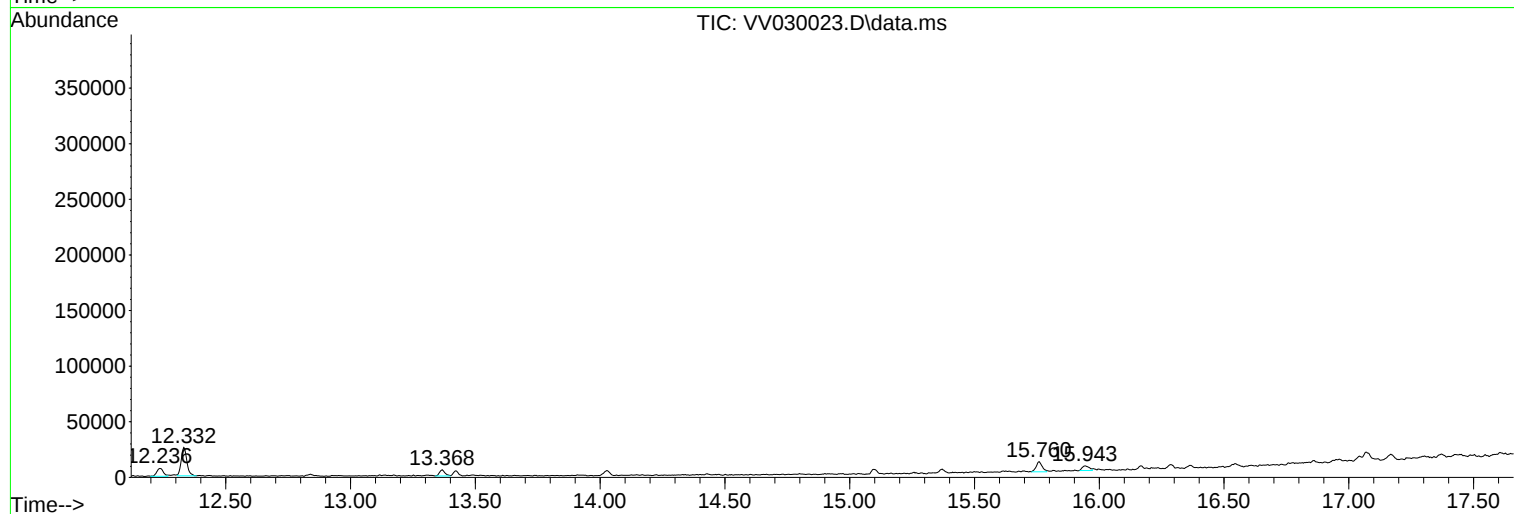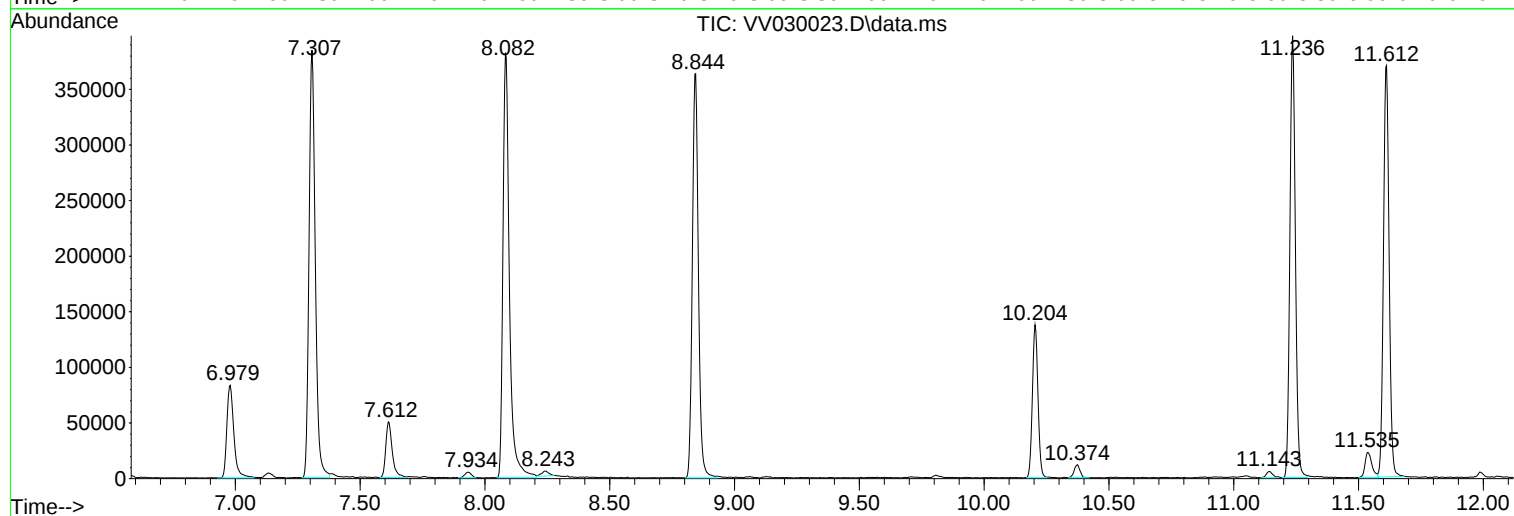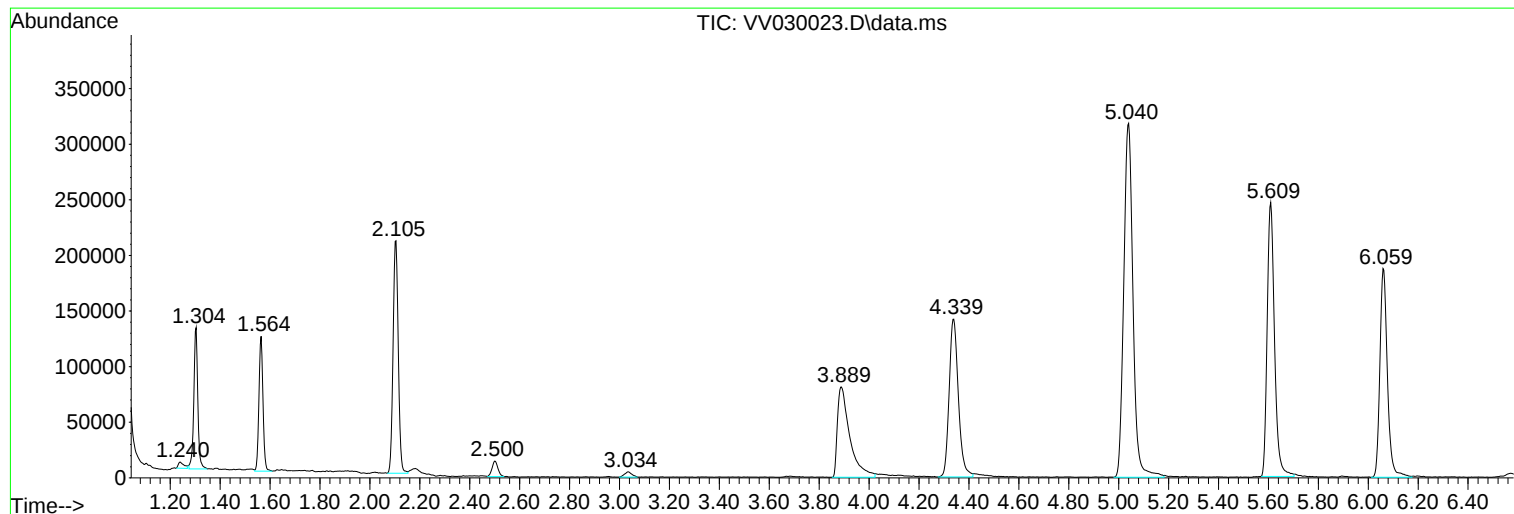

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030023.D
Acq On : 02 Feb 2023 15:08
Operator : SY/MD
Sample : 01408-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1156

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030023.D
Acq On : 02 Feb 2023 15:08
Operator : SY/MD
Sample : 01408-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1156

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
