

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
 Data File : VV030027.D
 Acq On : 02 Feb 2023 16:40
 Operator : SY/MD
 Sample : 01408-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1155

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	99	rVB	121665	135644	17.58%	2.007%
2	1.413	110	116	123	rVB	15229	16808	2.18%	0.249%
3	1.564	156	163	174	rVB	119359	130446	16.90%	1.931%
4	2.105	321	331	345	rBV	199514	285790	37.03%	4.230%
5	2.172	345	352	366	rVB	7258	15456	2.00%	0.229%
6	3.889	871	886	922	rBV	100200	329586	42.71%	4.878%
7	4.342	1006	1027	1052	rBV	133054	330630	42.84%	4.893%
8	5.040	1225	1244	1273	rBV2	308293	771752	100.00%	11.421%
9	5.609	1409	1421	1448	rBV	249237	510704	66.17%	7.558%
10	5.911	1501	1515	1538	rBV	51150	107869	13.98%	1.596%
11	6.063	1549	1562	1580	rBV	179912	366795	47.53%	5.428%
12	6.571	1708	1720	1745	rBV6	15651	36882	4.78%	0.546%
13	6.979	1836	1847	1872	rBV	82469	153896	19.94%	2.278%
14	7.136	1883	1896	1911	rVB	9593	18198	2.36%	0.269%
15	7.310	1937	1950	1968	rBV	357684	635678	82.37%	9.408%
16	7.616	2035	2045	2067	rBV	48493	88162	11.42%	1.305%
17	7.966	2145	2154	2171	rVB2	32982	57727	7.48%	0.854%
18	8.082	2179	2190	2230	rBV	376238	685862	88.87%	10.150%
19	8.844	2411	2427	2455	rBV	375522	625240	81.02%	9.253%
20	9.120	2504	2513	2526	rBV6	6525	12125	1.57%	0.179%
21	10.204	2837	2850	2868	rBV	132787	212006	27.47%	3.138%
22	10.371	2893	2902	2916	rVB2	7183	12164	1.58%	0.180%
23	11.236	3159	3171	3195	rBV	402086	618513	80.14%	9.154%
24	11.538	3255	3265	3277	rBV	18223	33824	4.38%	0.501%
25	11.612	3277	3288	3309	rVB	344337	551130	71.41%	8.156%
26	15.760	4569	4578	4586	rBV5	9409	14176	1.84%	0.210%




Sum of corrected areas: 6757063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030027.D
Acq On : 02 Feb 2023 16:40
Operator : SY/MD
Sample : 01408-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

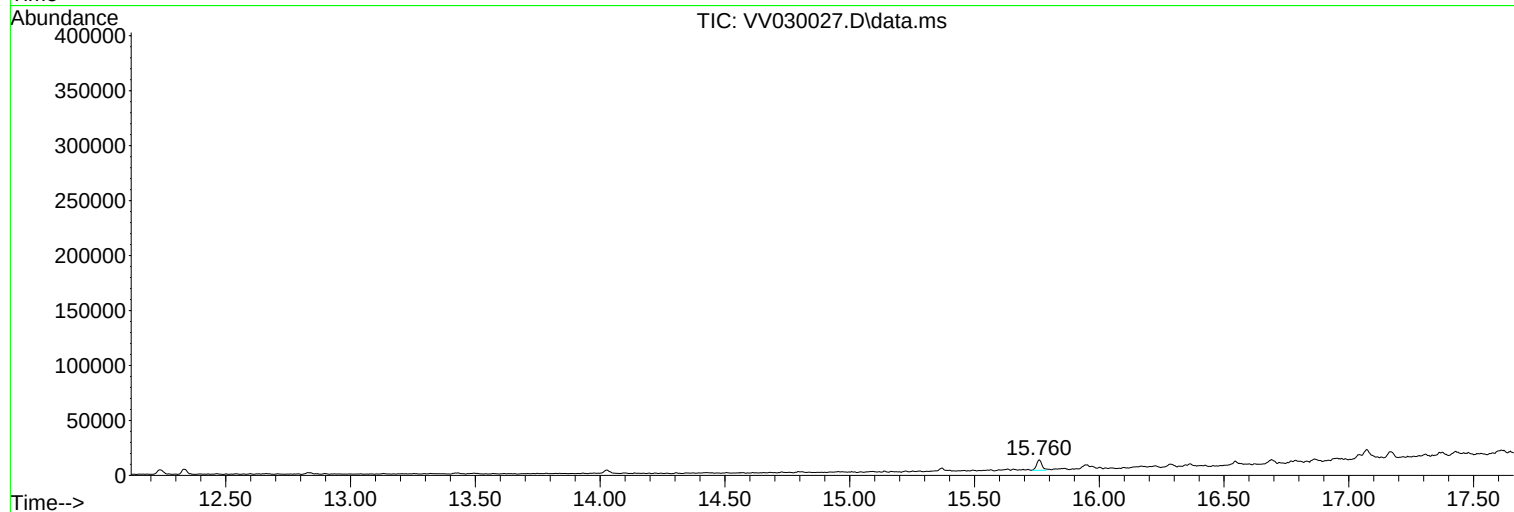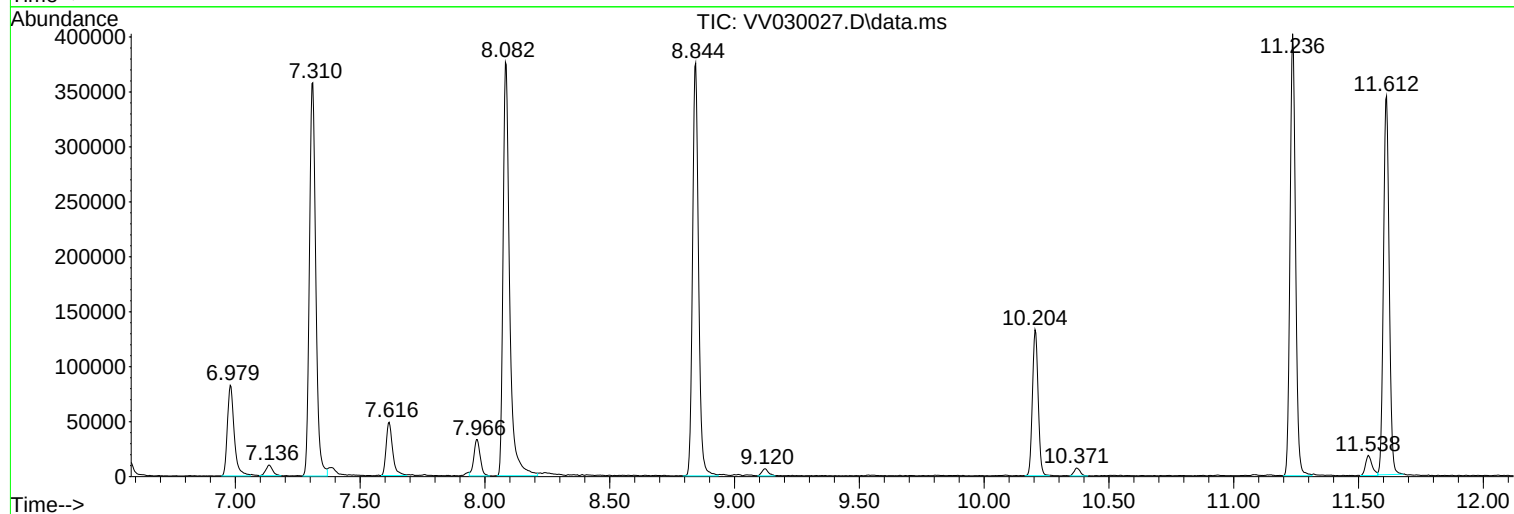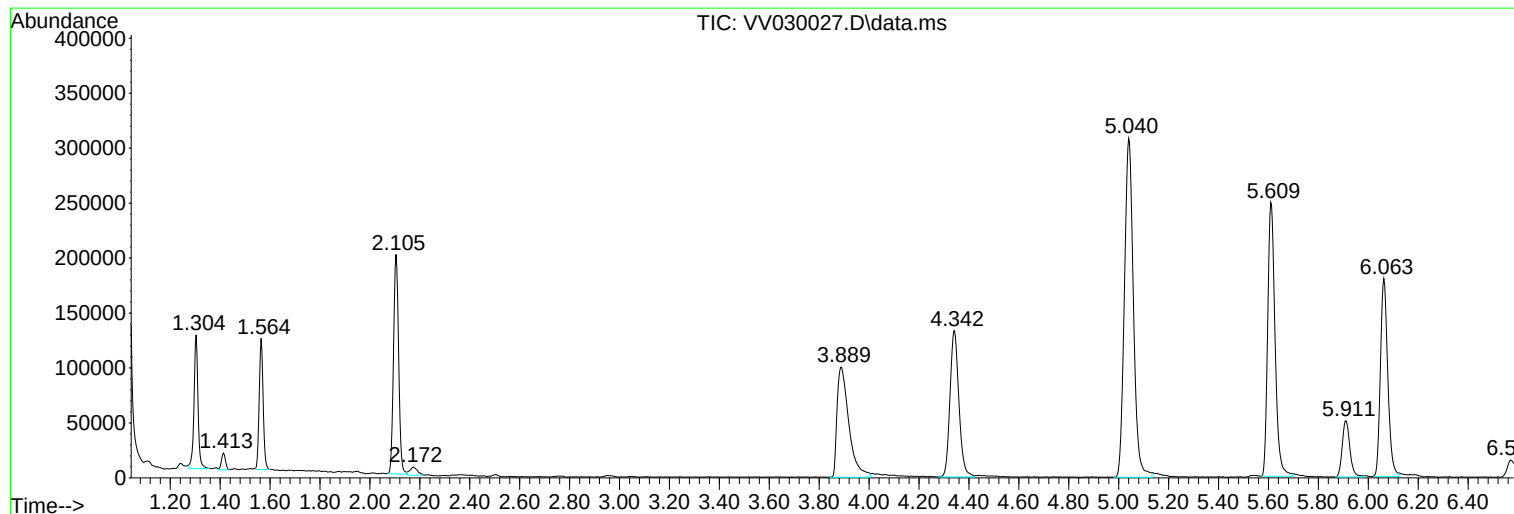

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030027.D
Acq On : 02 Feb 2023 16:40
Operator : SY/MD
Sample : 01408-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030027.D
Acq On : 02 Feb 2023 16:40
Operator : SY/MD
Sample : 01408-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc