
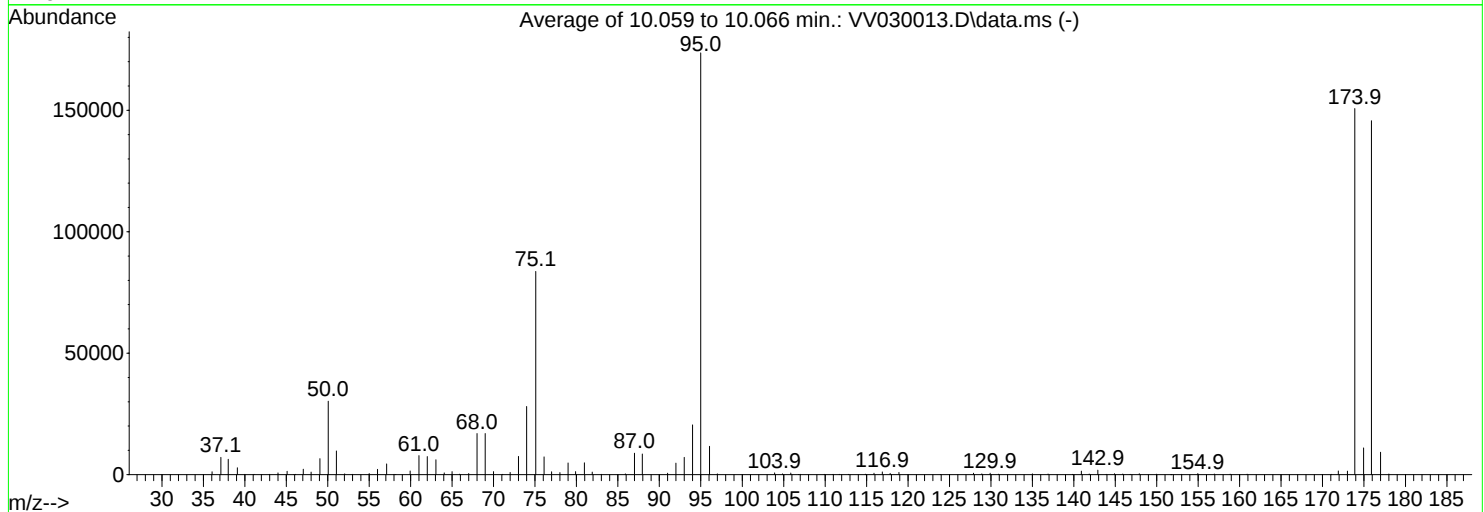


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020223\
Data File : VV030013.D
Acq On : 02 Feb 2023 09:35
Operator : SY/MD
Sample : BFB220
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB220

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Feb 03 01:11:57 2023

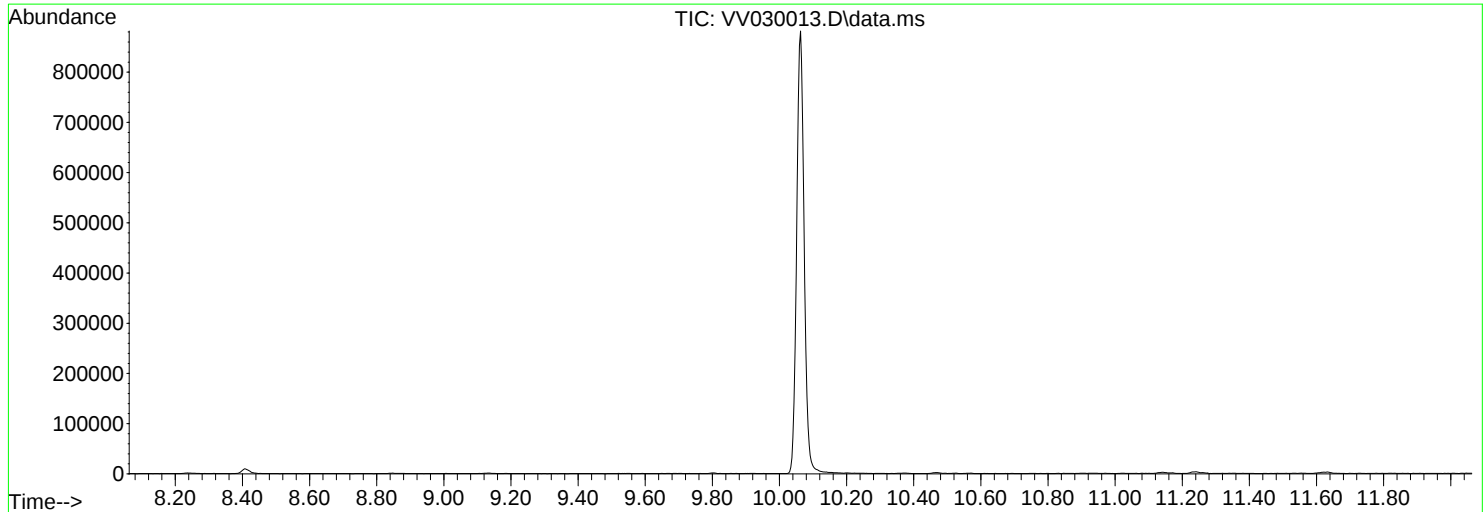

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2791

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	30256	PASS
75	95	30	80	48.2	83683	PASS
95	95	100	100	100.0	173653	PASS
96	95	5	9	6.7	11648	PASS
173	174	0.00	2	1.0	1475	PASS
174	95	50	120	86.8	150720	PASS
175	174	5	9	7.3	11021	PASS
176	174	95	105	96.7	145728	PASS
177	176	5	10	6.3	9235	PASS

m/z	Abundance
39.90	200.0
44.00	517.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.10	1219.0
37.10	7286.0
38.00	6278.0
39.10	2980.0
40.10	255.0
41.10	112.0
42.00	130.0
43.00	109.0
44.00	1303.0
45.10	1381.0
45.90	196.0
47.00	2283.0
48.00	1166.0
49.10	6885.0
50.10	30816.0
51.10	9901.0
52.10	346.0
53.00	150.0
55.00	419.0
56.00	2193.0
57.10	4559.0
58.00	212.0
60.00	1512.0
61.00	7855.0
62.00	7462.0
63.10	6230.0
64.00	734.0
65.00	1281.0
65.90	225.0
67.00	496.0
68.00	17296.0
69.00	17264.0
70.00	1202.0
71.10	103.0
72.00	1040.0
73.00	7675.0
74.00	28768.0
75.10	84152.0
76.10	7578.0
77.00	1128.0
78.00	907.0
79.00	4934.0
79.90	1202.0
80.90	5026.0
81.90	1016.0
83.00	131.0
85.90	326.0
87.00	8892.0
87.90	8486.0
91.00	577.0
92.00	4918.0
93.00	7322.0
94.00	20480.0
95.00	174848.0
96.10	11771.0
97.00	294.0
103.90	724.0
104.90	250.0
105.90	695.0
106.80	187.0
109.90	117.0
110.90	151.0
111.70	102.0
112.70	125.0
114.90	220.0
115.90	580.0
116.90	1113.0
117.90	498.0
118.90	919.0
123.90	123.0
127.90	565.0
128.90	332.0
129.90	663.0
130.90	194.0
135.00	320.0
136.90	280.0
139.80	149.0
140.90	1489.0
141.80	238.0
142.90	1862.0
143.90	157.0
144.90	496.0
145.90	270.0
146.80	136.0
147.90	419.0
150.00	209.0
151.70	102.0
153.00	119.0
155.00	445.0
157.00	250.0
158.80	197.0
160.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

171.00	170.0
171.90	1517.0
173.00	1420.0
173.90	148608.0
174.90	10675.0
175.90	142464.0
177.00	9105.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	1196.0
37.10	7445.0
38.00	6520.0
39.10	2949.0
40.10	317.0
41.10	136.0
42.10	122.0
43.00	129.0
44.00	1249.0
45.10	1429.0
46.10	166.0
47.10	2336.0
48.00	1110.0
49.00	6775.0
50.00	31312.0
51.10	10110.0
52.10	322.0
52.90	149.0
55.00	483.0
56.00	2236.0
57.10	4576.0
58.00	183.0
59.90	1532.0
61.00	8017.0
62.00	7629.0
63.10	6353.0
64.10	746.0
65.00	1292.0
65.90	230.0
67.00	466.0
68.00	17432.0
69.00	17584.0
70.00	1273.0
71.10	113.0
72.00	987.0
73.00	7767.0
74.00	29072.0
75.10	86552.0
76.10	7659.0
77.00	1267.0
78.00	862.0
79.00	5013.0
79.90	1262.0
81.00	5025.0
81.90	1130.0
83.00	139.0
85.90	315.0
87.00	9134.0
88.00	8848.0
91.00	654.0
92.00	4905.0
93.00	7291.0
94.00	21280.0
95.00	179776.0
96.10	12019.0
97.00	322.0
103.90	771.0
104.80	319.0
105.90	708.0
107.00	171.0
109.90	115.0
111.00	177.0
111.70	109.0
112.80	121.0
114.80	181.0
115.90	606.0
116.90	1226.0
117.90	560.0
118.90	916.0
123.90	104.0
127.90	625.0
128.90	370.0
129.90	639.0
130.90	232.0
135.00	340.0
136.90	262.0
139.90	153.0
140.90	1460.0
141.80	282.0
142.90	1902.0
143.90	126.0
144.90	412.0
145.90	291.0
146.80	138.0
147.90	436.0
149.90	197.0
153.00	144.0
155.00	437.0
156.90	264.0
158.90	202.0
160.90	163.0
171.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

171.90	1604.0
173.00	1530.0
173.90	156160.0
175.00	11484.0
175.90	150912.0
177.00	9511.0
178.00	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	1138.0
37.10	6702.0
38.00	6090.0
39.10	2628.0
40.10	355.0
41.10	142.0
42.90	190.0
44.10	1131.0
45.10	1294.0
46.10	155.0
47.10	2206.0
48.00	932.0
49.00	6086.0
50.00	28640.0
51.00	9265.0
52.00	291.0
52.90	139.0
55.00	468.0
56.00	2114.0
57.10	4063.0
58.20	171.0
60.00	1487.0
61.00	7600.0
62.00	7238.0
63.00	5915.0
64.10	700.0
65.00	1190.0
65.90	198.0
67.00	395.0
68.00	15988.0
69.00	15963.0
70.00	1225.0
71.10	120.0
72.00	832.0
73.00	7110.0
74.00	26288.0
75.10	80344.0
76.10	6756.0
77.00	1242.0
78.00	779.0
79.00	4567.0
79.90	1290.0
81.00	4673.0
81.90	1127.0
83.00	132.0
85.90	303.0
87.00	8533.0
88.00	8151.0
91.00	619.0
92.00	4461.0
93.00	6765.0
94.00	19784.0
95.00	166336.0
96.00	11153.0
97.00	345.0
103.90	708.0
104.80	346.0
105.80	678.0
107.00	147.0
109.90	118.0
111.00	154.0
111.70	104.0
112.90	121.0
114.80	138.0
115.90	555.0
116.90	1133.0
117.80	630.0
118.90	854.0
127.90	553.0
128.90	330.0
129.90	539.0
130.90	250.0
135.00	291.0
136.90	243.0
139.90	134.0
140.90	1338.0
141.90	274.0
142.90	1804.0
143.90	104.0
144.90	306.0
145.90	280.0
146.80	123.0
147.90	394.0
149.90	164.0
153.00	124.0
154.90	420.0
156.90	269.0
158.90	207.0
160.90	187.0
171.10	148.0
171.90	1507.0
173.00	1476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

173.90	147392.0
175.00	10904.0
175.90	143808.0
177.00	9090.0
178.00	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220