

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033958.D
 Acq On : 02 Feb 2024 09:43
 Operator : SY/MD
 Sample : VV0202MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	113877	122280	16.90%	2.085%
2	1.529	145	152	166	rVB	91777	109683	15.16%	1.870%
3	2.060	307	317	350	rVB	197724	292162	40.38%	4.981%
4	2.281	383	386	390	rBV2	202	221	0.03%	0.004%
5	2.371	411	414	416	rBV	223	125	0.02%	0.002%
6	2.400	420	423	427	rVB2	199	167	0.02%	0.003%
7	2.445	434	437	438	rBV	537	283	0.04%	0.005%
8	2.635	493	496	500	rBV	169	160	0.02%	0.003%
9	2.709	516	519	523	rBV2	177	163	0.02%	0.003%
10	2.767	534	537	539	rBV2	195	155	0.02%	0.003%
11	3.085	632	636	637	rBV	167	139	0.02%	0.002%
12	3.191	666	669	673	rVB2	334	264	0.04%	0.005%
13	3.217	673	677	679	rBV	191	184	0.03%	0.003%
14	3.352	717	719	723	rVB2	165	140	0.02%	0.002%
15	3.375	723	726	728	rBV2	183	111	0.02%	0.002%
16	3.439	743	746	747	rBV	190	128	0.02%	0.002%
17	3.484	758	760	765	rVB2	297	235	0.03%	0.004%
18	3.519	765	771	773	rBV2	246	337	0.05%	0.006%
19	3.555	778	782	784	rVV	172	113	0.02%	0.002%
20	3.596	793	795	799	rBV2	141	123	0.02%	0.002%
21	3.725	831	835	839	rBV2	157	115	0.02%	0.002%
22	3.786	846	854	892	rBV	49197	133920	18.51%	2.283%
23	4.246	982	997	1027	rBV	111818	285291	39.44%	4.864%
24	4.526	1081	1084	1085	rBV	260	153	0.02%	0.003%
25	4.571	1094	1098	1100	rBV3	308	313	0.04%	0.005%
26	4.686	1129	1134	1136	rBV2	286	226	0.03%	0.004%
27	4.953	1200	1217	1246	rBV2	274060	723443	100.00%	12.335%
28	5.394	1351	1354	1357	rBV3	313	250	0.03%	0.004%
29	5.455	1371	1373	1375	rBV2	256	122	0.02%	0.002%
30	5.493	1382	1385	1386	rBV	291	160	0.02%	0.003%
31	5.532	1386	1397	1428	rVV	249968	505232	69.84%	8.614%
32	5.828	1483	1489	1491	rBV3	1786	1956	0.27%	0.033%
33	5.931	1518	1521	1524	rBV2	281	210	0.03%	0.004%
34	5.985	1524	1538	1568	rBV	152329	318168	43.98%	5.425%
35	6.243	1615	1618	1622	rVB2	279	252	0.03%	0.004%
36	6.278	1626	1629	1630	rBV2	158	112	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033958.D
 Acq On : 02 Feb 2024 09:43
 Operator : SY/MD
 Sample : VV0202MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.317	1636	1641	1644	rBV2	195	170	0.02%	0.003%
38	6.474	1687	1690	1691	rBV2	231	134	0.02%	0.002%
39	6.509	1698	1701	1706	rBV2	161	173	0.02%	0.003%
40	6.551	1710	1714	1717	rBV2	164	169	0.02%	0.003%
41	6.628	1734	1738	1740	rBV2	187	175	0.02%	0.003%
42	6.680	1750	1754	1756	rBV	142	111	0.02%	0.002%
43	6.764	1777	1780	1784	rBV2	158	158	0.02%	0.003%
44	6.828	1797	1800	1802	rBV2	150	120	0.02%	0.002%
45	6.911	1816	1826	1853	rBV	94362	175472	24.26%	2.992%
46	7.243	1918	1929	1959	rBV	331808	585952	80.99%	9.990%
47	7.551	2016	2025	2052	rBV	62328	112037	15.49%	1.910%
48	7.744	2082	2085	2087	rBV2	357	181	0.03%	0.003%
49	8.024	2163	2172	2214	rBV	169266	334809	46.28%	5.708%
50	8.374	2278	2281	2282	rBV2	382	227	0.03%	0.004%
51	8.410	2290	2292	2295	rBV	246	182	0.03%	0.003%
52	8.500	2316	2320	2322	rBV	329	294	0.04%	0.005%
53	8.670	2368	2373	2376	rBV	192	225	0.03%	0.004%
54	8.783	2397	2408	2440	rBV	367714	607970	84.04%	10.366%
55	9.091	2501	2504	2511	rBB4	436	461	0.06%	0.008%
56	9.320	2569	2575	2579	rBV2	151	175	0.02%	0.003%
57	9.374	2587	2592	2596	rBV2	207	293	0.04%	0.005%
58	9.458	2615	2618	2621	rBV2	225	167	0.02%	0.003%
59	9.493	2621	2629	2634	rVV3	301	537	0.07%	0.009%
60	9.622	2667	2669	2673	rVB	325	184	0.03%	0.003%
61	9.866	2741	2745	2747	rBV	501	421	0.06%	0.007%
62	9.931	2758	2765	2769	rBV2	202	335	0.05%	0.006%
63	10.085	2810	2813	2816	rBV	161	174	0.02%	0.003%
64	10.152	2821	2834	2851	rBV	205659	320181	44.26%	5.459%
65	10.310	2879	2883	2884	rBV	236	185	0.03%	0.003%
66	10.371	2899	2902	2907	rBV2	215	163	0.02%	0.003%
67	10.406	2910	2913	2916	rBV	271	254	0.04%	0.004%
68	10.628	2980	2982	2985	rVB2	215	130	0.02%	0.002%
69	10.648	2986	2988	2993	rBV2	159	146	0.02%	0.002%
70	10.866	3049	3056	3066	rVB4	946	1631	0.23%	0.028%
71	10.911	3066	3070	3075	rBV2	221	275	0.04%	0.005%
72	10.976	3088	3090	3093	rBV	196	112	0.02%	0.002%
73	11.027	3103	3106	3109	rVB2	189	138	0.02%	0.002%
74	11.043	3109	3111	3116	rBV2	200	195	0.03%	0.003%
75	11.133	3133	3139	3145	rVB3	1269	1318	0.18%	0.022%
76	11.185	3145	3155	3181	rBV	395986	610209	84.35%	10.404%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033958.D
 Acq On : 02 Feb 2024 09:43
 Operator : SY/MD
 Sample : VV0202MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.406	3221	3224	3228	rBV	260	213	0.03%	0.004%
78	11.448	3235	3237	3240	rBV2	163	121	0.02%	0.002%
79	11.496	3249	3252	3253	rBV2	201	143	0.02%	0.002%
80	11.561	3260	3272	3299	rBV	335509	531323	73.44%	9.059%
81	12.046	3420	3423	3427	rBV2	198	201	0.03%	0.003%
82	12.127	3444	3448	3451	rBV2	181	115	0.02%	0.002%
83	12.291	3496	3499	3503	rVB	205	120	0.02%	0.002%
84	12.348	3514	3517	3522	rBV2	185	194	0.03%	0.003%
85	12.422	3537	3540	3543	rBV2	187	164	0.02%	0.003%
86	12.593	3584	3593	3601	rVB4	2458	3917	0.54%	0.067%
87	12.660	3611	3614	3616	rBV2	193	141	0.02%	0.002%
88	12.847	3669	3672	3674	rBV2	161	121	0.02%	0.002%
89	12.914	3691	3693	3696	rBV	209	164	0.02%	0.003%
90	13.017	3722	3725	3730	rVB2	169	137	0.02%	0.002%
91	13.204	3776	3783	3798	rVB2	6276	9244	1.28%	0.158%
92	13.358	3828	3831	3836	rBV2	193	188	0.03%	0.003%
93	13.400	3842	3844	3847	rBV	167	126	0.02%	0.002%
94	13.442	3849	3857	3879	rVB	30582	50892	7.03%	0.868%
95	13.686	3925	3933	3948	rVB3	8476	12819	1.77%	0.219%
96	13.786	3961	3964	3968	rBV	271	238	0.03%	0.004%
97	14.107	4061	4064	4068	rVB2	300	282	0.04%	0.005%
98	14.130	4068	4071	4076	rBV3	318	319	0.04%	0.005%
99	14.165	4079	4082	4088	rBV2	425	413	0.06%	0.007%
100	14.831	4287	4289	4291	rBV	388	227	0.03%	0.004%




Sum of corrected areas: 5865161

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033958.D
Acq On : 02 Feb 2024 09:43
Operator : SY/MD
Sample : VV0202MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

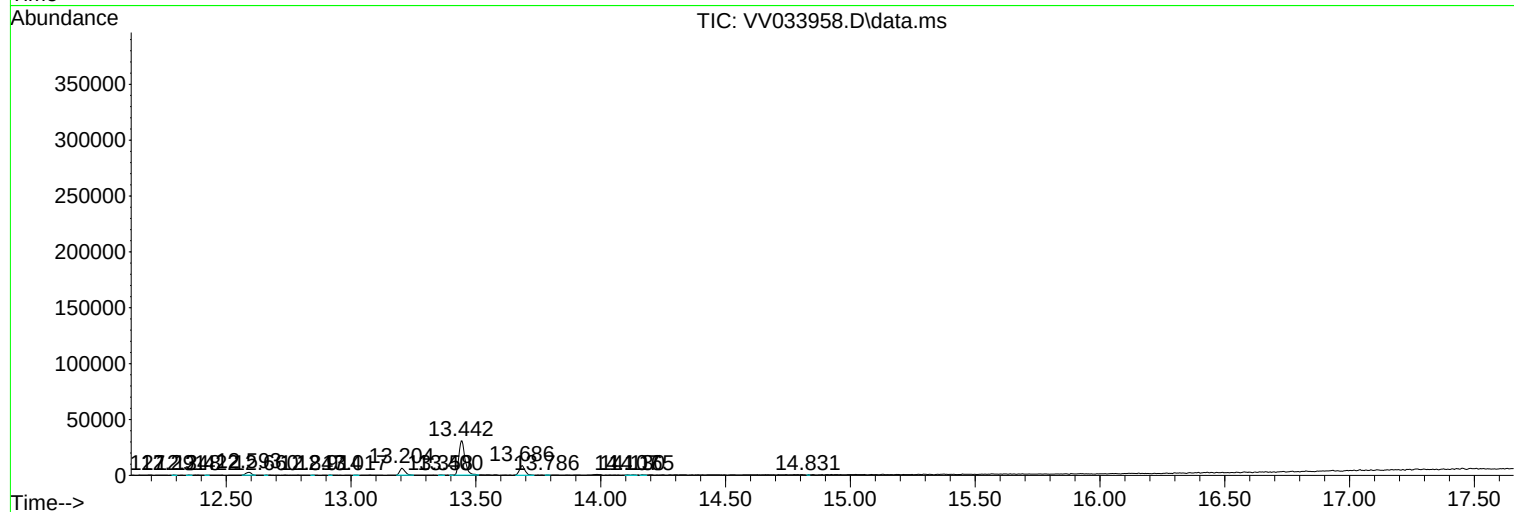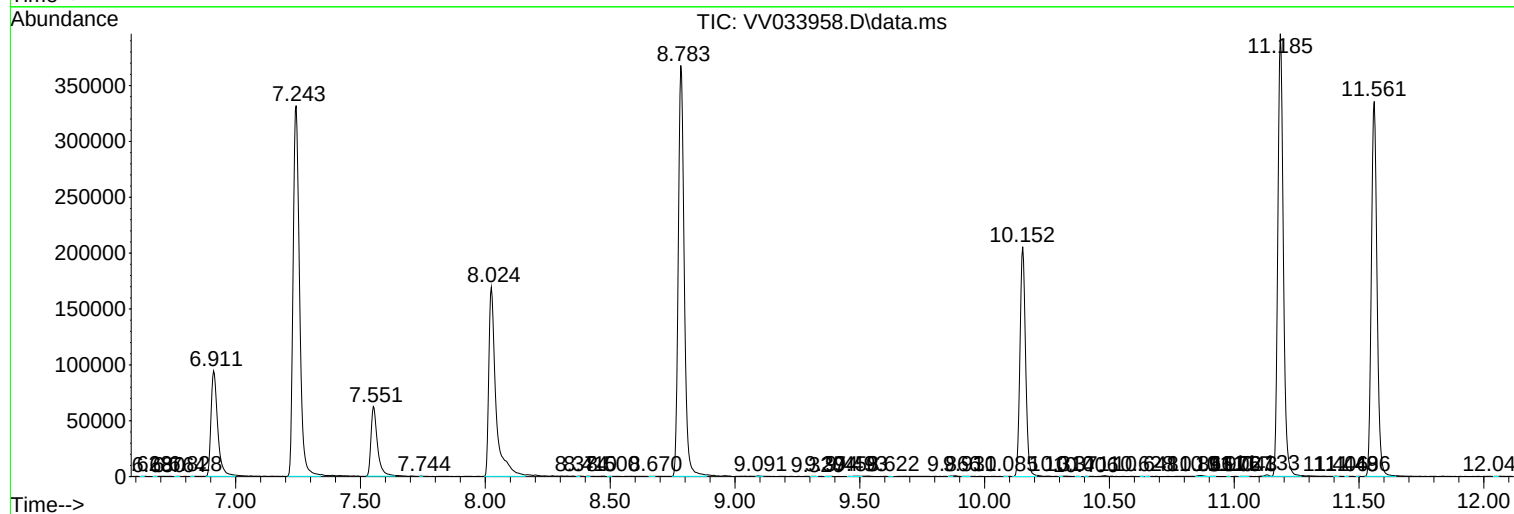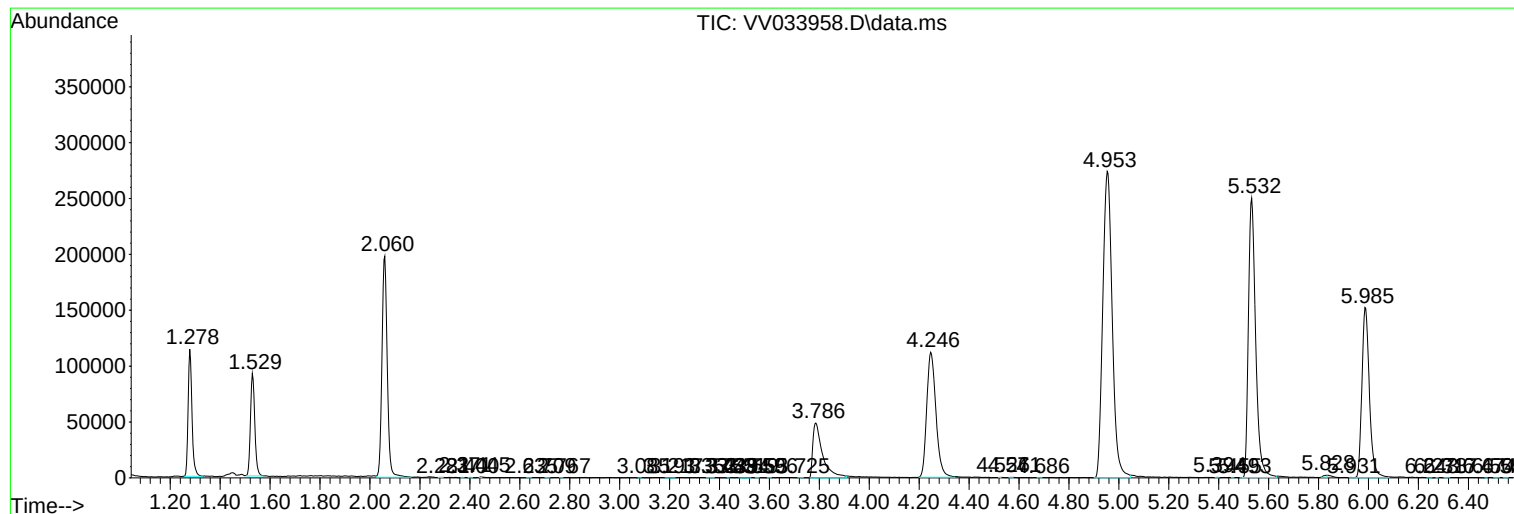

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033958.D
Acq On : 02 Feb 2024 09:43
Operator : SY/MD
Sample : VV0202MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033958.D
Acq On : 02 Feb 2024 09:43
Operator : SY/MD
Sample : VV0202MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc