

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033960.D
 Acq On : 02 Feb 2024 10:31
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033960.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	50	rBV	4118	4880	0.69%	0.087%
2	1.278	67	74	92	rBV	112473	121407	17.11%	2.155%
3	1.529	144	152	169	rVB	88143	107924	15.21%	1.915%
4	2.060	306	317	338	rBV	192392	282522	39.82%	5.014%
5	2.449	434	438	445	rVB2	652	718	0.10%	0.013%
6	2.487	447	450	455	rVB	190	165	0.02%	0.003%
7	2.613	482	489	495	rBV	161	337	0.05%	0.006%
8	2.751	525	532	534	rBV	167	205	0.03%	0.004%
9	2.793	541	545	548	rVB2	251	214	0.03%	0.004%
10	2.847	559	562	566	rVB2	331	316	0.04%	0.006%
11	2.989	603	606	609	rVB2	219	155	0.02%	0.003%
12	3.008	609	612	616	rBV2	170	168	0.02%	0.003%
13	3.050	618	625	629	rVB2	218	283	0.04%	0.005%
14	3.105	638	642	645	rVB	197	179	0.03%	0.003%
15	3.159	654	659	664	rBV2	202	260	0.04%	0.005%
16	3.265	689	692	696	rVV2	243	216	0.03%	0.004%
17	3.349	713	718	726	rVB2	218	362	0.05%	0.006%
18	3.471	752	756	758	rBV2	208	190	0.03%	0.003%
19	3.571	782	787	790	rBV	301	360	0.05%	0.006%
20	3.783	845	853	888	rBV	49207	130532	18.40%	2.317%
21	4.249	982	998	1026	rBV	107900	280966	39.60%	4.987%
22	4.500	1074	1076	1080	rVB2	394	217	0.03%	0.004%
23	4.526	1080	1084	1087	rBV2	197	238	0.03%	0.004%
24	4.593	1101	1105	1107	rBV	220	164	0.02%	0.003%
25	4.658	1120	1125	1128	rBV2	199	220	0.03%	0.004%
26	4.770	1155	1160	1165	rBV2	167	252	0.04%	0.004%
27	4.896	1196	1199	1202	rVB2	172	154	0.02%	0.003%
28	4.957	1202	1218	1248	rBV2	270719	709556	100.00%	12.594%
29	5.326	1328	1333	1339	rBV3	289	414	0.06%	0.007%
30	5.468	1373	1377	1383	rVB3	210	269	0.04%	0.005%
31	5.532	1385	1397	1426	rBV	237290	483637	68.16%	8.584%
32	5.834	1483	1491	1505	rVB5	2869	6254	0.88%	0.111%
33	5.896	1506	1510	1516	rVB2	278	283	0.04%	0.005%
34	5.989	1527	1539	1571	rBV	153522	314469	44.32%	5.581%
35	6.150	1586	1589	1594	rVB4	522	457	0.06%	0.008%
36	6.175	1594	1597	1600	rVB3	467	289	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033960.D
 Acq On : 02 Feb 2024 10:31
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.294	1627	1634	1638	rBV2	348	505	0.07%	0.009%
38	6.320	1638	1642	1648	rVV2	225	318	0.04%	0.006%
39	6.468	1683	1688	1691	rBV	296	319	0.04%	0.006%
40	6.571	1715	1720	1723	rVB2	158	193	0.03%	0.003%
41	6.593	1723	1727	1730	rBV	196	183	0.03%	0.003%
42	6.629	1733	1738	1741	rBV2	194	198	0.03%	0.004%
43	6.754	1771	1777	1779	rBV2	228	245	0.03%	0.004%
44	6.838	1800	1803	1808	rBV2	189	171	0.02%	0.003%
45	6.912	1817	1826	1857	rBV	88833	169911	23.95%	3.016%
46	7.153	1898	1901	1904	rBV3	248	154	0.02%	0.003%
47	7.243	1918	1929	1959	rBV	322780	571982	80.61%	10.152%
48	7.555	2016	2026	2046	rBV	60463	109683	15.46%	1.947%
49	7.715	2072	2076	2079	rBV3	225	159	0.02%	0.003%
50	7.754	2085	2088	2093	rVB3	347	296	0.04%	0.005%
51	7.969	2151	2155	2158	rVB	287	251	0.04%	0.004%
52	8.024	2162	2172	2208	rBV	164171	328392	46.28%	5.828%
53	8.362	2273	2277	2281	rBV2	210	218	0.03%	0.004%
54	8.384	2281	2284	2287	rVV	222	182	0.03%	0.003%
55	8.571	2335	2342	2344	rBV2	197	216	0.03%	0.004%
56	8.783	2398	2408	2447	rBV	350421	586421	82.65%	10.408%
57	9.133	2514	2517	2526	rBV	147	234	0.03%	0.004%
58	9.362	2585	2588	2592	rVB	181	160	0.02%	0.003%
59	9.439	2606	2612	2614	rBV2	220	208	0.03%	0.004%
60	9.776	2711	2717	2720	rBV2	235	263	0.04%	0.005%
61	9.834	2732	2735	2738	rBV	180	180	0.03%	0.003%
62	10.153	2822	2834	2855	rBV	199460	311326	43.88%	5.526%
63	10.320	2883	2886	2889	rBV3	207	162	0.02%	0.003%
64	10.371	2899	2902	2906	rBV2	162	150	0.02%	0.003%
65	10.423	2915	2918	2922	rBV2	264	249	0.04%	0.004%
66	10.490	2936	2939	2944	rVV	243	203	0.03%	0.004%
67	10.516	2944	2947	2953	rVB2	176	227	0.03%	0.004%
68	11.185	3145	3155	3181	rBV	371878	578702	81.56%	10.271%
69	11.561	3260	3272	3294	rBV	327846	510469	71.94%	9.060%
70	11.873	3365	3369	3372	rBV	223	243	0.03%	0.004%
71	12.037	3416	3420	3421	rBV	203	163	0.02%	0.003%
72	12.236	3479	3482	3486	rBV2	183	208	0.03%	0.004%
73	12.310	3500	3505	3507	rBV2	216	223	0.03%	0.004%
74	12.632	3601	3605	3606	rBV	243	190	0.03%	0.003%
75	12.734	3634	3637	3641	rVB2	178	157	0.02%	0.003%
76	12.773	3646	3649	3654	rBV2	255	253	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033960.D
 Acq On : 02 Feb 2024 10:31
 Operator : SY/MD
 Sample : P1299-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.860	3673	3676	3679	rBV2	155	155	0.02%	0.003%
78	12.966	3705	3709	3711	rBV2	331	173	0.02%	0.003%
79	13.214	3780	3786	3789	rBV2	451	521	0.07%	0.009%
80	13.300	3808	3813	3816	rBV2	248	244	0.03%	0.004%
81	13.451	3852	3860	3872	rBV3	2672	4218	0.59%	0.075%
82	13.522	3878	3882	3884	rBV	182	155	0.02%	0.003%
83	13.580	3896	3900	3904	rBV2	153	183	0.03%	0.003%
84	13.648	3912	3921	3922	rBV	485	498	0.07%	0.009%
85	13.689	3931	3934	3937	rBV3	355	365	0.05%	0.006%
86	13.821	3972	3975	3979	rBV	337	301	0.04%	0.005%
87	13.950	4010	4015	4019	rBV2	357	505	0.07%	0.009%
88	13.985	4023	4026	4030	rVV3	325	304	0.04%	0.005%
89	14.050	4041	4046	4048	rBV2	274	242	0.03%	0.004%
90	14.136	4067	4073	4075	rBV	218	246	0.03%	0.004%
91	14.291	4118	4121	4126	rBV3	284	261	0.04%	0.005%
92	14.323	4127	4131	4134	rVB2	320	259	0.04%	0.005%
93	14.345	4134	4138	4141	rBV2	299	302	0.04%	0.005%
94	14.583	4210	4212	4217	rVB2	394	290	0.04%	0.005%
95	14.609	4217	4220	4223	rBV	336	283	0.04%	0.005%
96	14.664	4234	4237	4240	rBV3	200	167	0.02%	0.003%
97	15.088	4368	4369	4372	rBV2	391	162	0.02%	0.003%
98	15.490	4492	4494	4501	rBV2	453	478	0.07%	0.008%
99	15.541	4508	4510	4512	rBV2	344	185	0.03%	0.003%
100	15.670	4548	4550	4559	rVB5	558	557	0.08%	0.010%




Sum of corrected areas: 5634253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033960.D
Acq On : 02 Feb 2024 10:31
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

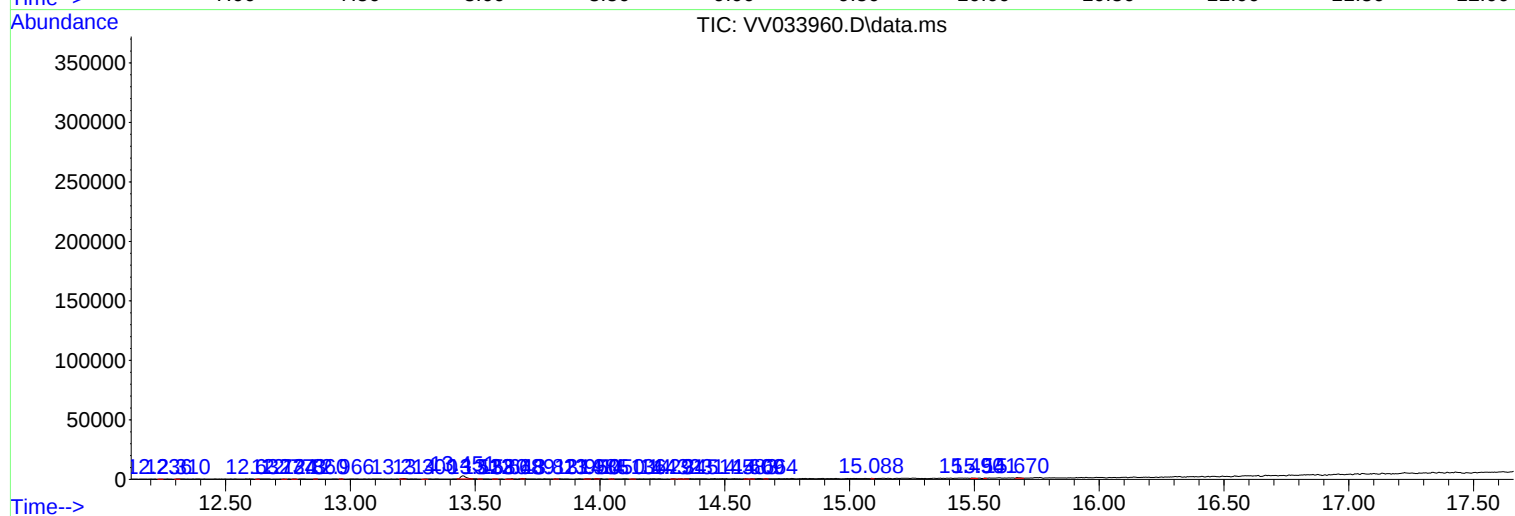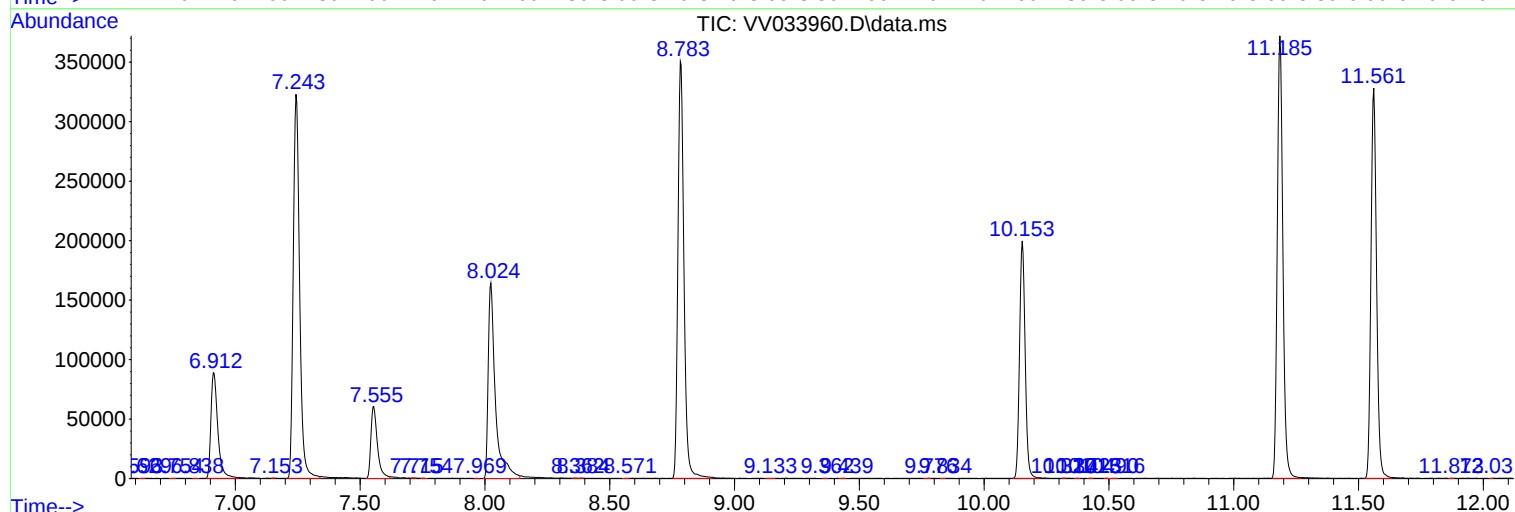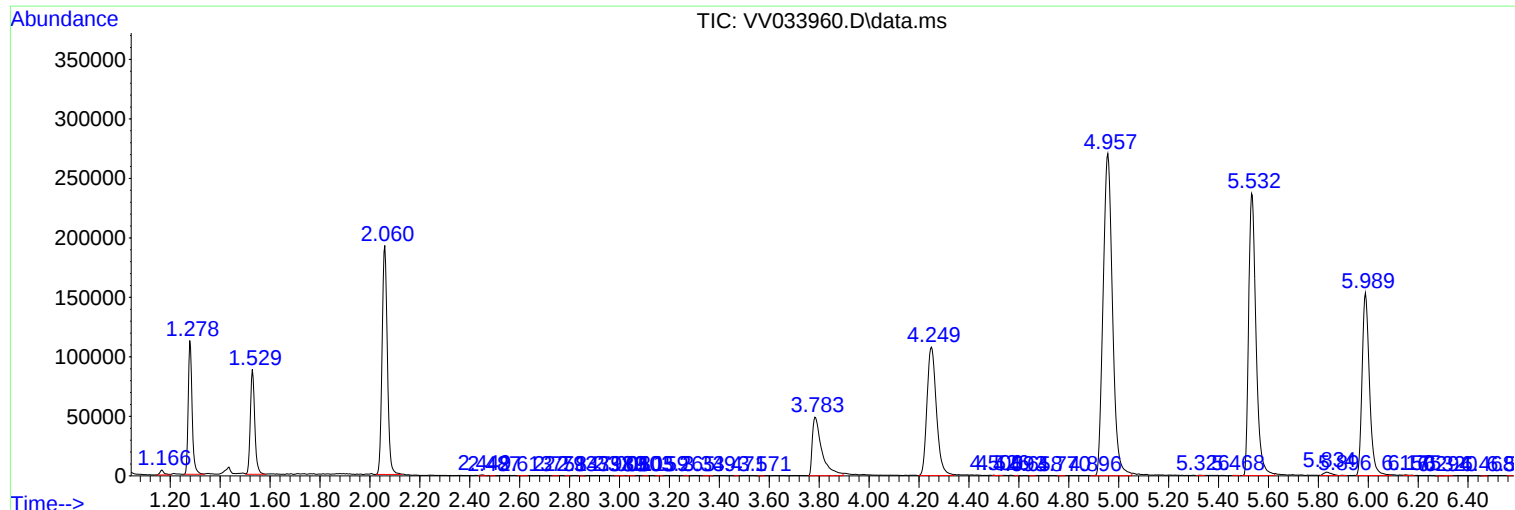

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033960.D
Acq On : 02 Feb 2024 10:31
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033960.D
Acq On : 02 Feb 2024 10:31
Operator : SY/MD
Sample : P1299-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------