

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033961.D
 Acq On : 02 Feb 2024 10:55
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	45	rBV	3969	4075	0.59%	0.074%
2	1.278	67	74	91	rBV	106113	115518	16.59%	2.105%
3	1.436	111	123	128	rBV4	4656	7564	1.09%	0.138%
4	1.529	144	152	171	rVB	84499	104556	15.02%	1.905%
5	2.059	306	317	341	rVB	185149	271205	38.96%	4.941%
6	2.185	353	356	363	rVB2	598	576	0.08%	0.010%
7	2.236	369	372	376	rBV3	353	299	0.04%	0.005%
8	2.368	411	413	419	rVB2	238	217	0.03%	0.004%
9	2.445	434	437	440	rBV	521	421	0.06%	0.008%
10	2.670	504	507	509	rBV	256	211	0.03%	0.004%
11	2.870	566	569	572	rBV	176	167	0.02%	0.003%
12	2.886	572	574	579	rVV	213	227	0.03%	0.004%
13	2.934	583	589	592	rVV2	188	258	0.04%	0.005%
14	2.963	592	598	603	rVB2	203	313	0.04%	0.006%
15	3.063	626	629	633	rBV2	186	194	0.03%	0.004%
16	3.175	661	664	667	rBV	216	168	0.02%	0.003%
17	3.371	722	725	728	rVB2	275	223	0.03%	0.004%
18	3.513	765	769	771	rBV	239	168	0.02%	0.003%
19	3.603	794	797	803	rBV2	233	267	0.04%	0.005%
20	3.783	845	853	892	rBV2	50069	132583	19.05%	2.416%
21	4.249	982	998	1029	rVV	108653	274475	39.43%	5.001%
22	4.468	1063	1066	1070	rBV2	534	414	0.06%	0.008%
23	4.731	1143	1148	1153	rVB2	188	220	0.03%	0.004%
24	4.780	1159	1163	1166	rBV2	151	160	0.02%	0.003%
25	4.870	1184	1191	1193	rBV2	143	226	0.03%	0.004%
26	4.957	1201	1218	1253	rBV2	263710	696130	100.00%	12.684%
27	5.153	1277	1279	1282	rBV3	343	173	0.02%	0.003%
28	5.214	1295	1298	1302	rBV2	396	349	0.05%	0.006%
29	5.317	1325	1330	1333	rBV2	212	264	0.04%	0.005%
30	5.487	1380	1383	1385	rBV2	211	164	0.02%	0.003%
31	5.532	1386	1397	1430	rVV	230993	471588	67.74%	8.592%
32	5.837	1482	1492	1498	rBV5	2645	4990	0.72%	0.091%
33	5.921	1512	1518	1523	rBV3	438	649	0.09%	0.012%
34	5.947	1523	1526	1527	rBV	306	172	0.02%	0.003%
35	5.989	1527	1539	1564	rVV	148549	307057	44.11%	5.595%
36	6.429	1672	1676	1684	rBV2	234	392	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033961.D
 Acq On : 02 Feb 2024 10:55
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.516	1698	1703	1706	rBV2	325	400	0.06%	0.007%
38	6.587	1721	1725	1727	rBV2	191	174	0.02%	0.003%
39	6.735	1767	1771	1775	rBV	159	191	0.03%	0.003%
40	6.776	1780	1784	1789	rBV	232	282	0.04%	0.005%
41	6.866	1809	1812	1815	rVB2	262	212	0.03%	0.004%
42	6.915	1815	1827	1859	rBV	87143	168209	24.16%	3.065%
43	7.243	1918	1929	1958	rBV	310591	556532	79.95%	10.140%
44	7.554	2016	2026	2052	rBV	58986	106782	15.34%	1.946%
45	7.754	2082	2088	2091	rBV2	231	230	0.03%	0.004%
46	7.799	2097	2102	2105	rVB2	186	202	0.03%	0.004%
47	7.882	2124	2128	2136	rVB2	336	321	0.05%	0.006%
48	7.927	2139	2142	2145	rBV2	233	217	0.03%	0.004%
49	8.024	2163	2172	2215	rBV	163669	327166	47.00%	5.961%
50	8.567	2334	2341	2346	rBV2	276	475	0.07%	0.009%
51	8.644	2361	2365	2369	rBV2	168	204	0.03%	0.004%
52	8.786	2398	2409	2444	rBV	342349	564518	81.09%	10.286%
53	9.027	2479	2484	2487	rBV2	149	184	0.03%	0.003%
54	9.120	2509	2513	2517	rVB2	180	194	0.03%	0.004%
55	9.162	2521	2526	2531	rBV2	224	284	0.04%	0.005%
56	9.197	2532	2537	2540	rBV2	163	184	0.03%	0.003%
57	9.378	2587	2593	2596	rBV2	217	285	0.04%	0.005%
58	9.480	2621	2625	2627	rBV	190	176	0.03%	0.003%
59	9.683	2685	2688	2694	rVB	251	171	0.02%	0.003%
60	9.718	2694	2699	2701	rBV2	206	223	0.03%	0.004%
61	10.066	2802	2807	2808	rBV	198	173	0.02%	0.003%
62	10.152	2823	2834	2855	rBV	193038	305959	43.95%	5.575%
63	10.265	2867	2869	2873	rVB3	250	183	0.03%	0.003%
64	10.329	2886	2889	2892	rVB2	291	196	0.03%	0.004%
65	10.361	2893	2899	2901	rBV2	219	254	0.04%	0.005%
66	10.439	2918	2923	2925	rBV2	195	174	0.02%	0.003%
67	10.638	2979	2985	2989	rBV2	202	298	0.04%	0.005%
68	10.712	3004	3008	3011	rBV	203	189	0.03%	0.003%
69	10.876	3056	3059	3062	rBV	161	158	0.02%	0.003%
70	10.947	3079	3081	3088	rVB2	208	188	0.03%	0.003%
71	10.982	3088	3092	3094	rBV	209	168	0.02%	0.003%
72	11.133	3133	3139	3144	rVB	185	231	0.03%	0.004%
73	11.185	3144	3155	3183	rBV	360386	556321	79.92%	10.136%
74	11.387	3216	3218	3225	rVV2	122	159	0.02%	0.003%
75	11.561	3260	3272	3295	rBV	318939	491422	70.59%	8.954%
76	11.734	3322	3326	3328	rBV	212	193	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033961.D
 Acq On : 02 Feb 2024 10:55
 Operator : SY/MD
 Sample : P1310-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.943	3388	3391	3395	rVB2	196	175	0.03%	0.003%
78	12.062	3427	3428	3433	rVB2	217	156	0.02%	0.003%
79	12.088	3433	3436	3439	rBV	236	153	0.02%	0.003%
80	12.130	3442	3449	3453	rVB2	317	394	0.06%	0.007%
81	12.416	3533	3538	3540	rBV2	176	159	0.02%	0.003%
82	12.554	3577	3581	3585	rVB2	208	234	0.03%	0.004%
83	12.577	3585	3588	3591	rBV2	208	172	0.02%	0.003%
84	12.837	3664	3669	3671	rBV	187	201	0.03%	0.004%
85	12.898	3685	3688	3692	rBV2	199	215	0.03%	0.004%
86	13.342	3820	3826	3827	rBV	233	191	0.03%	0.003%
87	13.455	3853	3861	3868	rBV	1223	1841	0.26%	0.034%
88	13.580	3895	3900	3903	rBV2	228	246	0.04%	0.004%
89	13.625	3908	3914	3918	rBV2	169	242	0.03%	0.004%
90	13.824	3972	3976	3980	rBV2	327	274	0.04%	0.005%
91	13.889	3993	3996	3999	rBV3	322	288	0.04%	0.005%
92	13.975	4020	4023	4024	rBV	391	210	0.03%	0.004%
93	14.088	4055	4058	4062	rBV	333	243	0.03%	0.004%
94	14.265	4106	4113	4115	rBV2	431	417	0.06%	0.008%
95	14.712	4249	4252	4256	rVB4	318	226	0.03%	0.004%
96	14.824	4284	4287	4294	rBV3	314	391	0.06%	0.007%
97	14.979	4331	4335	4338	rBV2	348	312	0.04%	0.006%
98	15.065	4360	4362	4368	rBV4	297	267	0.04%	0.005%
99	15.123	4377	4380	4383	rBV2	357	321	0.05%	0.006%
100	15.316	4438	4440	4445	rBV3	425	338	0.05%	0.006%




Sum of corrected areas: 5488381

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033961.D
Acq On : 02 Feb 2024 10:55
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

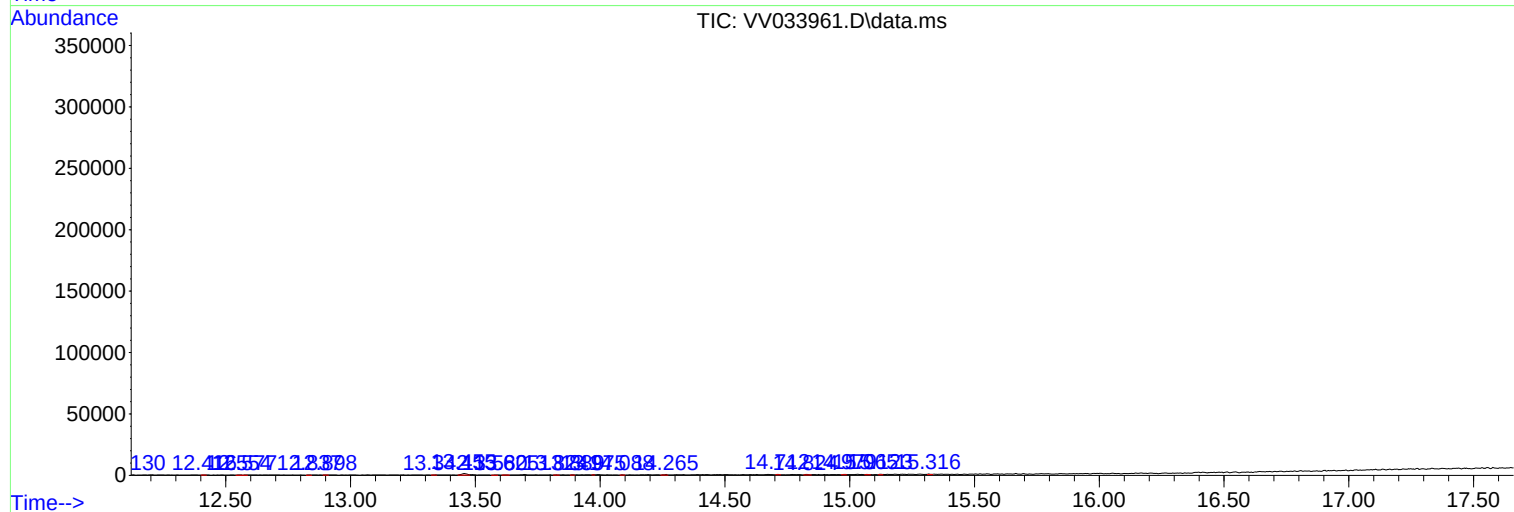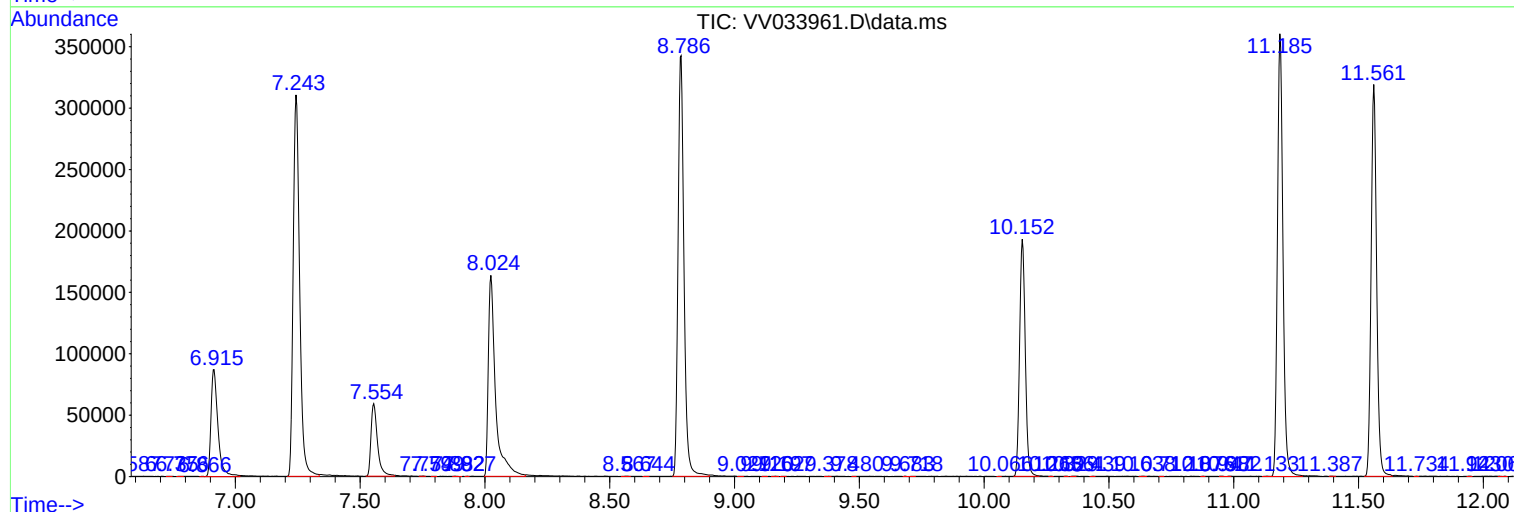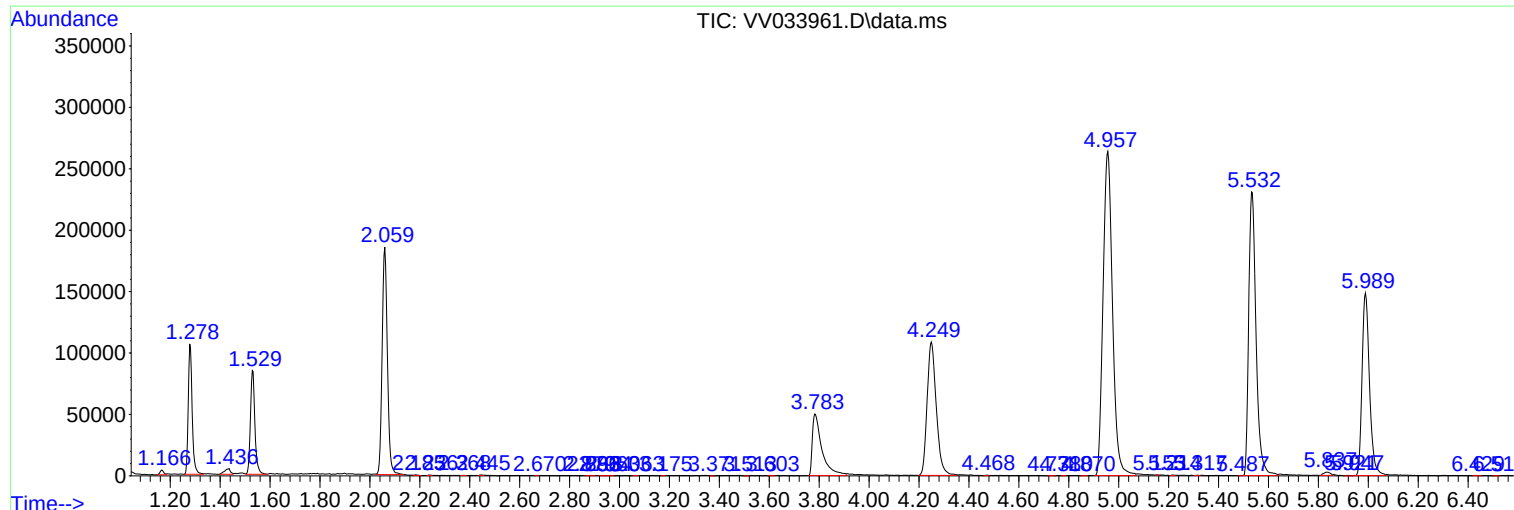

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033961.D
Acq On : 02 Feb 2024 10:55
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033961.D
Acq On : 02 Feb 2024 10:55
Operator : SY/MD
Sample : P1310-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc