

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033962.D
 Acq On : 02 Feb 2024 11:18
 Operator : SY/MD
 Sample : P1300-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	44	rBV	4016	4045	0.57%	0.072%
2	1.214	51	54	61	rBV4	730	760	0.11%	0.014%
3	1.278	67	74	87	rBV	111478	118281	16.75%	2.105%
4	1.433	112	122	128	rBV6	4591	6495	0.92%	0.116%
5	1.529	144	152	171	rVB	87182	108485	15.37%	1.931%
6	1.979	290	292	294	rBV	573	245	0.03%	0.004%
7	2.060	306	317	332	rBV	191135	278527	39.45%	4.957%
8	2.182	352	355	361	rVB	254	251	0.04%	0.004%
9	2.278	382	385	388	rBV	180	173	0.02%	0.003%
10	2.446	434	437	444	rVB3	877	911	0.13%	0.016%
11	2.474	444	446	451	rBV2	189	193	0.03%	0.003%
12	2.519	457	460	465	rBV2	136	164	0.02%	0.003%
13	2.561	471	473	476	rVB2	352	193	0.03%	0.003%
14	2.626	489	493	494	rBV	260	185	0.03%	0.003%
15	2.696	511	515	517	rBV	225	185	0.03%	0.003%
16	2.738	522	528	533	rBV2	214	290	0.04%	0.005%
17	2.892	572	576	578	rBV	190	154	0.02%	0.003%
18	3.220	674	678	681	rBV2	156	179	0.03%	0.003%
19	3.323	704	710	713	rBV2	196	241	0.03%	0.004%
20	3.439	743	746	749	rBV2	182	159	0.02%	0.003%
21	3.487	758	761	763	rBV	286	249	0.04%	0.004%
22	3.728	830	836	839	rBV2	223	299	0.04%	0.005%
23	3.783	845	853	901	rBV	49616	135278	19.16%	2.407%
24	4.249	982	998	1025	rBV	110922	280204	39.69%	4.987%
25	4.487	1065	1072	1074	rBV2	336	392	0.06%	0.007%
26	4.571	1092	1098	1101	rBB2	202	211	0.03%	0.004%
27	4.587	1101	1103	1107	rBV2	256	181	0.03%	0.003%
28	4.629	1113	1116	1119	rBV2	297	250	0.04%	0.004%
29	4.661	1120	1126	1128	rVV	268	243	0.03%	0.004%
30	4.777	1158	1162	1164	rBV2	158	165	0.02%	0.003%
31	4.870	1186	1191	1194	rBV	318	399	0.06%	0.007%
32	4.957	1202	1218	1246	rBV2	268768	705996	100.00%	12.564%
33	5.288	1317	1321	1322	rBV	303	226	0.03%	0.004%
34	5.410	1356	1359	1362	rVB2	320	206	0.03%	0.004%
35	5.532	1386	1397	1427	rBV	231003	474771	67.25%	8.449%
36	5.834	1483	1491	1505	rBV3	2939	6210	0.88%	0.111%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033962.D
 Acq On : 02 Feb 2024 11:18
 Operator : SY/MD
 Sample : P1300-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1566	rBV	152381	311597	44.14%	5.545%
38	6.265	1622	1625	1629	rBV2	179	198	0.03%	0.004%
39	6.288	1629	1632	1636	rVB	267	183	0.03%	0.003%
40	6.809	1789	1794	1799	rBV2	208	318	0.05%	0.006%
41	6.915	1817	1827	1858	rBV	89832	168899	23.92%	3.006%
42	7.088	1879	1881	1887	rVB2	368	287	0.04%	0.005%
43	7.124	1889	1892	1894	rVB3	268	194	0.03%	0.003%
44	7.243	1918	1929	1962	rBV	327426	575859	81.57%	10.248%
45	7.555	2017	2026	2050	rBV	62328	110535	15.66%	1.967%
46	8.024	2163	2172	2213	rBV	167397	331424	46.94%	5.898%
47	8.365	2274	2278	2285	rVV3	263	419	0.06%	0.007%
48	8.416	2289	2294	2298	rVV3	225	243	0.03%	0.004%
49	8.519	2324	2326	2329	rBV	212	164	0.02%	0.003%
50	8.683	2373	2377	2379	rBV	202	168	0.02%	0.003%
51	8.783	2397	2408	2450	rBV	351725	580442	82.22%	10.330%
52	8.921	2450	2451	2457	rVB3	448	239	0.03%	0.004%
53	8.998	2473	2475	2478	rVB	292	155	0.02%	0.003%
54	9.059	2488	2494	2497	rBV2	175	225	0.03%	0.004%
55	9.268	2553	2559	2562	rBV2	217	278	0.04%	0.005%
56	9.391	2594	2597	2599	rBV2	185	157	0.02%	0.003%
57	9.651	2676	2678	2684	rVB	199	201	0.03%	0.004%
58	9.693	2684	2691	2693	rBV2	222	299	0.04%	0.005%
59	10.008	2780	2789	2792	rBV2	228	324	0.05%	0.006%
60	10.153	2822	2834	2864	rVB	200589	314046	44.48%	5.589%
61	10.304	2875	2881	2885	rBV2	186	252	0.04%	0.004%
62	10.326	2885	2888	2892	rVB2	366	330	0.05%	0.006%
63	10.471	2930	2933	2938	rBV2	149	181	0.03%	0.003%
64	10.526	2946	2950	2952	rBV	199	169	0.02%	0.003%
65	10.593	2966	2971	2974	rBV2	154	197	0.03%	0.004%
66	10.664	2989	2993	2999	rBV	186	250	0.04%	0.004%
67	10.857	3045	3053	3058	rBV2	264	492	0.07%	0.009%
68	10.934	3074	3077	3081	rBV2	158	183	0.03%	0.003%
69	11.024	3103	3105	3112	rBV2	115	154	0.02%	0.003%
70	11.185	3144	3155	3182	rBV	366530	571570	80.96%	10.172%
71	11.561	3260	3272	3294	rBV	324639	514286	72.85%	9.152%
72	11.757	3328	3333	3334	rBV	185	174	0.02%	0.003%
73	12.181	3461	3465	3469	rBV2	170	217	0.03%	0.004%
74	12.201	3469	3471	3478	rVB3	214	193	0.03%	0.003%
75	12.345	3513	3516	3519	rBV2	189	176	0.02%	0.003%
76	12.757	3642	3644	3649	rVB2	191	172	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033962.D
 Acq On : 02 Feb 2024 11:18
 Operator : SY/MD
 Sample : P1300-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.789	3649	3654	3657	rBV	210	239	0.03%	0.004%
78	12.921	3686	3695	3703	rBV2	344	623	0.09%	0.011%
79	13.085	3743	3746	3750	rBV3	191	192	0.03%	0.003%
80	13.156	3764	3768	3773	rBV2	159	199	0.03%	0.004%
81	13.407	3842	3846	3849	rBV2	195	180	0.03%	0.003%
82	13.426	3849	3852	3854	rBV	345	178	0.03%	0.003%
83	13.458	3854	3862	3873	rVV3	636	1391	0.20%	0.025%
84	13.567	3893	3896	3899	rBV2	239	203	0.03%	0.004%
85	13.628	3913	3915	3919	rVB	380	282	0.04%	0.005%
86	13.654	3919	3923	3925	rBV2	194	198	0.03%	0.004%
87	13.741	3944	3950	3954	rBV2	267	389	0.06%	0.007%
88	13.937	4005	4011	4013	rBV2	222	250	0.04%	0.004%
89	13.979	4020	4024	4030	rBV2	559	902	0.13%	0.016%
90	14.136	4068	4073	4075	rBV2	222	219	0.03%	0.004%
91	14.265	4108	4113	4115	rBV3	241	219	0.03%	0.004%
92	14.403	4153	4156	4162	rBV2	207	244	0.03%	0.004%
93	14.458	4170	4173	4177	rBV2	172	169	0.02%	0.003%
94	14.628	4222	4226	4227	rBV2	254	173	0.02%	0.003%
95	14.879	4301	4304	4308	rVB4	272	224	0.03%	0.004%
96	15.053	4354	4358	4360	rBV3	301	239	0.03%	0.004%
97	15.085	4365	4368	4374	rBV3	376	439	0.06%	0.008%
98	15.329	4442	4444	4448	rBV2	318	210	0.03%	0.004%
99	15.374	4456	4458	4463	rVB2	400	271	0.04%	0.005%
100	15.426	4470	4474	4475	rBV3	322	273	0.04%	0.005%




Sum of corrected areas: 5619152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033962.D
Acq On : 02 Feb 2024 11:18
Operator : SY/MD
Sample : P1300-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

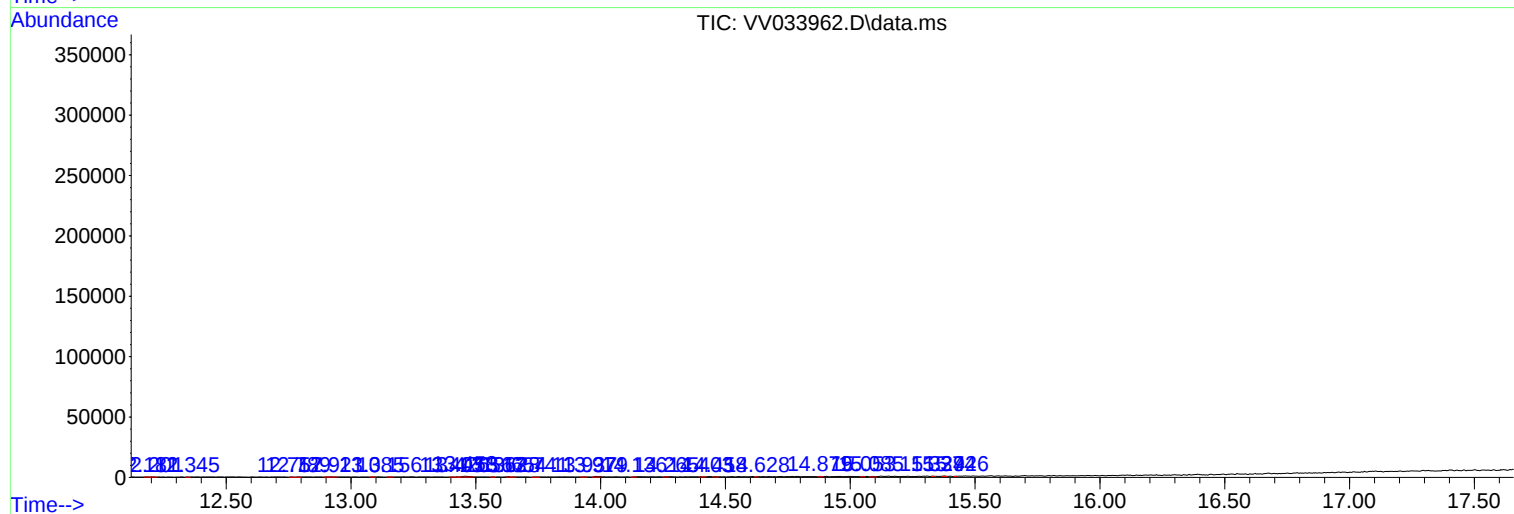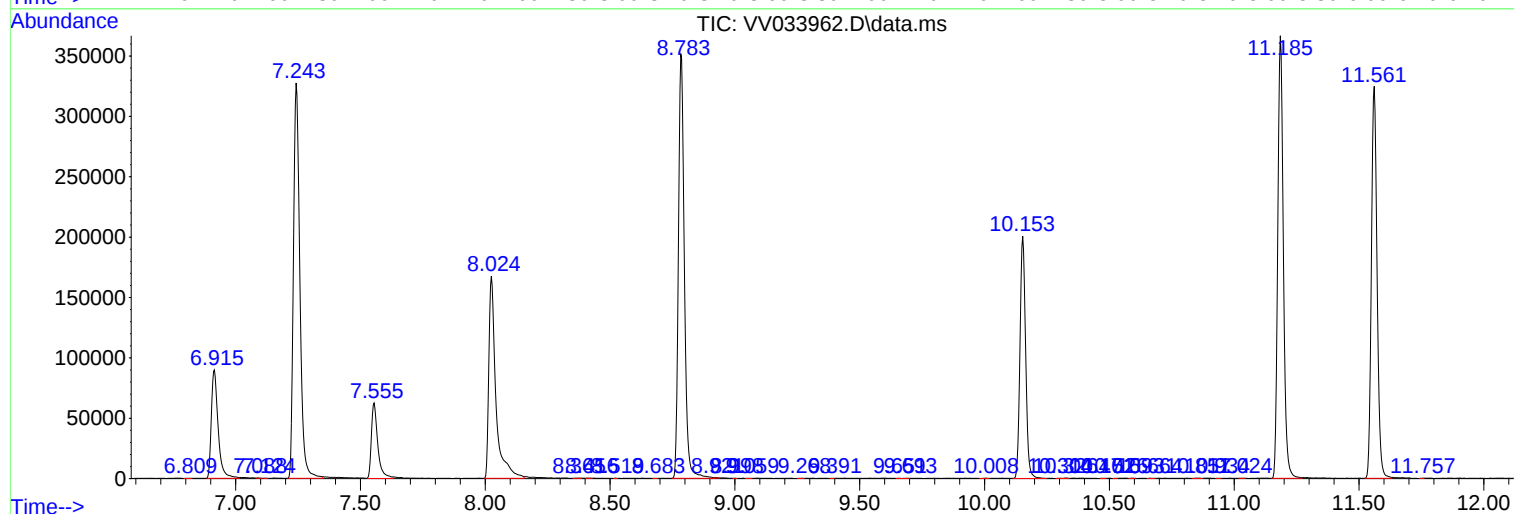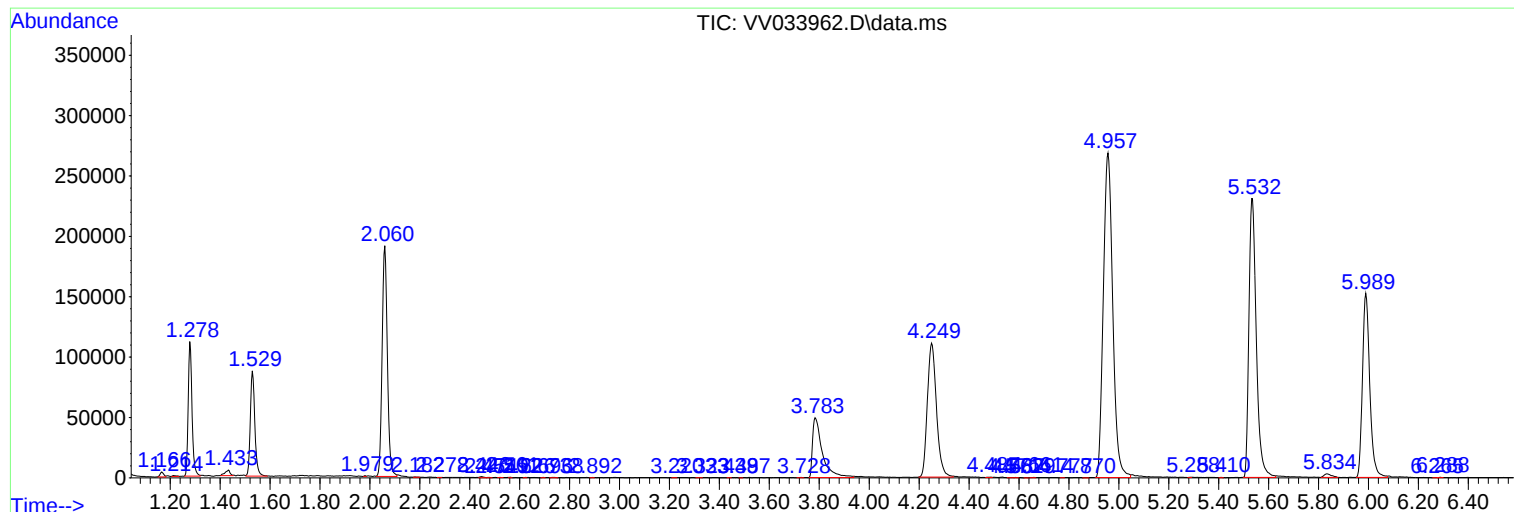

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033962.D
Acq On : 02 Feb 2024 11:18
Operator : SY/MD
Sample : P1300-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033962.D
Acq On : 02 Feb 2024 11:18
Operator : SY/MD
Sample : P1300-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc