

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033963.D
 Acq On : 02 Feb 2024 11:42
 Operator : SY/MD
 Sample : P1329-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	4019	4242	0.61%	0.077%
2	1.278	67	74	89	rBV	109118	117473	16.85%	2.133%
3	1.436	112	123	130	rBV7	3937	6826	0.98%	0.124%
4	1.529	144	152	171	rVB	86572	105580	15.14%	1.917%
5	2.060	306	317	337	rVB	185882	272158	39.04%	4.942%
6	2.243	371	374	377	rVB	306	223	0.03%	0.004%
7	2.330	397	401	404	rBV	276	237	0.03%	0.004%
8	2.449	428	438	441	rBV4	970	1199	0.17%	0.022%
9	2.558	469	472	476	rVV2	262	169	0.02%	0.003%
10	2.677	503	509	511	rBV2	208	203	0.03%	0.004%
11	2.754	527	533	537	rBV2	184	257	0.04%	0.005%
12	2.953	590	595	597	rBV	207	164	0.02%	0.003%
13	3.060	624	628	631	rVB2	270	242	0.03%	0.004%
14	3.085	631	636	643	rBV2	168	338	0.05%	0.006%
15	3.121	644	647	653	rVB2	214	273	0.04%	0.005%
16	3.156	653	658	662	rBV	202	184	0.03%	0.003%
17	3.185	662	667	674	rVB2	288	383	0.05%	0.007%
18	3.233	679	682	688	rVB	264	264	0.04%	0.005%
19	3.404	732	735	739	rVB2	202	165	0.02%	0.003%
20	3.429	739	743	748	rBV2	210	242	0.03%	0.004%
21	3.661	805	815	818	rVB2	228	444	0.06%	0.008%
22	3.687	818	823	825	rBV	189	227	0.03%	0.004%
23	3.783	845	853	893	rBV	49289	132508	19.01%	2.406%
24	4.066	937	941	943	rBV	258	244	0.03%	0.004%
25	4.249	982	998	1025	rBV	108524	276298	39.63%	5.018%
26	4.436	1053	1056	1059	rVB3	365	216	0.03%	0.004%
27	4.523	1080	1083	1084	rBV2	320	184	0.03%	0.003%
28	4.957	1202	1218	1251	rBV2	266232	697193	100.00%	12.661%
29	5.236	1303	1305	1309	rBV2	294	187	0.03%	0.003%
30	5.330	1327	1334	1336	rBV3	212	229	0.03%	0.004%
31	5.352	1336	1341	1345	rVB2	201	253	0.04%	0.005%
32	5.394	1348	1354	1360	rVB2	258	289	0.04%	0.005%
33	5.432	1360	1366	1369	rBV2	244	288	0.04%	0.005%
34	5.532	1387	1397	1432	rBV	225814	464193	66.58%	8.430%
35	5.796	1475	1479	1482	rBV2	204	173	0.02%	0.003%
36	5.834	1482	1491	1505	rVB4	2893	6387	0.92%	0.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033963.D
 Acq On : 02 Feb 2024 11:42
 Operator : SY/MD
 Sample : P1329-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1572	rBV	149866	312075	44.76%	5.667%
38	6.188	1597	1601	1605	rVB2	197	176	0.03%	0.003%
39	6.757	1774	1778	1781	rBV2	189	206	0.03%	0.004%
40	6.825	1795	1799	1801	rBV2	160	164	0.02%	0.003%
41	6.876	1809	1815	1817	rBV	232	226	0.03%	0.004%
42	6.915	1817	1827	1857	rVV	87955	165792	23.78%	3.011%
43	7.243	1917	1929	1963	rBV	315984	562506	80.68%	10.215%
44	7.555	2017	2026	2058	rVV2	61539	109573	15.72%	1.990%
45	7.799	2097	2102	2106	rBV2	200	232	0.03%	0.004%
46	7.838	2110	2114	2120	rBV2	189	292	0.04%	0.005%
47	7.870	2121	2124	2131	rVB3	191	185	0.03%	0.003%
48	8.024	2163	2172	2211	rBV	165057	326806	46.87%	5.935%
49	8.362	2275	2277	2281	rVB2	271	172	0.02%	0.003%
50	8.448	2300	2304	2305	rBV	190	163	0.02%	0.003%
51	8.702	2378	2383	2388	rBV2	151	176	0.03%	0.003%
52	8.783	2396	2408	2441	rBV	338694	562532	80.69%	10.216%
53	8.985	2467	2471	2475	rBV3	234	213	0.03%	0.004%
54	9.178	2524	2531	2535	rBV2	190	291	0.04%	0.005%
55	9.233	2543	2548	2550	rBV2	273	284	0.04%	0.005%
56	9.304	2567	2570	2574	rBV	174	184	0.03%	0.003%
57	9.448	2613	2615	2620	rBV	205	219	0.03%	0.004%
58	9.979	2776	2780	2784	rBV2	228	204	0.03%	0.004%
59	10.114	2816	2822	2823	rBV	232	185	0.03%	0.003%
60	10.153	2823	2834	2859	rVV	195327	310875	44.59%	5.646%
61	10.333	2884	2890	2897	rBV2	266	455	0.07%	0.008%
62	10.493	2936	2940	2947	rBV2	174	237	0.03%	0.004%
63	10.654	2985	2990	2995	rVV2	129	169	0.02%	0.003%
64	10.789	3029	3032	3038	rVB2	208	241	0.03%	0.004%
65	10.818	3038	3041	3046	rBV2	194	203	0.03%	0.004%
66	10.911	3068	3070	3074	rBV2	199	196	0.03%	0.004%
67	10.992	3089	3095	3101	rVB2	263	324	0.05%	0.006%
68	11.088	3121	3125	3129	rBV	207	215	0.03%	0.004%
69	11.185	3145	3155	3178	rBV	351153	547930	78.59%	9.951%
70	11.561	3260	3272	3295	rBV	321037	505259	72.47%	9.176%
71	11.657	3299	3302	3307	rVB3	216	225	0.03%	0.004%
72	11.821	3347	3353	3356	rBV2	195	262	0.04%	0.005%
73	12.111	3439	3443	3449	rVB2	264	299	0.04%	0.005%
74	12.152	3453	3456	3461	rBV2	248	311	0.04%	0.006%
75	12.361	3517	3521	3525	rBV2	273	230	0.03%	0.004%
76	12.394	3527	3531	3534	rBV2	229	257	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033963.D
 Acq On : 02 Feb 2024 11:42
 Operator : SY/MD
 Sample : P1329-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.455	3547	3550	3553	rBV	214	180	0.03%	0.003%
78	12.487	3557	3560	3563	rBV2	235	206	0.03%	0.004%
79	12.564	3580	3584	3587	rBV	192	211	0.03%	0.004%
80	12.824	3661	3665	3668	rBV2	175	171	0.02%	0.003%
81	13.037	3727	3731	3739	rVV2	196	293	0.04%	0.005%
82	13.455	3856	3861	3867	rBV	364	407	0.06%	0.007%
83	13.622	3908	3913	3917	rBV2	345	385	0.06%	0.007%
84	13.664	3922	3926	3928	rBV2	235	201	0.03%	0.004%
85	13.712	3937	3941	3944	rVB2	353	268	0.04%	0.005%
86	13.966	4018	4020	4023	rBV	255	193	0.03%	0.004%
87	14.069	4049	4052	4056	rBV	228	237	0.03%	0.004%
88	14.104	4060	4063	4065	rVB2	318	183	0.03%	0.003%
89	14.213	4093	4097	4101	rVB2	293	265	0.04%	0.005%
90	14.349	4134	4139	4142	rBV2	203	195	0.03%	0.004%
91	14.394	4150	4153	4157	rVB2	276	261	0.04%	0.005%
92	14.416	4157	4160	4165	rBV	383	427	0.06%	0.008%
93	14.824	4285	4287	4290	rVB2	402	190	0.03%	0.003%
94	14.857	4295	4297	4301	rVB2	340	165	0.02%	0.003%
95	15.024	4346	4349	4352	rVV2	263	219	0.03%	0.004%
96	15.191	4397	4401	4402	rBV3	325	287	0.04%	0.005%
97	15.291	4430	4432	4436	rVB	494	268	0.04%	0.005%
98	15.320	4437	4441	4443	rBV	302	224	0.03%	0.004%
99	15.493	4493	4495	4498	rBV2	421	201	0.03%	0.004%
100	15.538	4506	4509	4511	rBV2	364	238	0.03%	0.004%




Sum of corrected areas: 5506554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033963.D
Acq On : 02 Feb 2024 11:42
Operator : SY/MD
Sample : P1329-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

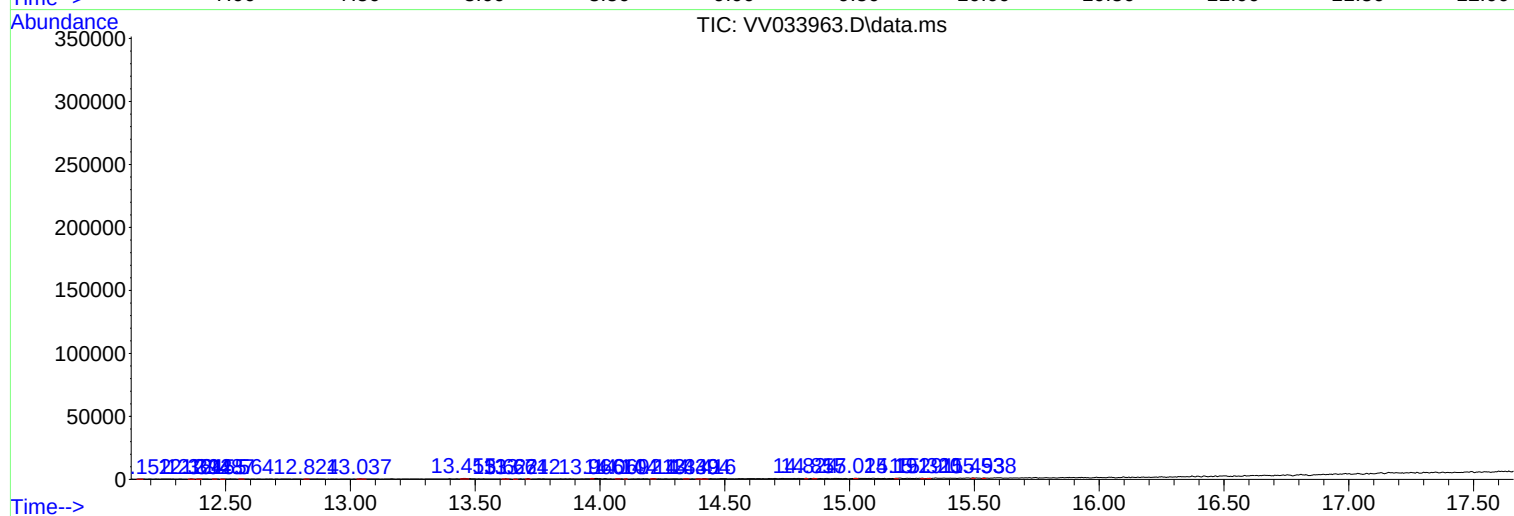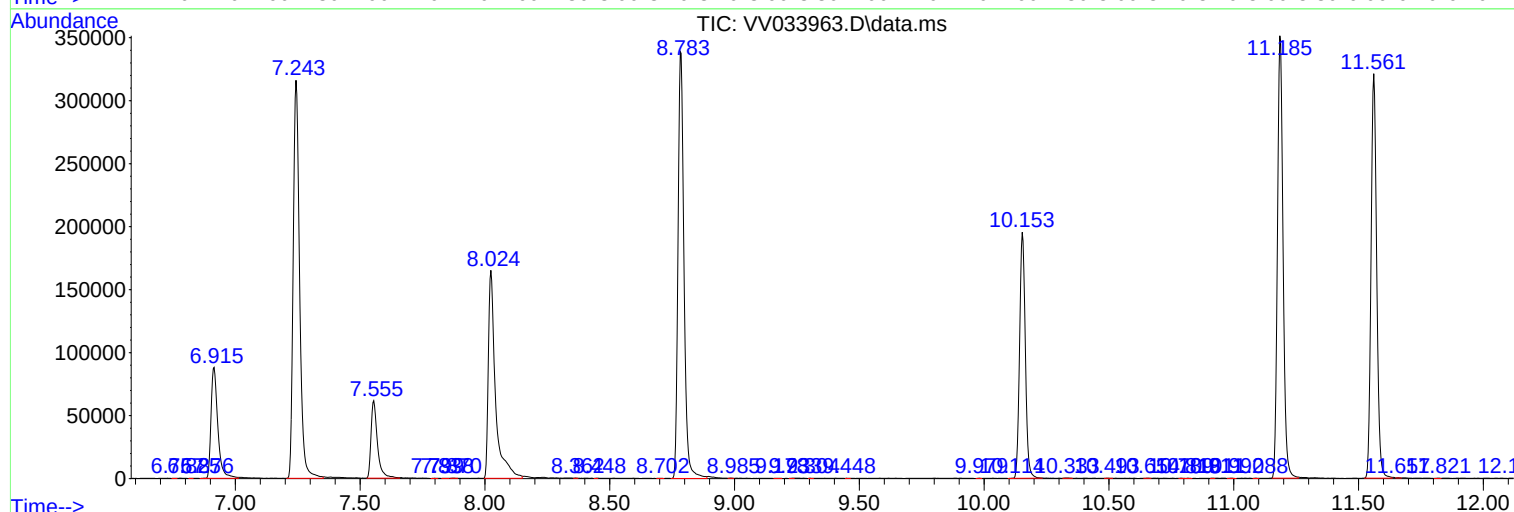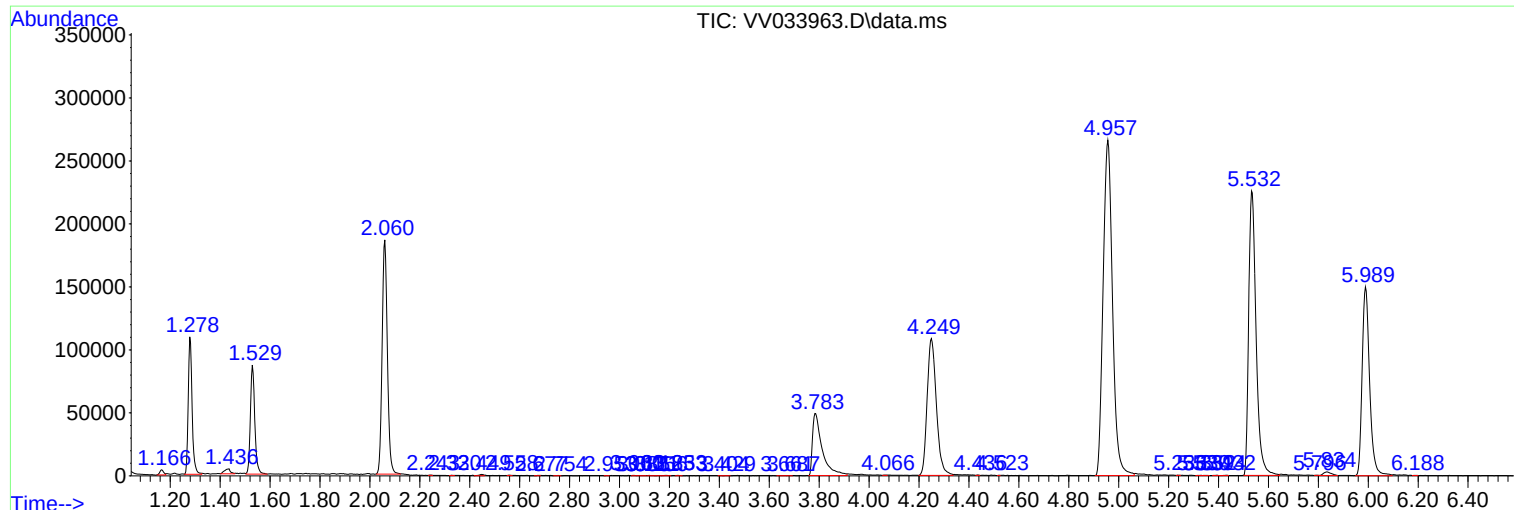

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033963.D
Acq On : 02 Feb 2024 11:42
Operator : SY/MD
Sample : P1329-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033963.D
Acq On : 02 Feb 2024 11:42
Operator : SY/MD
Sample : P1329-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc