

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033964.D
 Acq On : 02 Feb 2024 12:12
 Operator : SY/MD
 Sample : P1309-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	2059	2617	0.39%	0.050%
2	1.278	67	74	90	rBV	98488	106997	16.04%	2.028%
3	1.433	112	122	129	rBV5	5160	8328	1.25%	0.158%
4	1.529	144	152	166	rVB	78518	97179	14.57%	1.842%
5	2.056	306	316	335	rBV	174930	253940	38.06%	4.812%
6	2.240	371	373	377	rVB3	233	186	0.03%	0.004%
7	2.417	423	428	431	rVB2	177	199	0.03%	0.004%
8	2.442	431	436	447	rVB6	764	1257	0.19%	0.024%
9	2.552	463	470	478	rVB4	657	1287	0.19%	0.024%
10	2.593	478	483	485	rBV2	190	177	0.03%	0.003%
11	2.626	488	493	497	rVB2	199	257	0.04%	0.005%
12	2.764	533	536	539	rBV2	178	176	0.03%	0.003%
13	2.883	566	573	576	rVB2	231	209	0.03%	0.004%
14	3.304	700	704	709	rBV	182	228	0.03%	0.004%
15	3.658	809	814	816	rBV	167	203	0.03%	0.004%
16	3.783	845	853	898	rBV	47597	129775	19.45%	2.459%
17	4.246	982	997	1027	rBV2	102675	261318	39.17%	4.952%
18	4.526	1079	1084	1088	rBV2	282	268	0.04%	0.005%
19	4.558	1091	1094	1096	rBV	330	237	0.04%	0.004%
20	4.641	1114	1120	1122	rBV2	232	238	0.04%	0.005%
21	4.744	1149	1152	1155	rBV2	307	316	0.05%	0.006%
22	4.767	1157	1159	1162	rVB2	297	192	0.03%	0.004%
23	4.799	1166	1169	1172	rVB2	278	201	0.03%	0.004%
24	4.838	1176	1181	1183	rBV	162	178	0.03%	0.003%
25	4.953	1201	1217	1248	rBV2	251688	667149	100.00%	12.642%
26	5.249	1306	1309	1313	rVB2	367	309	0.05%	0.006%
27	5.378	1346	1349	1351	rBV	320	207	0.03%	0.004%
28	5.484	1380	1382	1386	rVB2	340	216	0.03%	0.004%
29	5.532	1386	1397	1425	rBV	214201	439874	65.93%	8.335%
30	5.776	1470	1473	1476	rVB	264	177	0.03%	0.003%
31	5.834	1482	1491	1503	rVB6	2821	6026	0.90%	0.114%
32	5.931	1516	1521	1525	rBV3	402	530	0.08%	0.010%
33	5.989	1525	1539	1569	rVV	141633	296674	44.47%	5.622%
34	6.169	1593	1595	1599	rVB	234	178	0.03%	0.003%
35	6.211	1604	1608	1612	rVB2	235	193	0.03%	0.004%
36	6.378	1657	1660	1668	rBV	201	250	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033964.D
 Acq On : 02 Feb 2024 12:12
 Operator : SY/MD
 Sample : P1309-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.416	1668	1672	1677	rBV	236	318	0.05%	0.006%
38	6.609	1725	1732	1734	rBV	169	210	0.03%	0.004%
39	6.680	1750	1754	1758	rBV2	228	229	0.03%	0.004%
40	6.767	1777	1781	1784	rBV2	196	198	0.03%	0.004%
41	6.912	1817	1826	1853	rBV	84988	160158	24.01%	3.035%
42	7.140	1891	1897	1898	rBV	333	398	0.06%	0.008%
43	7.243	1917	1929	1965	rBV	302724	536726	80.45%	10.171%
44	7.555	2014	2026	2055	rBV2	58096	107586	16.13%	2.039%
45	7.735	2080	2082	2087	rVB3	277	177	0.03%	0.003%
46	7.760	2087	2090	2092	rBV2	356	232	0.03%	0.004%
47	7.870	2120	2124	2126	rBV	261	209	0.03%	0.004%
48	7.969	2153	2155	2160	rVB2	305	285	0.04%	0.005%
49	8.024	2161	2172	2215	rBV	156622	314966	47.21%	5.969%
50	8.214	2229	2231	2234	rBV2	361	261	0.04%	0.005%
51	8.503	2317	2321	2325	rBV	192	230	0.03%	0.004%
52	8.625	2356	2359	2362	rBV2	236	191	0.03%	0.004%
53	8.654	2365	2368	2371	rBV2	205	180	0.03%	0.003%
54	8.783	2396	2408	2437	rBV	323538	536111	80.36%	10.159%
55	9.014	2475	2480	2483	rBV2	196	229	0.03%	0.004%
56	9.159	2521	2525	2530	rBV2	179	244	0.04%	0.005%
57	9.181	2530	2532	2541	rVB	237	264	0.04%	0.005%
58	9.223	2541	2545	2550	rVB2	184	171	0.03%	0.003%
59	9.493	2627	2629	2634	rVB	187	174	0.03%	0.003%
60	9.657	2674	2680	2683	rBV	257	315	0.05%	0.006%
61	9.744	2703	2707	2711	rBV	200	240	0.04%	0.005%
62	9.831	2730	2734	2737	rBV2	148	175	0.03%	0.003%
63	9.882	2746	2750	2753	rBV2	177	182	0.03%	0.003%
64	9.976	2776	2779	2785	rBV2	168	230	0.03%	0.004%
65	10.153	2823	2834	2859	rVV	190751	300635	45.06%	5.697%
66	10.326	2885	2888	2891	rVB	287	186	0.03%	0.004%
67	10.358	2891	2898	2901	rBV2	166	210	0.03%	0.004%
68	10.474	2932	2934	2939	rBV2	165	168	0.03%	0.003%
69	10.632	2980	2983	2990	rBV2	209	299	0.04%	0.006%
70	10.985	3090	3093	3102	rVB2	275	324	0.05%	0.006%
71	11.140	3136	3141	3144	rBV2	183	240	0.04%	0.005%
72	11.185	3144	3155	3184	rVV	350787	536410	80.40%	10.165%
73	11.288	3184	3187	3190	rVV2	392	259	0.04%	0.005%
74	11.500	3251	3253	3257	rVB2	250	165	0.02%	0.003%
75	11.561	3261	3272	3300	rVV	310790	489843	73.42%	9.282%
76	12.030	3415	3418	3424	rBV2	210	196	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033964.D
 Acq On : 02 Feb 2024 12:12
 Operator : SY/MD
 Sample : P1309-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.120	3441	3446	3453	rVB2	205	294	0.04%	0.006%
78	12.339	3506	3514	3520	rBV2	261	433	0.06%	0.008%
79	12.506	3562	3566	3571	rBV	4674	3739	0.56%	0.071%
80	12.587	3588	3591	3598	rBV2	178	223	0.03%	0.004%
81	12.648	3603	3610	3613	rBV2	225	273	0.04%	0.005%
82	12.744	3638	3640	3647	rVB2	251	269	0.04%	0.005%
83	12.786	3647	3653	3655	rBV2	230	234	0.04%	0.004%
84	12.911	3689	3692	3696	rBV2	225	229	0.03%	0.004%
85	13.027	3725	3728	3733	rVV2	162	175	0.03%	0.003%
86	13.156	3761	3768	3771	rVB2	244	315	0.05%	0.006%
87	13.191	3774	3779	3783	rVB2	244	256	0.04%	0.005%
88	13.230	3786	3791	3792	rBV2	279	242	0.04%	0.005%
89	13.294	3804	3811	3812	rBV	217	249	0.04%	0.005%
90	13.403	3841	3845	3847	rBV	234	195	0.03%	0.004%
91	13.779	3957	3962	3966	rBV2	266	243	0.04%	0.005%
92	14.017	4033	4036	4041	rVB	310	212	0.03%	0.004%
93	14.120	4065	4068	4071	rVB2	275	180	0.03%	0.003%
94	14.149	4074	4077	4080	rVB2	350	229	0.03%	0.004%
95	14.217	4095	4098	4100	rBV	280	184	0.03%	0.003%
96	14.303	4122	4125	4128	rBV2	252	186	0.03%	0.004%
97	14.545	4197	4200	4203	rVB2	292	209	0.03%	0.004%
98	14.564	4203	4206	4208	rBV3	217	170	0.03%	0.003%
99	15.474	4486	4489	4491	rBV	378	217	0.03%	0.004%
100	15.557	4510	4515	4518	rBV3	501	595	0.09%	0.011%




Sum of corrected areas: 5277121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033964.D
Acq On : 02 Feb 2024 12:12
Operator : SY/MD
Sample : P1309-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

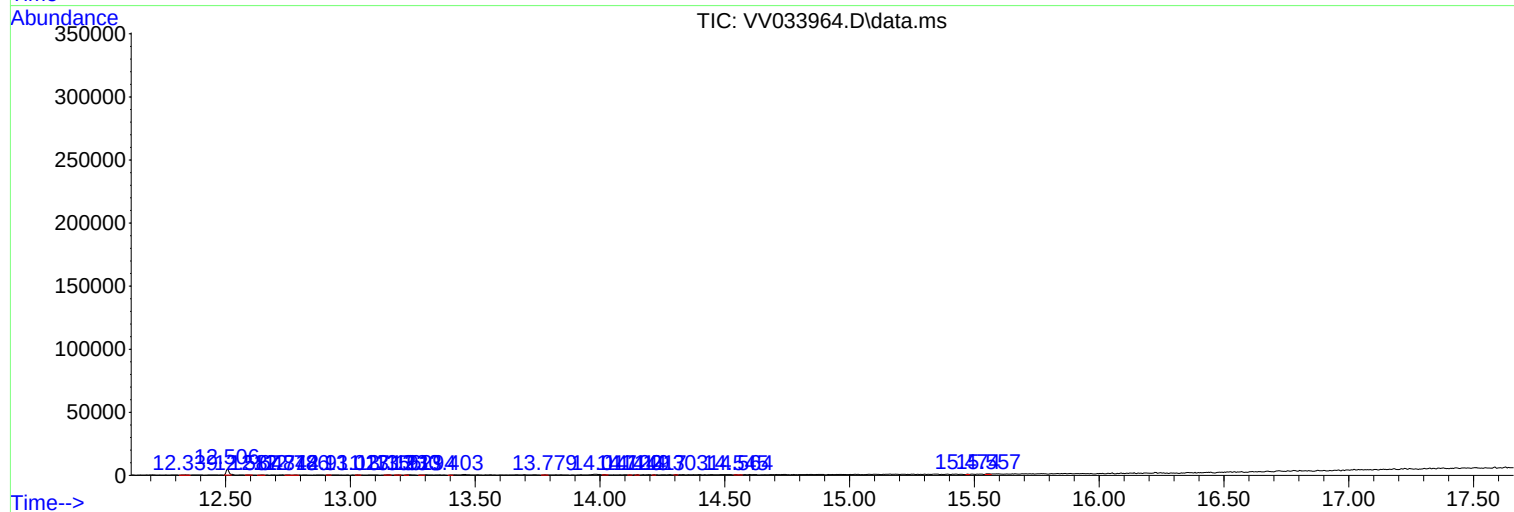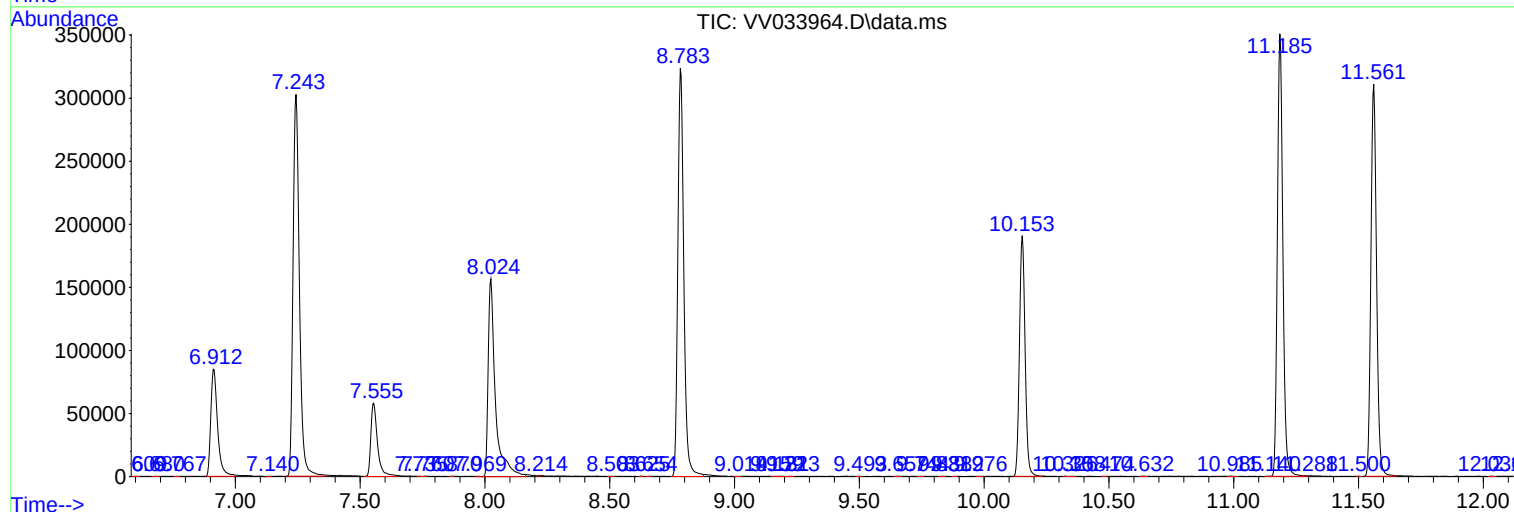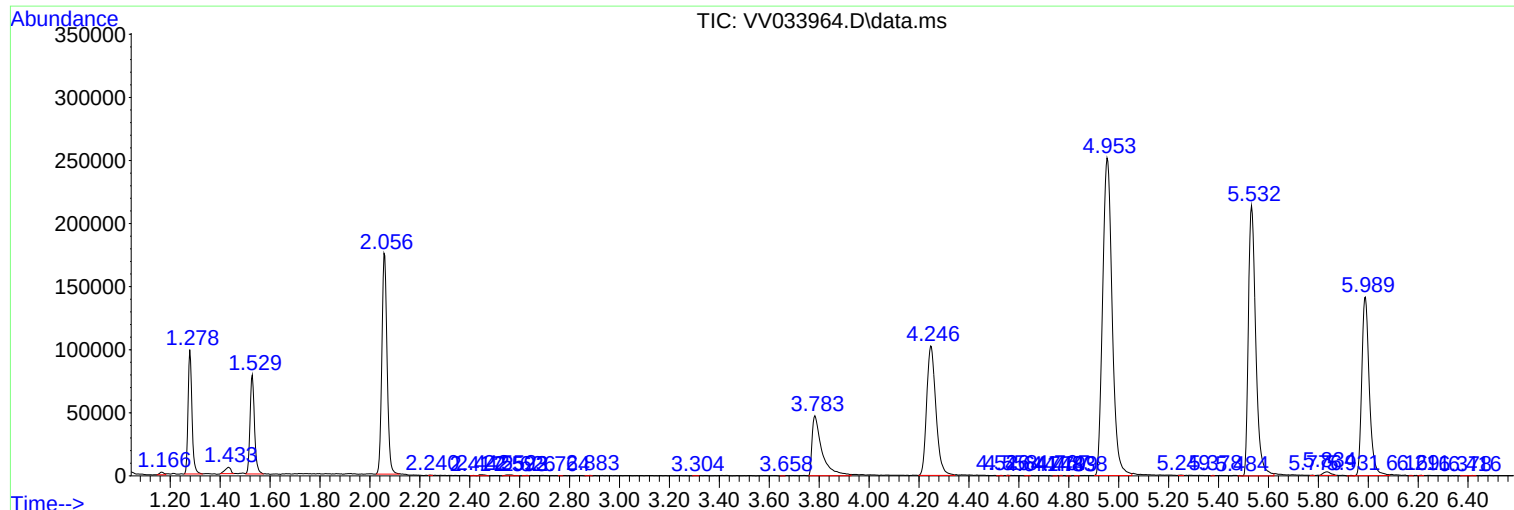

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033964.D
Acq On : 02 Feb 2024 12:12
Operator : SY/MD
Sample : P1309-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033964.D
Acq On : 02 Feb 2024 12:12
Operator : SY/MD
Sample : P1309-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------