

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033967.D
 Acq On : 02 Feb 2024 14:04
 Operator : SY/MD
 Sample : P1348-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	4021	5069	0.71%	0.087%
2	1.278	67	74	88	rBV	112218	121941	16.97%	2.088%
3	1.426	114	120	131	rVB4	3619	5479	0.76%	0.094%
4	1.529	144	152	172	rVB	88049	110942	15.44%	1.900%
5	1.979	290	292	293	rBV2	460	192	0.03%	0.003%
6	2.060	306	317	340	rBV	194372	285890	39.80%	4.896%
7	2.227	361	369	382	rVB2	1960	3818	0.53%	0.065%
8	2.400	419	423	427	rBV2	170	171	0.02%	0.003%
9	2.449	435	438	440	rBV	381	305	0.04%	0.005%
10	2.558	462	472	483	rVV4	1182	2520	0.35%	0.043%
11	2.770	534	538	542	rVB	313	340	0.05%	0.006%
12	2.793	542	545	546	rBV	292	190	0.03%	0.003%
13	2.835	556	558	563	rVB	157	154	0.02%	0.003%
14	2.905	575	580	581	rBV2	148	152	0.02%	0.003%
15	2.970	597	600	605	rBV	228	220	0.03%	0.004%
16	3.182	663	666	671	rVB2	297	271	0.04%	0.005%
17	3.207	671	674	676	rBV	268	192	0.03%	0.003%
18	3.285	695	698	702	rBV2	145	166	0.02%	0.003%
19	3.461	745	753	757	rBV2	188	255	0.04%	0.004%
20	3.622	799	803	805	rBV	153	159	0.02%	0.003%
21	3.667	812	817	823	rVB2	338	427	0.06%	0.007%
22	3.783	844	853	884	rBV	51976	141785	19.74%	2.428%
23	4.130	958	961	966	rVB3	249	277	0.04%	0.005%
24	4.156	966	969	972	rBV2	218	207	0.03%	0.004%
25	4.249	982	998	1024	rBV	112333	285475	39.74%	4.889%
26	4.539	1085	1088	1090	rBV	249	177	0.02%	0.003%
27	4.584	1100	1102	1105	rVV	272	181	0.03%	0.003%
28	4.629	1112	1116	1120	rBV2	260	330	0.05%	0.006%
29	4.957	1202	1218	1249	rBV2	273245	718359	100.00%	12.302%
30	5.178	1284	1287	1289	rBV2	281	228	0.03%	0.004%
31	5.227	1300	1302	1305	rVB3	323	183	0.03%	0.003%
32	5.291	1318	1322	1325	rVB2	220	175	0.02%	0.003%
33	5.387	1348	1352	1355	rBV2	296	284	0.04%	0.005%
34	5.410	1355	1359	1361	rVB2	205	158	0.02%	0.003%
35	5.532	1386	1397	1438	rBV	258828	528632	73.59%	9.053%
36	5.834	1481	1491	1509	rVB6	3060	6998	0.97%	0.120%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033967.D
 Acq On : 02 Feb 2024 14:04
 Operator : SY/MD
 Sample : P1348-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1564	rBV	151175	316415	44.05%	5.418%
38	6.542	1707	1711	1716	rBV2	285	284	0.04%	0.005%
39	6.616	1730	1734	1740	rVB2	213	276	0.04%	0.005%
40	6.648	1740	1744	1746	rBV	181	171	0.02%	0.003%
41	6.764	1777	1780	1784	rBV2	193	188	0.03%	0.003%
42	6.828	1796	1800	1804	rBV2	165	185	0.03%	0.003%
43	6.912	1816	1826	1851	rBV	92437	171323	23.85%	2.934%
44	7.124	1889	1892	1893	rBV	273	160	0.02%	0.003%
45	7.243	1918	1929	1960	rBV	329496	584486	81.36%	10.009%
46	7.555	2014	2026	2050	rBV	63016	113500	15.80%	1.944%
47	7.764	2086	2091	2094	rVB2	171	194	0.03%	0.003%
48	7.866	2121	2123	2126	rBV2	203	160	0.02%	0.003%
49	8.024	2160	2172	2206	rBV	164416	322450	44.89%	5.522%
50	8.317	2259	2263	2266	rBV	275	273	0.04%	0.005%
51	8.439	2298	2301	2305	rVB2	419	299	0.04%	0.005%
52	8.783	2397	2408	2431	rBV	381461	630396	87.76%	10.795%
53	9.095	2503	2505	2512	rVB2	174	164	0.02%	0.003%
54	9.439	2609	2612	2616	rVB2	209	161	0.02%	0.003%
55	9.471	2616	2622	2626	rBV2	219	222	0.03%	0.004%
56	9.786	2716	2720	2727	rVB2	195	276	0.04%	0.005%
57	9.828	2729	2733	2737	rBV2	159	202	0.03%	0.003%
58	9.876	2742	2748	2753	rVB2	233	302	0.04%	0.005%
59	9.940	2765	2768	2772	rVB	193	163	0.02%	0.003%
60	9.972	2772	2778	2781	rBV2	207	280	0.04%	0.005%
61	10.153	2823	2834	2863	rBV	198472	310795	43.26%	5.322%
62	10.272	2867	2871	2874	rBV2	242	161	0.02%	0.003%
63	10.329	2884	2889	2893	rVB2	297	329	0.05%	0.006%
64	10.368	2898	2901	2903	rBV	225	184	0.03%	0.003%
65	10.551	2953	2958	2963	rBV2	208	233	0.03%	0.004%
66	10.612	2974	2977	2984	rBV2	162	247	0.03%	0.004%
67	10.661	2988	2992	2995	rBV2	186	177	0.02%	0.003%
68	10.757	3019	3022	3025	rBV	275	256	0.04%	0.004%
69	10.780	3025	3029	3034	rVV	205	295	0.04%	0.005%
70	10.985	3086	3093	3098	rVB2	216	342	0.05%	0.006%
71	11.014	3098	3102	3108	rBV2	235	269	0.04%	0.005%
72	11.185	3144	3155	3182	rBV	413832	630595	87.78%	10.799%
73	11.561	3258	3272	3297	rBV	332418	523891	72.93%	8.971%
74	11.661	3301	3303	3311	rVB2	684	570	0.08%	0.010%
75	11.725	3321	3323	3325	rBV	289	152	0.02%	0.003%
76	11.763	3332	3335	3338	rBV2	178	171	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033967.D
 Acq On : 02 Feb 2024 14:04
 Operator : SY/MD
 Sample : P1348-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.834	3354	3357	3362	rVB2	193	196	0.03%	0.003%
78	11.886	3371	3373	3379	rVB2	278	228	0.03%	0.004%
79	11.918	3379	3383	3387	rBV	177	172	0.02%	0.003%
80	11.940	3387	3390	3392	rBV2	192	159	0.02%	0.003%
81	12.197	3467	3470	3475	rVV2	210	183	0.03%	0.003%
82	12.394	3529	3531	3534	rBV	207	165	0.02%	0.003%
83	12.561	3580	3583	3585	rBV	195	165	0.02%	0.003%
84	12.757	3640	3644	3646	rBV2	162	156	0.02%	0.003%
85	12.815	3658	3662	3666	rVB	242	212	0.03%	0.004%
86	12.841	3666	3670	3676	rBV2	274	292	0.04%	0.005%
87	12.969	3706	3710	3713	rBV	179	180	0.03%	0.003%
88	13.596	3901	3905	3907	rBV	231	197	0.03%	0.003%
89	14.037	4039	4042	4044	rBV2	240	164	0.02%	0.003%
90	14.159	4076	4080	4083	rBV2	357	347	0.05%	0.006%
91	14.220	4094	4099	4101	rBV2	373	391	0.05%	0.007%
92	14.320	4127	4130	4134	rBV3	217	194	0.03%	0.003%
93	14.400	4152	4155	4159	rBV2	231	189	0.03%	0.003%
94	14.500	4184	4186	4191	rBV3	211	238	0.03%	0.004%
95	14.596	4212	4216	4219	rBV3	568	533	0.07%	0.009%
96	14.953	4322	4327	4331	rBV2	458	416	0.06%	0.007%
97	15.037	4349	4353	4356	rBV2	540	399	0.06%	0.007%
98	15.455	4480	4483	4485	rBV2	420	304	0.04%	0.005%
99	15.580	4520	4522	4527	rBV2	434	279	0.04%	0.005%
100	15.776	4580	4583	4586	rBV2	462	318	0.04%	0.005%

Sum of corrected areas: 5839576




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033967.D
Acq On : 02 Feb 2024 14:04
Operator : SY/MD
Sample : P1348-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

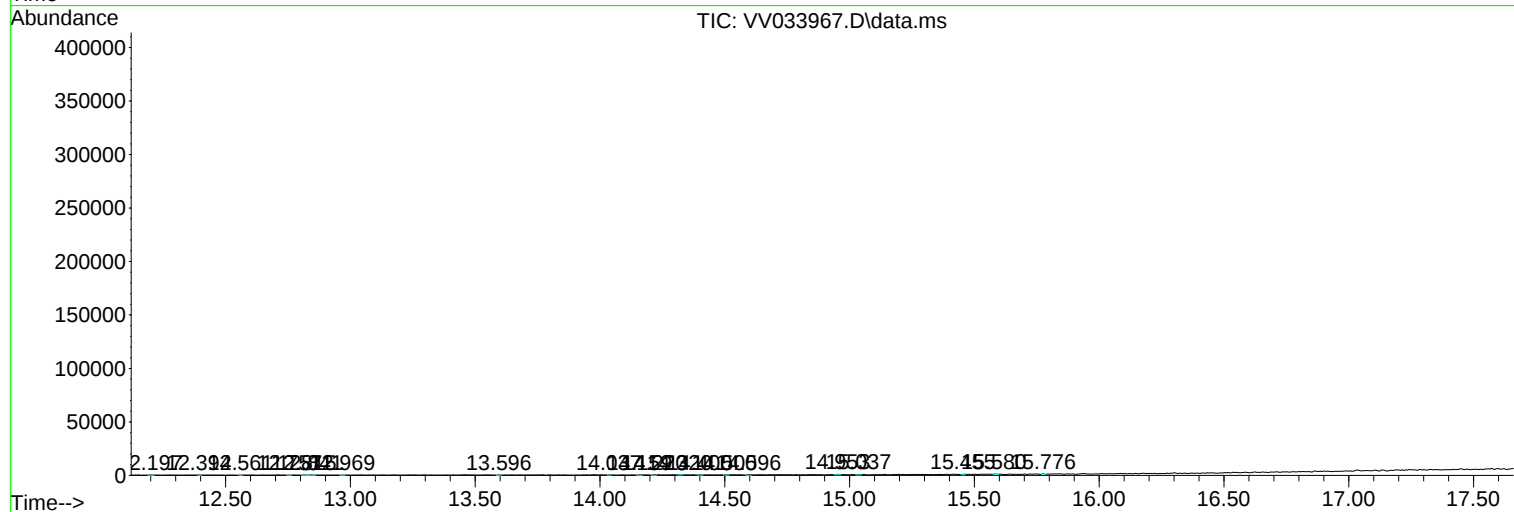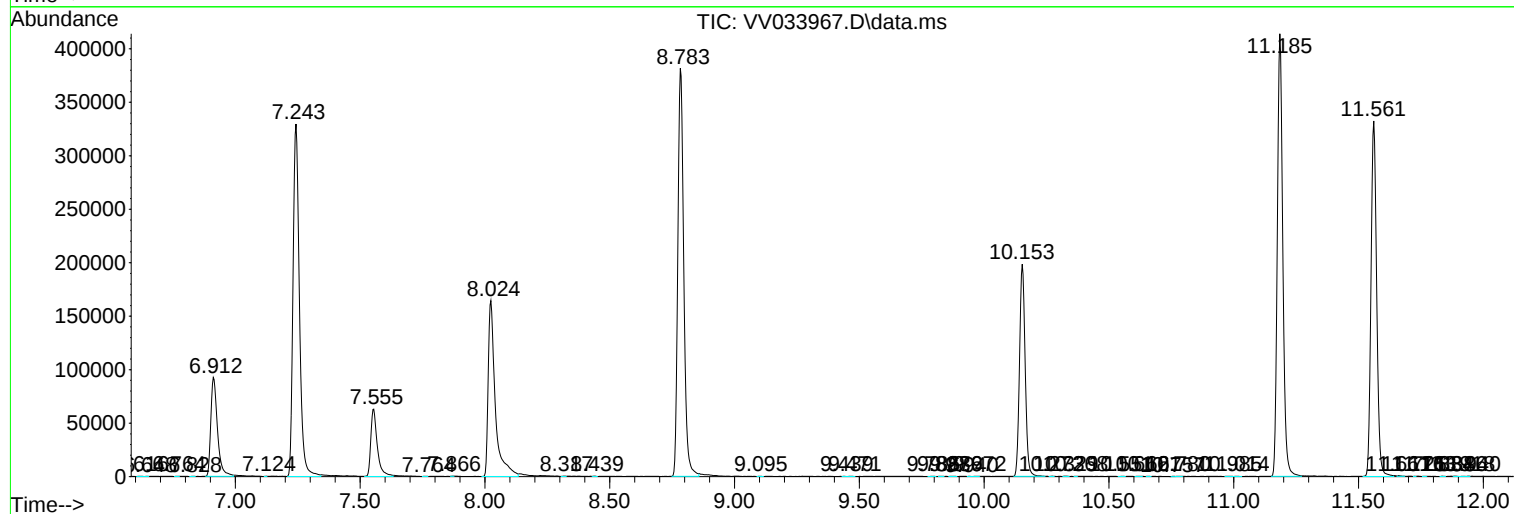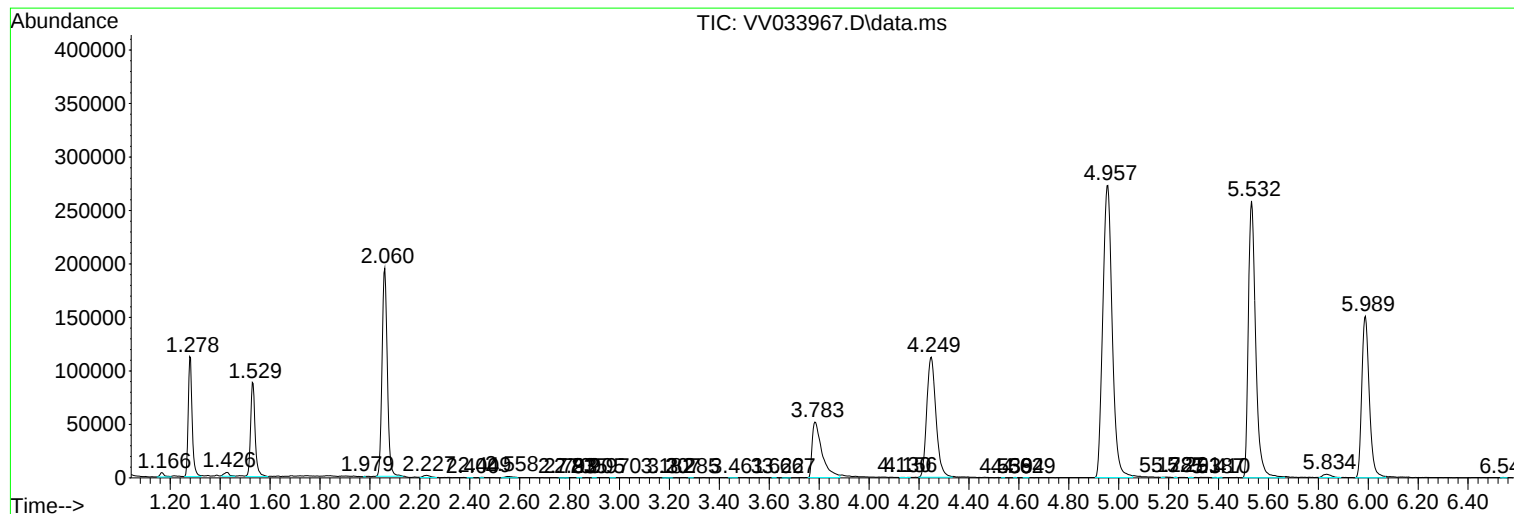

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033967.D
Acq On : 02 Feb 2024 14:04
Operator : SY/MD
Sample : P1348-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033967.D
Acq On : 02 Feb 2024 14:04
Operator : SY/MD
Sample : P1348-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc