

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033968.D
 Acq On : 02 Feb 2024 14:28
 Operator : SY/MD
 Sample : P1348-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	49	rBV	4783	5722	0.27%	0.067%
2	1.278	67	74	92	rVB	110801	119095	5.70%	1.403%
3	1.385	103	107	112	rBV	2447	2208	0.11%	0.026%
4	1.529	144	152	170	rVB	87944	107743	5.15%	1.270%
5	1.931	275	277	283	rBV3	619	550	0.03%	0.006%
6	1.999	295	298	303	rBV4	768	656	0.03%	0.008%
7	2.060	306	317	328	rBV	189654	277067	13.25%	3.265%
8	2.192	356	358	360	rVB2	422	174	0.01%	0.002%
9	2.230	363	370	372	rBV4	471	502	0.02%	0.006%
10	2.259	377	379	384	rVB2	278	194	0.01%	0.002%
11	2.413	424	427	430	rBV2	166	158	0.01%	0.002%
12	2.561	459	473	486	rVV	3757	7652	0.37%	0.090%
13	2.642	493	498	502	rBV2	167	171	0.01%	0.002%
14	2.696	509	515	519	rBV	222	319	0.02%	0.004%
15	2.796	540	546	548	rBV2	300	288	0.01%	0.003%
16	2.954	592	595	599	rVB	203	162	0.01%	0.002%
17	3.069	626	631	634	rBV	170	202	0.01%	0.002%
18	3.217	672	677	679	rBV	166	193	0.01%	0.002%
19	3.246	683	686	690	rBV2	232	222	0.01%	0.003%
20	3.465	749	754	756	rBV	283	280	0.01%	0.003%
21	3.648	810	811	817	rVB2	241	228	0.01%	0.003%
22	3.683	817	822	826	rBV2	316	407	0.02%	0.005%
23	3.786	841	854	887	rBV2	57430	166006	7.94%	1.956%
24	4.249	981	998	1027	rBV	110356	282441	13.51%	3.328%
25	4.519	1078	1082	1091	rVB3	357	358	0.02%	0.004%
26	4.690	1131	1135	1137	rBV2	249	175	0.01%	0.002%
27	4.728	1144	1147	1150	rVB2	209	150	0.01%	0.002%
28	4.957	1201	1218	1248	rBV2	270730	718481	34.37%	8.466%
29	5.301	1318	1325	1329	rVB2	292	405	0.02%	0.005%
30	5.375	1346	1348	1353	rVB2	212	202	0.01%	0.002%
31	5.423	1360	1363	1366	rBV2	250	206	0.01%	0.002%
32	5.532	1386	1397	1433	rBV	238473	489280	23.41%	5.765%
33	5.838	1483	1492	1503	rVB4	2499	5627	0.27%	0.066%
34	5.941	1521	1524	1526	rBB2	368	217	0.01%	0.003%
35	5.989	1526	1539	1561	rBV2	151857	312543	14.95%	3.683%
36	6.317	1637	1641	1644	rBV2	170	208	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033968.D
 Acq On : 02 Feb 2024 14:28
 Operator : SY/MD
 Sample : P1348-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.519	1700	1704	1706	rBV2	211	180	0.01%	0.002%
38	6.761	1775	1779	1782	rBV	179	157	0.01%	0.002%
39	6.786	1782	1787	1793	rBV2	241	317	0.02%	0.004%
40	6.915	1816	1827	1850	rBV	90528	168449	8.06%	1.985%
41	7.137	1893	1896	1899	rBV2	217	155	0.01%	0.002%
42	7.159	1899	1903	1906	rVB3	250	161	0.01%	0.002%
43	7.188	1910	1912	1914	rBV2	263	156	0.01%	0.002%
44	7.243	1918	1929	1953	rBV	326705	573012	27.41%	6.752%
45	7.555	2017	2026	2048	rBV	61801	110679	5.29%	1.304%
46	7.825	2107	2110	2112	rBV	216	147	0.01%	0.002%
47	7.879	2122	2127	2134	rVV2	375	566	0.03%	0.007%
48	8.024	2163	2172	2209	rBV	172924	334268	15.99%	3.939%
49	8.352	2272	2274	2277	rVB3	325	186	0.01%	0.002%
50	8.381	2277	2283	2285	rBV2	183	238	0.01%	0.003%
51	8.683	2373	2377	2382	rVB2	193	223	0.01%	0.003%
52	8.783	2397	2408	2446	rBV2	363072	751842	35.97%	8.859%
53	9.108	2505	2509	2513	rBV2	176	230	0.01%	0.003%
54	9.143	2516	2520	2522	rBV2	205	167	0.01%	0.002%
55	9.416	2601	2605	2609	rVB	308	286	0.01%	0.003%
56	9.449	2610	2615	2616	rBV2	234	191	0.01%	0.002%
57	9.709	2691	2696	2701	rBV2	178	306	0.01%	0.004%
58	9.818	2727	2730	2735	rBV2	200	224	0.01%	0.003%
59	9.992	2779	2784	2787	rBV2	192	234	0.01%	0.003%
60	10.075	2806	2810	2812	rBV2	174	146	0.01%	0.002%
61	10.153	2823	2834	2856	rBV	201941	315530	15.09%	3.718%
62	10.500	2938	2942	2944	rBV2	326	278	0.01%	0.003%
63	10.635	2980	2984	2986	rVB	191	149	0.01%	0.002%
64	10.844	3043	3049	3056	rBV2	208	406	0.02%	0.005%
65	10.911	3064	3070	3072	rBV2	192	188	0.01%	0.002%
66	11.120	3125	3135	3145	rBV2	42675	66513	3.18%	0.784%
67	11.185	3145	3155	3181	rVB2	398192	717421	34.32%	8.453%
68	11.413	3224	3226	3229	rVB	368	254	0.01%	0.003%
69	11.458	3235	3240	3245	rBV2	163	200	0.01%	0.002%
70	11.577	3254	3277	3297	rBV2	1078390	2090420	100.00%	24.631%
71	11.767	3333	3336	3339	rBV3	190	165	0.01%	0.002%
72	12.046	3420	3423	3425	rVV2	243	193	0.01%	0.002%
73	12.082	3429	3434	3437	rVB2	236	199	0.01%	0.002%
74	12.339	3510	3514	3520	rBV2	216	238	0.01%	0.003%
75	12.407	3533	3535	3540	rVB2	257	240	0.01%	0.003%
76	12.432	3540	3543	3545	rBV	220	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033968.D
 Acq On : 02 Feb 2024 14:28
 Operator : SY/MD
 Sample : P1348-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.538	3571	3576	3578	rBV	159	174	0.01%	0.002%
78	12.583	3581	3590	3606	rVV3	9794	17940	0.86%	0.211%
79	12.664	3613	3615	3617	rVV	312	166	0.01%	0.002%
80	12.693	3617	3624	3630	rVB6	1832	2542	0.12%	0.030%
81	12.854	3670	3674	3676	rBV2	206	190	0.01%	0.002%
82	12.879	3679	3682	3689	rVV2	178	254	0.01%	0.003%
83	13.088	3742	3747	3750	rVB2	192	204	0.01%	0.002%
84	13.198	3770	3781	3809	rBV	348804	521860	24.96%	6.149%
85	13.345	3824	3827	3833	rVB	290	275	0.01%	0.003%
86	13.374	3833	3836	3843	rVB2	220	212	0.01%	0.002%
87	13.455	3855	3861	3870	rBV2	731	1168	0.06%	0.014%
88	13.554	3886	3892	3893	rBV2	150	163	0.01%	0.002%
89	13.622	3910	3913	3916	rBV2	191	169	0.01%	0.002%
90	13.680	3920	3931	3950	rVV	166569	252928	12.10%	2.980%
91	13.792	3964	3966	3971	rVB	247	161	0.01%	0.002%
92	14.098	4052	4061	4069	rBV7	2026	3661	0.18%	0.043%
93	14.214	4095	4097	4100	rBV	278	169	0.01%	0.002%
94	14.310	4123	4127	4135	rBV	398	627	0.03%	0.007%
95	14.410	4154	4158	4163	rBV3	306	351	0.02%	0.004%
96	14.448	4167	4170	4175	rBV3	205	190	0.01%	0.002%
97	14.490	4180	4183	4187	rBV	182	193	0.01%	0.002%
98	14.760	4257	4267	4279	rBV4	5153	8866	0.42%	0.104%
99	15.046	4352	4356	4357	rBV2	484	334	0.02%	0.004%
100	15.336	4436	4446	4459	rBV2	25677	38583	1.85%	0.455%




Sum of corrected areas: 8486953

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033968.D
Acq On : 02 Feb 2024 14:28
Operator : SY/MD
Sample : P1348-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

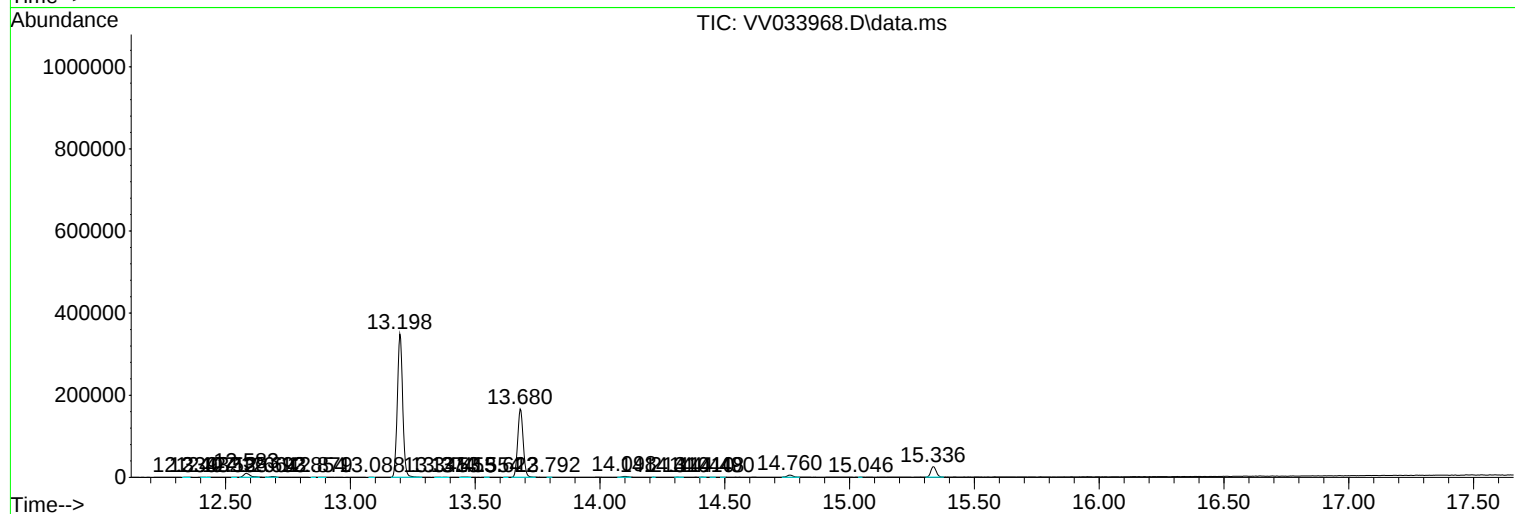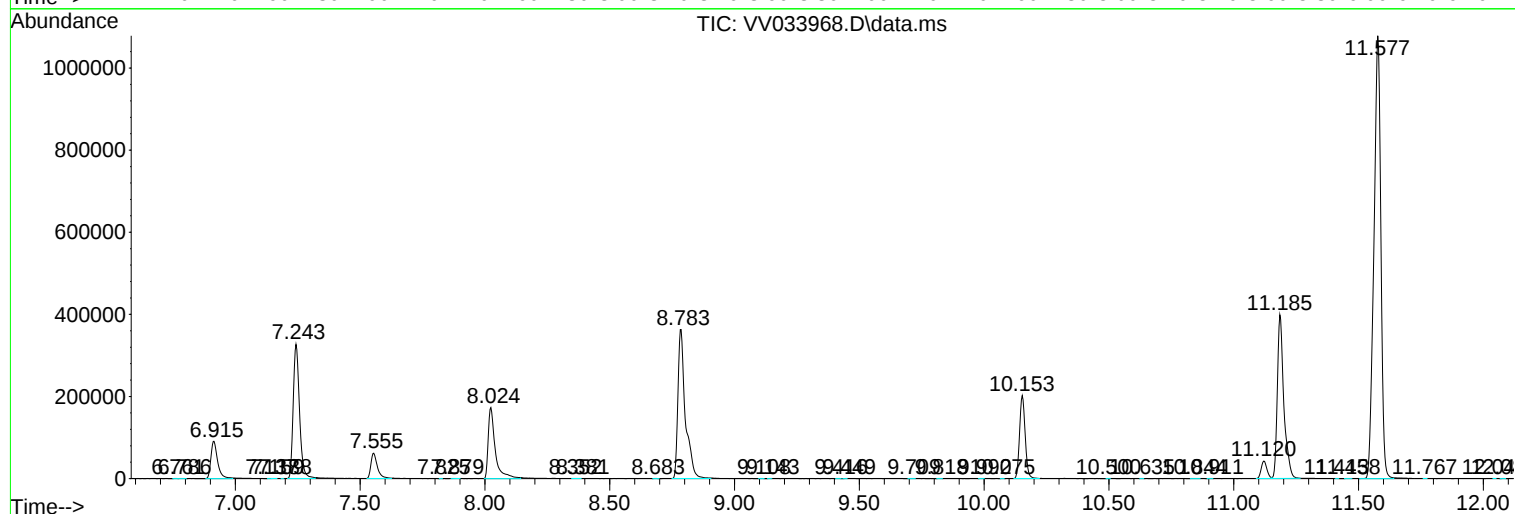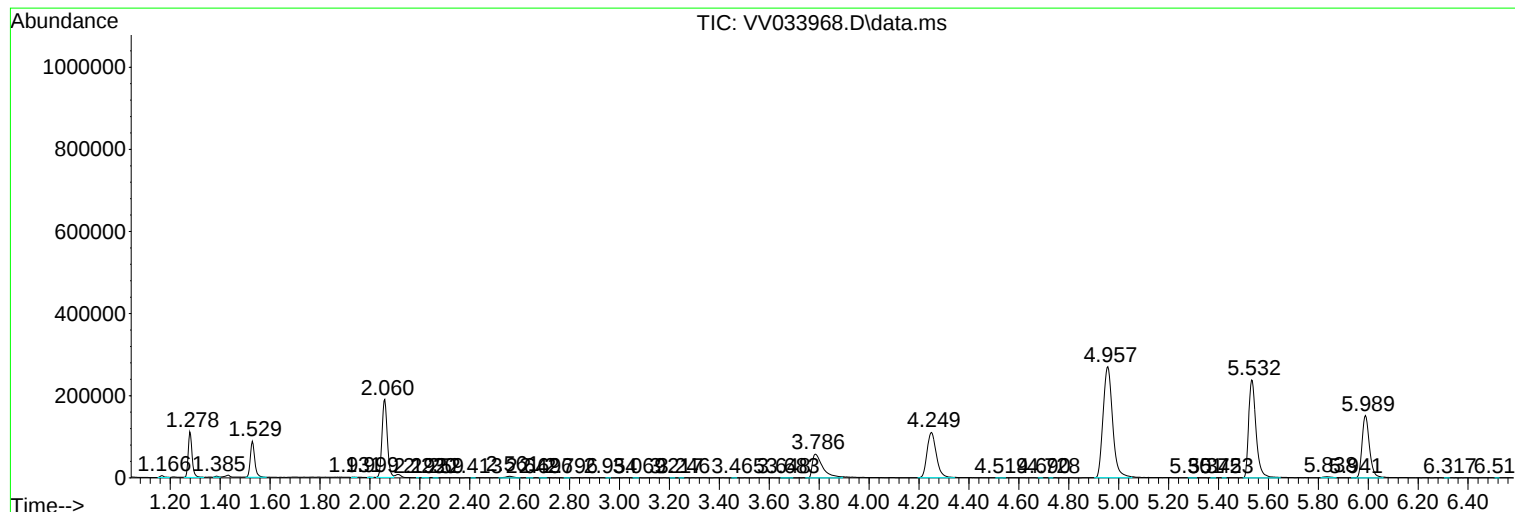

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033968.D
Acq On : 02 Feb 2024 14:28
Operator : SY/MD
Sample : P1348-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033968.D
Acq On : 02 Feb 2024 14:28
Operator : SY/MD
Sample : P1348-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc