

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033969.D
 Acq On : 02 Feb 2024 14:52
 Operator : SY/MD
 Sample : P1348-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	4398	4428	0.61%	0.078%
2	1.217	50	55	58	rBV2	1255	1080	0.15%	0.019%
3	1.278	67	74	87	rBV	112293	120293	16.64%	2.107%
4	1.430	115	121	128	rVB4	4290	5084	0.70%	0.089%
5	1.529	144	152	168	rVB	90127	109420	15.14%	1.917%
6	2.060	306	317	346	rVB	196637	291299	40.30%	5.103%
7	2.224	361	368	387	rVB2	2299	4457	0.62%	0.078%
8	2.446	433	437	439	rBV	302	180	0.02%	0.003%
9	2.487	447	450	453	rBV	196	193	0.03%	0.003%
10	2.590	479	482	490	rBV2	193	356	0.05%	0.006%
11	2.709	514	519	523	rBV	146	213	0.03%	0.004%
12	3.008	608	612	617	rBV	225	222	0.03%	0.004%
13	3.246	682	686	689	rBV2	203	189	0.03%	0.003%
14	3.619	799	802	806	rVB	295	274	0.04%	0.005%
15	3.677	817	820	826	rVB	212	210	0.03%	0.004%
16	3.783	843	853	893	rBV	50804	139081	19.24%	2.436%
17	4.249	982	998	1024	rBV	111919	286110	39.58%	5.012%
18	4.510	1075	1079	1080	rVB	357	231	0.03%	0.004%
19	4.523	1080	1083	1086	rBV	373	246	0.03%	0.004%
20	4.568	1093	1097	1101	rBV2	199	215	0.03%	0.004%
21	4.780	1160	1163	1167	rBV2	162	189	0.03%	0.003%
22	4.957	1201	1218	1244	rBV2	276379	722819	100.00%	12.661%
23	5.140	1273	1275	1282	rVB3	325	364	0.05%	0.006%
24	5.474	1376	1379	1381	rVB2	326	188	0.03%	0.003%
25	5.487	1381	1383	1386	rBV	229	175	0.02%	0.003%
26	5.535	1386	1398	1430	rBV	234945	481503	66.61%	8.434%
27	5.693	1445	1447	1456	rVB2	392	449	0.06%	0.008%
28	5.796	1477	1479	1482	rBV2	258	178	0.02%	0.003%
29	5.838	1482	1492	1507	rVB4	2930	6639	0.92%	0.116%
30	5.902	1507	1512	1515	rBV3	204	232	0.03%	0.004%
31	5.989	1526	1539	1567	rBV	152235	314486	43.51%	5.509%
32	6.146	1585	1588	1590	rBV3	301	204	0.03%	0.004%
33	6.433	1675	1677	1680	rVB	314	179	0.02%	0.003%
34	6.455	1681	1684	1688	rVB2	278	241	0.03%	0.004%
35	6.709	1757	1763	1766	rBV2	181	227	0.03%	0.004%
36	6.767	1778	1781	1785	rBV2	150	177	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033969.D
 Acq On : 02 Feb 2024 14:52
 Operator : SY/MD
 Sample : P1348-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.828	1797	1800	1804	rBV2	192	175	0.02%	0.003%
38	6.912	1816	1826	1857	rBV	90553	167364	23.15%	2.932%
39	7.092	1878	1882	1883	rBV	263	207	0.03%	0.004%
40	7.156	1900	1902	1909	rVB2	429	340	0.05%	0.006%
41	7.201	1910	1916	1918	rBV2	182	216	0.03%	0.004%
42	7.243	1918	1929	1964	rBV	327321	575460	79.61%	10.080%
43	7.555	2016	2026	2049	rBV	62317	108926	15.07%	1.908%
44	8.024	2161	2172	2216	rBV	170512	334347	46.26%	5.857%
45	8.288	2250	2254	2260	rBV3	344	381	0.05%	0.007%
46	8.416	2292	2294	2299	rVB2	276	220	0.03%	0.004%
47	8.490	2313	2317	2321	rVB2	252	203	0.03%	0.004%
48	8.783	2397	2408	2434	rBV	349359	574416	79.47%	10.062%
49	8.966	2461	2465	2468	rBV2	237	235	0.03%	0.004%
50	9.018	2477	2481	2487	rVB2	462	384	0.05%	0.007%
51	9.330	2573	2578	2580	rBV	199	191	0.03%	0.003%
52	9.471	2615	2622	2627	rBV2	232	338	0.05%	0.006%
53	9.657	2675	2680	2683	rBV	309	360	0.05%	0.006%
54	9.683	2683	2688	2692	rVB2	234	315	0.04%	0.006%
55	10.153	2823	2834	2852	rBV	202512	317381	43.91%	5.559%
56	10.313	2879	2884	2885	rBV	265	209	0.03%	0.004%
57	10.545	2951	2956	2962	rBV2	171	281	0.04%	0.005%
58	10.767	3020	3025	3027	rBV2	192	223	0.03%	0.004%
59	10.911	3067	3070	3074	rBV2	172	186	0.03%	0.003%
60	11.095	3122	3127	3128	rBV	237	192	0.03%	0.003%
61	11.130	3135	3138	3140	rBV	291	208	0.03%	0.004%
62	11.185	3144	3155	3181	rVV	362992	563052	77.90%	9.863%
63	11.275	3181	3183	3187	rVB2	523	360	0.05%	0.006%
64	11.333	3199	3201	3206	rVB3	407	287	0.04%	0.005%
65	11.445	3233	3236	3240	rBV2	234	249	0.03%	0.004%
66	11.561	3260	3272	3295	rVV	324566	529983	73.32%	9.283%
67	11.725	3321	3323	3331	rVB3	293	334	0.05%	0.006%
68	12.114	3438	3444	3446	rBV	200	221	0.03%	0.004%
69	12.223	3475	3478	3483	rBV2	197	265	0.04%	0.005%
70	12.635	3603	3606	3609	rVB2	301	190	0.03%	0.003%
71	12.661	3609	3614	3621	rBV2	287	419	0.06%	0.007%
72	12.837	3663	3669	3672	rBV	154	208	0.03%	0.004%
73	12.947	3700	3703	3708	rBV2	151	199	0.03%	0.003%
74	12.995	3714	3718	3722	rBV2	248	283	0.04%	0.005%
75	13.127	3757	3759	3763	rVB	335	223	0.03%	0.004%
76	13.149	3763	3766	3769	rBV2	180	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033969.D
 Acq On : 02 Feb 2024 14:52
 Operator : SY/MD
 Sample : P1348-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	13.204	3775	3783	3793	rBV2	10894	16151	2.23%	0.283%
78	13.349	3823	3828	3830	rBV	227	218	0.03%	0.004%
79	13.413	3843	3848	3850	rBV	205	204	0.03%	0.004%
80	13.509	3875	3878	3884	rBV	243	310	0.04%	0.005%
81	13.686	3925	3933	3943	rBV3	5890	9073	1.26%	0.159%
82	13.866	3987	3989	3995	rVB2	277	260	0.04%	0.005%
83	13.895	3995	3998	4000	rBV2	318	236	0.03%	0.004%
84	13.934	4007	4010	4012	rBV2	325	236	0.03%	0.004%
85	13.950	4012	4015	4019	rVB2	317	249	0.03%	0.004%
86	13.989	4019	4027	4034	rBV2	398	714	0.10%	0.013%
87	14.243	4102	4106	4108	rVB2	244	181	0.03%	0.003%
88	14.297	4120	4123	4126	rVB2	333	192	0.03%	0.003%
89	14.333	4126	4134	4135	rBV	324	378	0.05%	0.007%
90	14.452	4169	4171	4175	rVB	291	180	0.02%	0.003%
91	14.477	4175	4179	4180	rBV2	289	247	0.03%	0.004%
92	14.773	4267	4271	4274	rBV	278	251	0.03%	0.004%
93	14.966	4326	4331	4334	rVB2	371	358	0.05%	0.006%
94	14.988	4334	4338	4341	rBV2	427	423	0.06%	0.007%
95	15.030	4348	4351	4352	rBV2	314	200	0.03%	0.004%
96	15.149	4385	4388	4390	rBV2	323	207	0.03%	0.004%
97	15.226	4409	4412	4414	rBV	284	208	0.03%	0.004%
98	15.339	4439	4447	4457	rVB5	4787	6505	0.90%	0.114%
99	15.451	4478	4482	4485	rBV2	345	354	0.05%	0.006%
100	16.017	4656	4658	4662	rBV2	499	331	0.05%	0.006%




Sum of corrected areas: 5708904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033969.D
Acq On : 02 Feb 2024 14:52
Operator : SY/MD
Sample : P1348-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

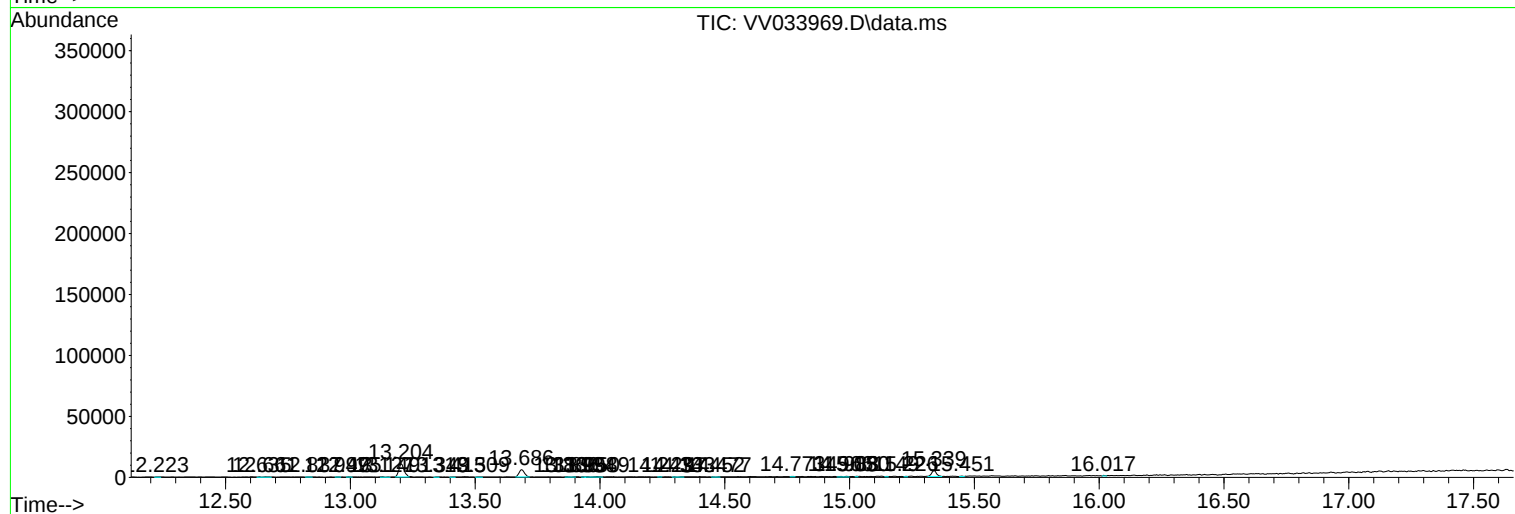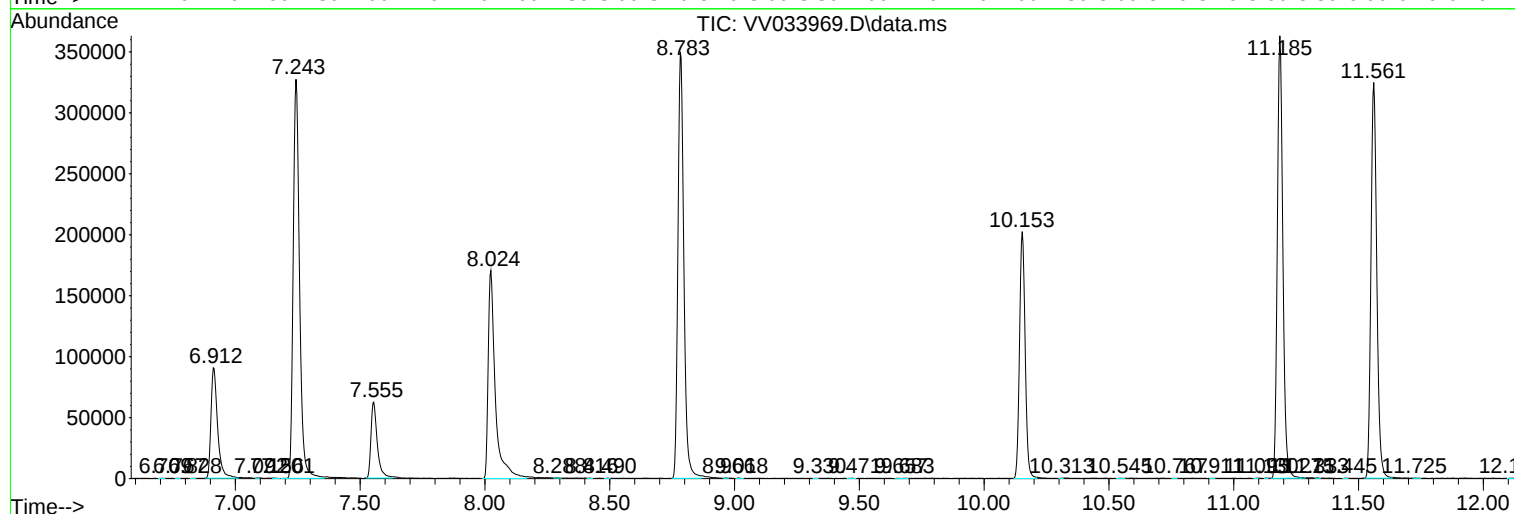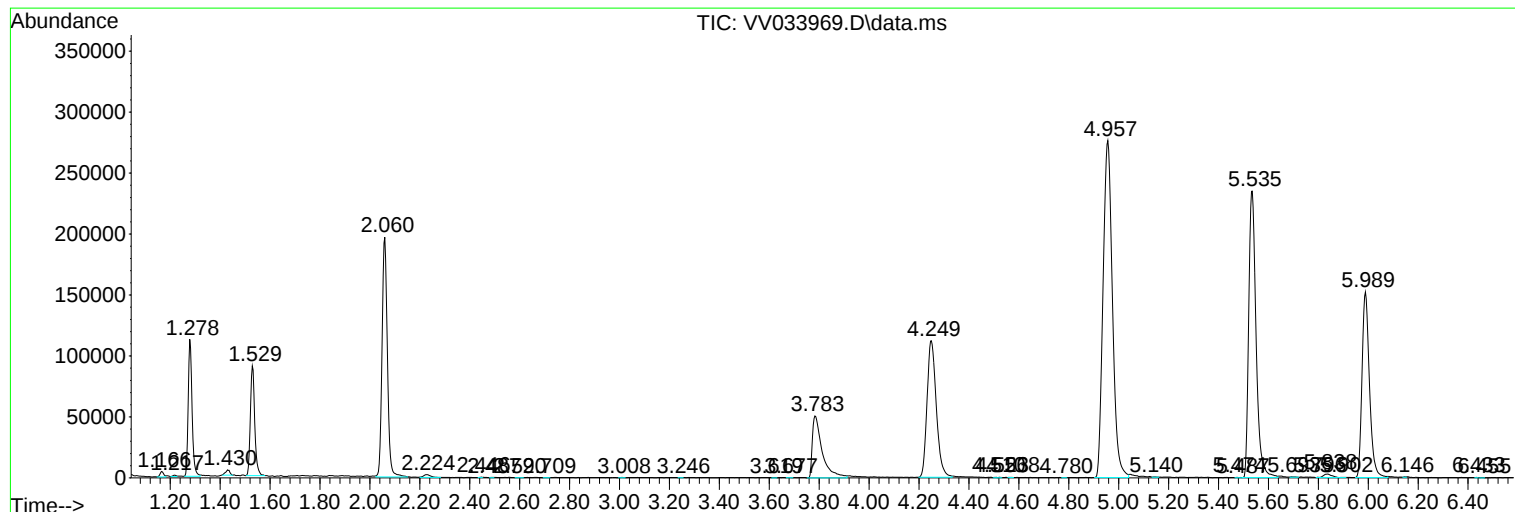

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033969.D
Acq On : 02 Feb 2024 14:52
Operator : SY/MD
Sample : P1348-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033969.D
Acq On : 02 Feb 2024 14:52
Operator : SY/MD
Sample : P1348-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
