

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033970.D
 Acq On : 02 Feb 2024 15:16
 Operator : SY/MD
 Sample : P1348-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	4702	4795	0.68%	0.086%
2	1.217	51	55	59	rBV	883	908	0.13%	0.016%
3	1.278	67	74	91	rBV	109523	116389	16.52%	2.083%
4	1.433	112	122	131	rBV6	4139	7212	1.02%	0.129%
5	1.529	144	152	167	rBV	86299	104086	14.78%	1.863%
6	2.060	306	317	330	rBV	187670	271154	38.49%	4.853%
7	2.182	352	355	360	rBV3	405	400	0.06%	0.007%
8	2.227	360	369	380	rVV2	2224	4028	0.57%	0.072%
9	2.356	404	409	415	rVB2	255	337	0.05%	0.006%
10	2.513	453	458	461	rBV2	300	266	0.04%	0.005%
11	2.552	466	470	474	rBV2	320	291	0.04%	0.005%
12	2.770	531	538	539	rBV2	204	239	0.03%	0.004%
13	2.928	582	587	593	rVB	215	224	0.03%	0.004%
14	3.130	646	650	653	rBV2	243	216	0.03%	0.004%
15	3.230	677	681	684	rBV2	173	185	0.03%	0.003%
16	3.282	694	697	700	rBV2	193	172	0.02%	0.003%
17	3.500	759	765	770	rVB2	334	532	0.08%	0.010%
18	3.523	770	772	775	rBV2	272	239	0.03%	0.004%
19	3.783	845	853	895	rBV	48899	132288	18.78%	2.368%
20	4.127	957	960	961	rBV	250	167	0.02%	0.003%
21	4.249	981	998	1029	rBV	107166	276245	39.22%	4.944%
22	4.355	1029	1031	1034	rBV2	364	201	0.03%	0.004%
23	4.481	1068	1070	1077	rVB3	420	461	0.07%	0.008%
24	4.558	1092	1094	1098	rVB2	323	275	0.04%	0.005%
25	4.580	1098	1101	1105	rBV2	314	316	0.04%	0.006%
26	4.648	1119	1122	1125	rBV2	287	306	0.04%	0.005%
27	4.680	1131	1132	1137	rBV2	232	169	0.02%	0.003%
28	4.728	1142	1147	1151	rVB2	224	246	0.03%	0.004%
29	4.957	1198	1218	1254	rBV2	266171	704405	100.00%	12.607%
30	5.272	1312	1316	1317	rBV	339	231	0.03%	0.004%
31	5.323	1328	1332	1335	rVV	313	316	0.04%	0.006%
32	5.368	1344	1346	1351	rVB2	297	215	0.03%	0.004%
33	5.532	1387	1397	1430	rVV	237108	483889	68.69%	8.660%
34	5.831	1482	1490	1503	rVB3	2781	5741	0.82%	0.103%
35	5.989	1525	1539	1563	rBV	148663	308366	43.78%	5.519%
36	6.706	1757	1762	1766	rBV2	163	219	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033970.D
 Acq On : 02 Feb 2024 15:16
 Operator : SY/MD
 Sample : P1348-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.825	1794	1799	1804	rVB2	231	214	0.03%	0.004%
38	6.915	1817	1827	1850	rBV	88647	163329	23.19%	2.923%
39	7.243	1916	1929	1955	rBV	319756	563625	80.01%	10.088%
40	7.506	2007	2011	2015	rVB2	394	421	0.06%	0.008%
41	7.555	2015	2026	2054	rBV2	60734	111152	15.78%	1.989%
42	7.738	2079	2083	2086	rBV	272	241	0.03%	0.004%
43	7.879	2120	2127	2134	rVB	335	574	0.08%	0.010%
44	7.976	2153	2157	2160	rVB2	294	259	0.04%	0.005%
45	8.024	2160	2172	2211	rBV	166568	332883	47.26%	5.958%
46	8.378	2279	2282	2286	rBV2	219	207	0.03%	0.004%
47	8.584	2342	2346	2348	rBV	170	160	0.02%	0.003%
48	8.783	2398	2408	2437	rBV	354982	588922	83.61%	10.540%
49	9.034	2482	2486	2490	rBV2	154	193	0.03%	0.003%
50	9.217	2538	2543	2544	rBV2	152	157	0.02%	0.003%
51	9.313	2570	2573	2575	rBV	220	182	0.03%	0.003%
52	9.413	2600	2604	2606	rBV	279	299	0.04%	0.005%
53	9.593	2656	2660	2662	rBV2	146	150	0.02%	0.003%
54	9.709	2692	2696	2698	rBV2	173	161	0.02%	0.003%
55	9.789	2716	2721	2726	rBV2	258	296	0.04%	0.005%
56	9.815	2726	2729	2735	rBV2	244	326	0.05%	0.006%
57	9.924	2759	2763	2766	rBV	222	210	0.03%	0.004%
58	10.037	2791	2798	2801	rBV2	250	349	0.05%	0.006%
59	10.063	2801	2806	2812	rBV2	196	312	0.04%	0.006%
60	10.153	2822	2834	2854	rBV	197779	310078	44.02%	5.550%
61	10.223	2854	2856	2862	rVB2	597	427	0.06%	0.008%
62	10.477	2931	2935	2939	rVB	236	240	0.03%	0.004%
63	10.516	2945	2947	2952	rBV	138	154	0.02%	0.003%
64	10.805	3032	3037	3042	rBV2	229	254	0.04%	0.005%
65	11.018	3099	3103	3106	rBV2	200	211	0.03%	0.004%
66	11.108	3129	3131	3135	rVV2	192	146	0.02%	0.003%
67	11.185	3144	3155	3183	rBV	369134	572924	81.33%	10.254%
68	11.310	3192	3194	3198	rVB3	528	362	0.05%	0.006%
69	11.458	3234	3240	3244	rBV2	174	297	0.04%	0.005%
70	11.561	3261	3272	3300	rBV	316814	501497	71.19%	8.976%
71	11.751	3328	3331	3333	rBV2	293	172	0.02%	0.003%
72	11.773	3335	3338	3342	rBV2	169	187	0.03%	0.003%
73	11.850	3359	3362	3367	rVB2	216	189	0.03%	0.003%
74	11.989	3402	3405	3408	rBV2	181	174	0.02%	0.003%
75	12.178	3460	3464	3471	rBV2	219	352	0.05%	0.006%
76	12.262	3486	3490	3493	rVB2	197	173	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033970.D
 Acq On : 02 Feb 2024 15:16
 Operator : SY/MD
 Sample : P1348-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.397	3529	3532	3536	rBV	164	152	0.02%	0.003%
78	12.448	3545	3548	3550	rBV2	189	151	0.02%	0.003%
79	12.863	3674	3677	3680	rBV	261	225	0.03%	0.004%
80	13.085	3743	3746	3750	rBV2	214	225	0.03%	0.004%
81	13.210	3778	3785	3793	rVV4	2011	3039	0.43%	0.054%
82	13.371	3828	3835	3838	rBV2	244	304	0.04%	0.005%
83	13.461	3860	3863	3865	rBV	284	208	0.03%	0.004%
84	13.532	3882	3885	3890	rVB2	252	273	0.04%	0.005%
85	13.564	3890	3895	3898	rBV2	365	364	0.05%	0.007%
86	13.638	3915	3918	3924	rBV2	216	263	0.04%	0.005%
87	13.686	3928	3933	3934	rBV	825	593	0.08%	0.011%
88	13.786	3960	3964	3966	rBV	175	156	0.02%	0.003%
89	13.831	3971	3978	3981	rBV2	329	288	0.04%	0.005%
90	13.879	3988	3993	3995	rBV2	372	321	0.05%	0.006%
91	13.992	4023	4028	4033	rVB3	448	606	0.09%	0.011%
92	14.021	4034	4037	4040	rBV	244	181	0.03%	0.003%
93	14.104	4060	4063	4065	rBV	258	168	0.02%	0.003%
94	14.149	4074	4077	4079	rBV2	269	164	0.02%	0.003%
95	14.304	4123	4125	4128	rVB3	315	182	0.03%	0.003%
96	14.435	4162	4166	4169	rVB2	223	221	0.03%	0.004%
97	14.458	4170	4173	4180	rBV2	247	340	0.05%	0.006%
98	14.525	4189	4194	4198	rBV2	237	346	0.05%	0.006%
99	14.603	4215	4218	4220	rBV2	201	162	0.02%	0.003%
100	14.976	4331	4334	4337	rBV2	279	196	0.03%	0.004%




Sum of corrected areas: 5587316

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033970.D
Acq On : 02 Feb 2024 15:16
Operator : SY/MD
Sample : P1348-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

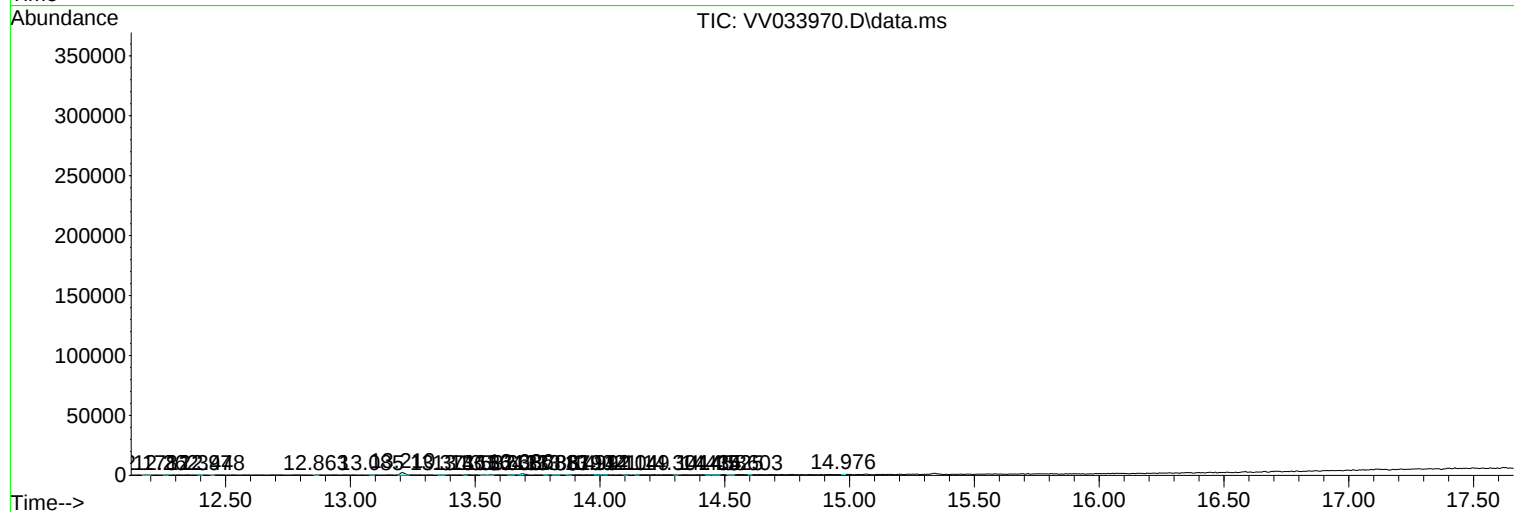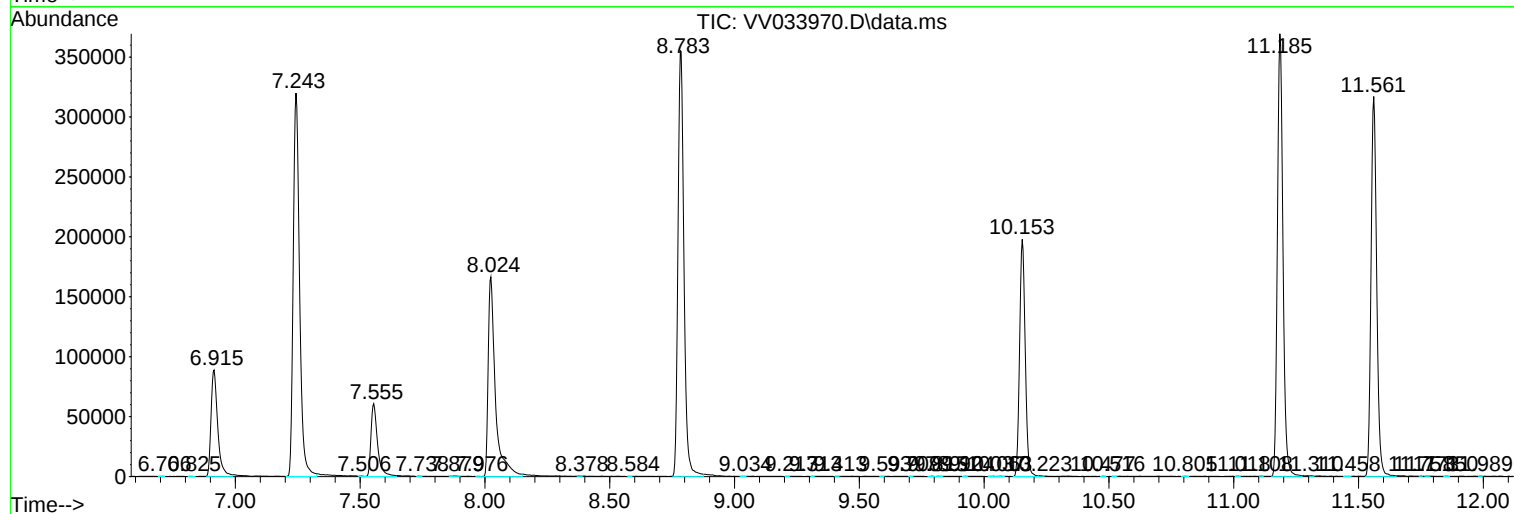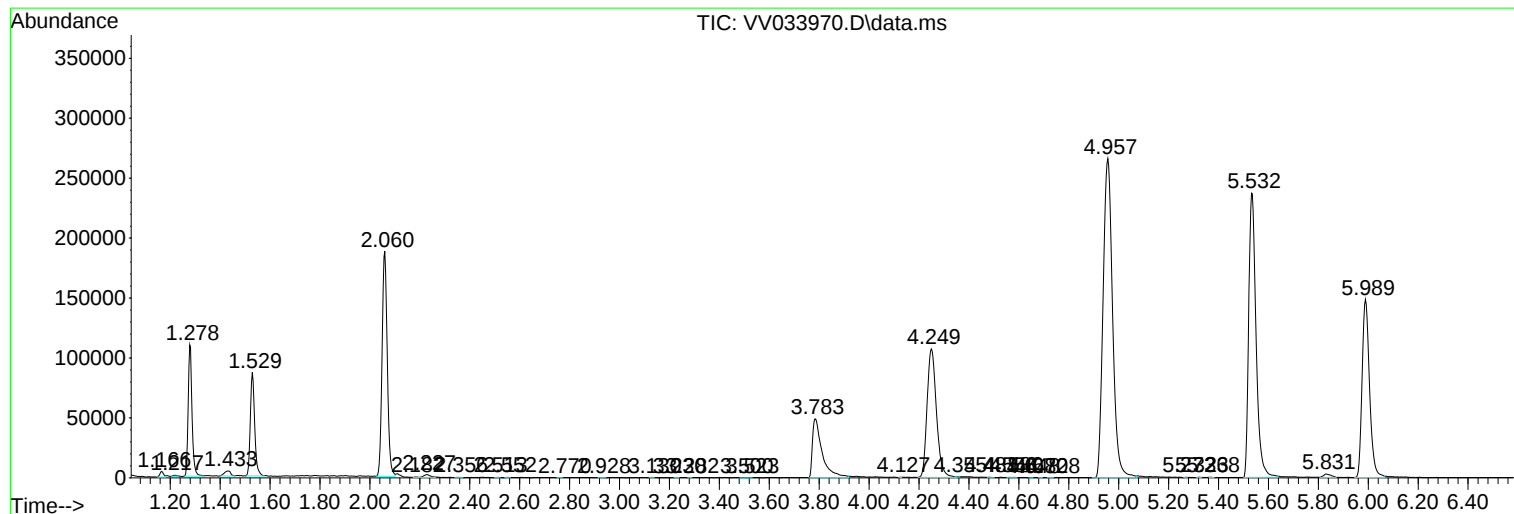

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033970.D
Acq On : 02 Feb 2024 15:16
Operator : SY/MD
Sample : P1348-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033970.D
Acq On : 02 Feb 2024 15:16
Operator : SY/MD
Sample : P1348-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------