

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033974.D
 Acq On : 02 Feb 2024 16:52
 Operator : SY/MD
 Sample : P1348-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	3766	3829	0.53%	0.066%
2	1.278	67	74	97	rBV	109578	118890	16.45%	2.035%
3	1.478	134	136	140	rBV3	777	506	0.07%	0.009%
4	1.529	144	152	175	rVB	89422	110128	15.24%	1.885%
5	1.687	199	201	205	rBV3	679	444	0.06%	0.008%
6	1.921	270	274	278	rBB5	754	671	0.09%	0.011%
7	2.059	306	317	334	rBV	193883	281874	39.01%	4.826%
8	2.281	381	386	390	rBV2	228	260	0.04%	0.004%
9	2.449	431	438	449	rVV3	1507	2474	0.34%	0.042%
10	2.526	459	462	465	rBV2	221	218	0.03%	0.004%
11	2.596	480	484	490	rBV2	251	361	0.05%	0.006%
12	2.674	502	508	510	rBV2	243	282	0.04%	0.005%
13	2.895	571	577	583	rBV2	225	413	0.06%	0.007%
14	3.008	608	612	615	rBV2	175	190	0.03%	0.003%
15	3.185	660	667	675	rVB2	195	351	0.05%	0.006%
16	3.288	695	699	703	rBV2	185	209	0.03%	0.004%
17	3.558	780	783	788	rBV2	206	220	0.03%	0.004%
18	3.600	792	796	798	rBV2	252	217	0.03%	0.004%
19	3.706	826	829	832	rBB	309	228	0.03%	0.004%
20	3.783	845	853	883	rBV	49441	129300	17.90%	2.214%
21	3.976	909	913	916	rBV	337	268	0.04%	0.005%
22	4.249	982	998	1026	rBV	112721	287464	39.79%	4.922%
23	4.436	1053	1056	1061	rVB3	361	289	0.04%	0.005%
24	4.465	1061	1065	1066	rBV2	260	197	0.03%	0.003%
25	4.535	1085	1087	1090	rBV2	317	221	0.03%	0.004%
26	4.863	1184	1189	1192	rBV2	192	246	0.03%	0.004%
27	4.956	1200	1218	1248	rBV2	276467	722525	100.00%	12.370%
28	5.339	1334	1337	1344	rVB3	246	205	0.03%	0.004%
29	5.387	1347	1352	1354	rBV2	313	264	0.04%	0.005%
30	5.426	1360	1364	1367	rBV3	320	256	0.04%	0.004%
31	5.535	1384	1398	1427	rBV	239170	489949	67.81%	8.388%
32	5.837	1483	1492	1505	rVB6	2730	6173	0.85%	0.106%
33	5.892	1505	1509	1513	rVB2	347	280	0.04%	0.005%
34	5.918	1513	1517	1519	rBV	318	215	0.03%	0.004%
35	5.989	1527	1539	1566	rBV	156021	319413	44.21%	5.469%
36	6.178	1596	1598	1603	rVB3	526	371	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020224\
 Data File : VW033974.D
 Acq On : 02 Feb 2024 16:52
 Operator : SY/MD
 Sample : P1348-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.243	1613	1618	1621	rVB2	375	345	0.05%	0.006%
38	6.403	1657	1668	1671	rBV	248	413	0.06%	0.007%
39	6.497	1693	1697	1703	rVB2	182	245	0.03%	0.004%
40	6.538	1707	1710	1712	rBV	253	208	0.03%	0.004%
41	6.638	1738	1741	1745	rBV	182	206	0.03%	0.004%
42	6.696	1756	1759	1763	rBV2	294	358	0.05%	0.006%
43	6.744	1769	1774	1779	rBV2	172	290	0.04%	0.005%
44	6.915	1815	1827	1849	rBV	93613	173331	23.99%	2.968%
45	7.243	1918	1929	1966	rBV	335338	587744	81.35%	10.063%
46	7.487	2002	2005	2009	rBV3	259	261	0.04%	0.004%
47	7.554	2017	2026	2055	rBV	63613	114313	15.82%	1.957%
48	7.789	2097	2099	2104	rVB	252	203	0.03%	0.003%
49	7.927	2137	2142	2145	rBV2	218	267	0.04%	0.005%
50	8.024	2163	2172	2213	rBV	172514	335989	46.50%	5.752%
51	8.355	2272	2275	2279	rBV2	317	347	0.05%	0.006%
52	8.564	2335	2340	2344	rBV2	199	277	0.04%	0.005%
53	8.786	2397	2409	2440	rBV	360563	604859	83.71%	10.356%
54	9.455	2613	2617	2620	rBV	204	219	0.03%	0.004%
55	9.664	2676	2682	2687	rBV	176	253	0.04%	0.004%
56	10.152	2823	2834	2854	rVV	203274	323334	44.75%	5.536%
57	10.326	2880	2888	2892	rBV2	548	821	0.11%	0.014%
58	10.451	2921	2927	2929	rBV2	314	349	0.05%	0.006%
59	10.725	3008	3012	3015	rBV2	192	202	0.03%	0.003%
60	10.776	3021	3028	3030	rBV	232	309	0.04%	0.005%
61	11.130	3133	3138	3145	rBV3	462	577	0.08%	0.010%
62	11.185	3145	3155	3180	rBV	388118	606490	83.94%	10.384%
63	11.561	3260	3272	3294	rBV	344293	551456	76.32%	9.441%
64	11.773	3335	3338	3344	rBV	234	239	0.03%	0.004%
65	11.898	3372	3377	3378	rBV	238	231	0.03%	0.004%
66	12.001	3405	3409	3411	rBV	217	190	0.03%	0.003%
67	12.046	3417	3423	3426	rBV2	221	253	0.04%	0.004%
68	12.117	3441	3445	3448	rBV2	212	221	0.03%	0.004%
69	12.381	3524	3527	3530	rBV2	201	192	0.03%	0.003%
70	12.545	3572	3578	3581	rBV2	258	312	0.04%	0.005%
71	12.574	3581	3587	3590	rBV2	171	243	0.03%	0.004%
72	12.786	3648	3653	3656	rBV	183	201	0.03%	0.003%
73	12.831	3660	3667	3673	rVV4	1629	2043	0.28%	0.035%
74	12.930	3694	3698	3701	rVB2	303	240	0.03%	0.004%
75	13.207	3777	3784	3796	rVB4	4661	7060	0.98%	0.121%
76	13.577	3896	3899	3901	rBV2	526	343	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
 Data File : VV033974.D
 Acq On : 02 Feb 2024 16:52
 Operator : SY/MD
 Sample : P1348-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	13.689	3926	3934	3941	rBV3	1179	1513	0.21%	0.026%
78	13.844	3973	3982	3990	rBV2	5015	6984	0.97%	0.120%
79	13.988	4021	4027	4033	rBV2	628	837	0.12%	0.014%
80	14.043	4041	4044	4047	rBV3	259	226	0.03%	0.004%
81	14.287	4117	4120	4124	rVB2	347	349	0.05%	0.006%
82	14.329	4124	4133	4135	rBV4	744	870	0.12%	0.015%
83	14.390	4149	4152	4155	rBV	286	220	0.03%	0.004%
84	14.532	4194	4196	4200	rVB2	359	209	0.03%	0.004%
85	14.590	4207	4214	4222	rBV5	2376	3556	0.49%	0.061%
86	14.789	4260	4276	4287	rBV6	5875	10387	1.44%	0.178%
87	14.885	4302	4306	4310	rBV3	837	928	0.13%	0.016%
88	14.946	4322	4325	4327	rBV	457	264	0.04%	0.005%
89	15.033	4349	4352	4355	rBV2	432	386	0.05%	0.007%
90	15.233	4410	4414	4416	rBV4	419	310	0.04%	0.005%
91	15.361	4448	4454	4461	rVB6	2313	3386	0.47%	0.058%
92	15.432	4474	4476	4477	rBV	521	236	0.03%	0.004%
93	15.483	4490	4492	4494	rBV2	432	226	0.03%	0.004%
94	15.564	4515	4517	4520	rBV2	465	322	0.04%	0.006%
95	15.599	4524	4528	4529	rVV3	919	613	0.08%	0.010%
96	15.615	4529	4533	4543	rVB7	1926	3010	0.42%	0.052%
97	15.676	4543	4552	4563	rBV6	4189	6181	0.86%	0.106%
98	15.721	4563	4566	4570	rBV3	538	527	0.07%	0.009%
99	15.753	4570	4576	4583	rBV6	2608	3919	0.54%	0.067%
100	15.972	4640	4644	4645	rBV3	686	537	0.07%	0.009%




Sum of corrected areas: 5840831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033974.D
Acq On : 02 Feb 2024 16:52
Operator : SY/MD
Sample : P1348-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

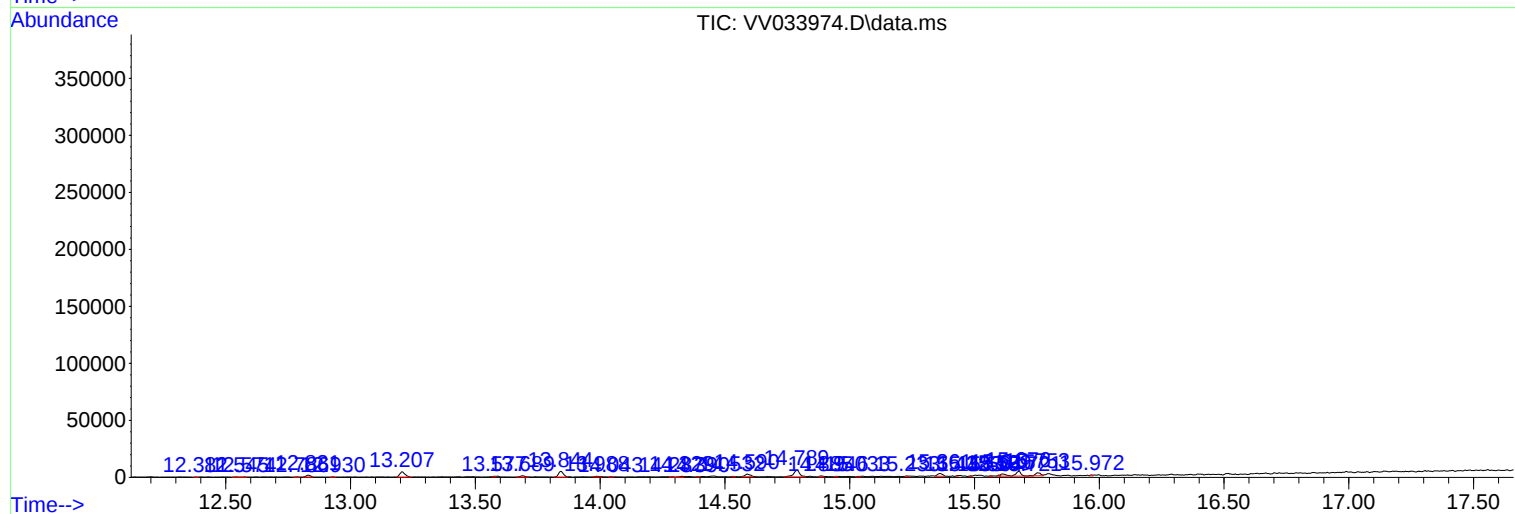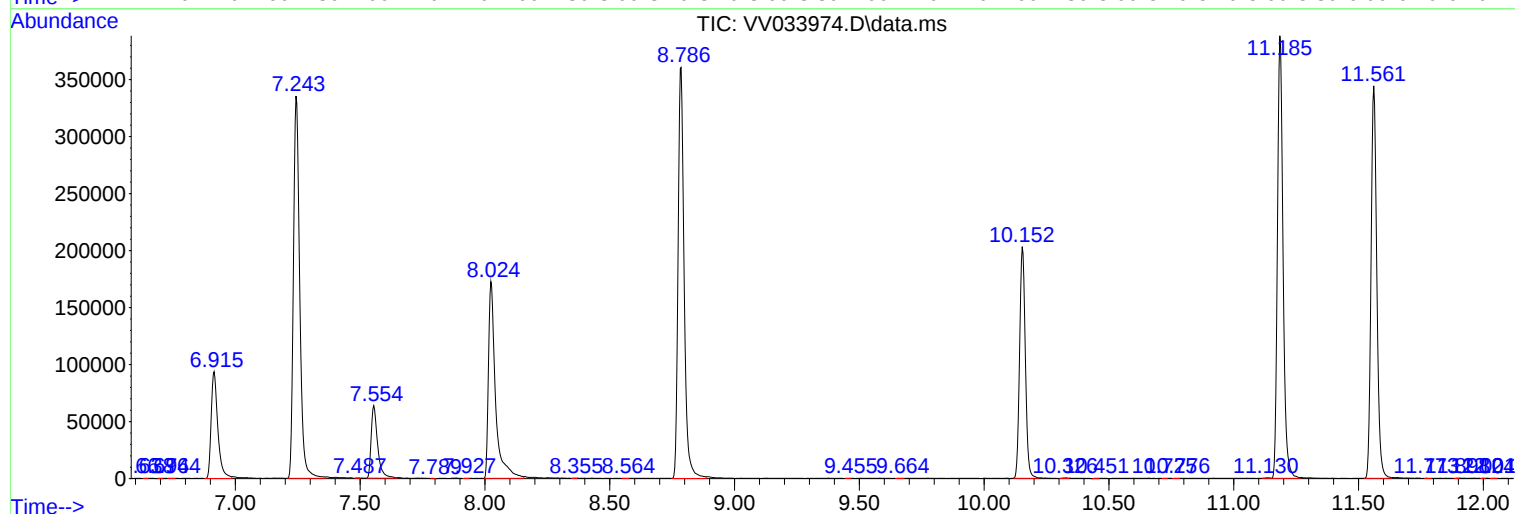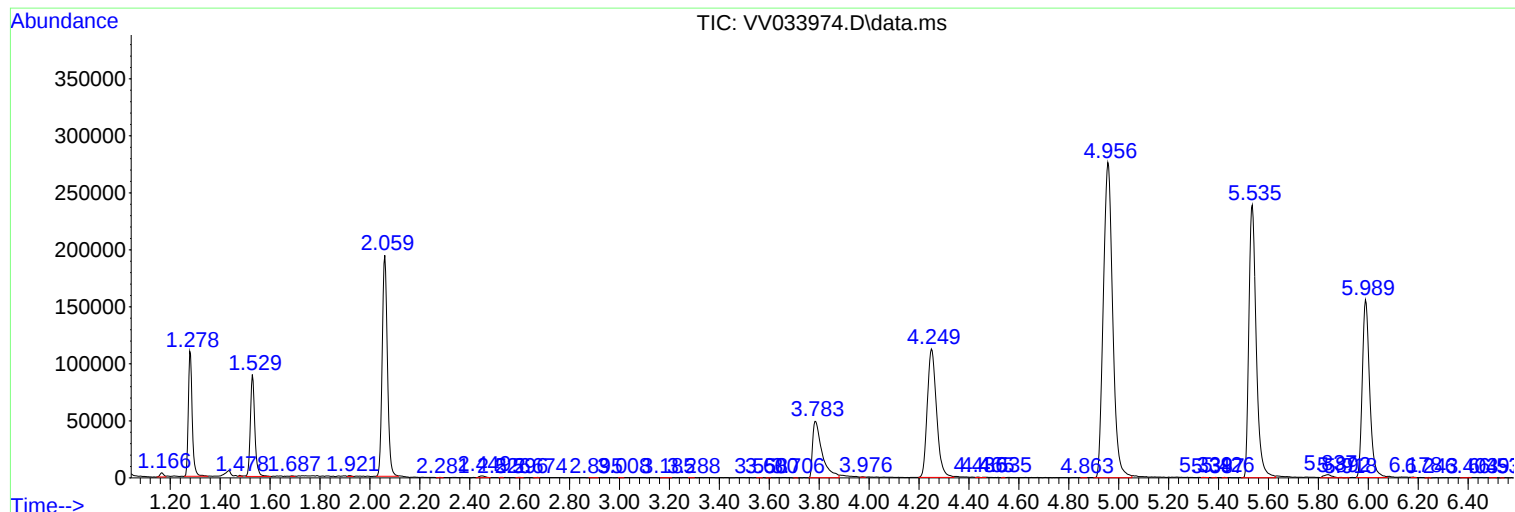

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033974.D
Acq On : 02 Feb 2024 16:52
Operator : SY/MD
Sample : P1348-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020224\
Data File : VV033974.D
Acq On : 02 Feb 2024 16:52
Operator : SY/MD
Sample : P1348-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------