

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014481.D
 Acq On : 03 Feb 2020 11:16
 Operator : SY/MD
 Sample : VV0203MBL01
 Misc : 5.00g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Quant Time: Feb 04 04:55:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 04 04:44:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	447464	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	417116	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	204940	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	112864	45.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.84%
7) Chloroethane-d5	1.59	69	81834	52.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.92%
11) 1,1-Dichloroethene-d2	2.13	63	129525	39.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.08%
21) 2-Butanone-d5	3.92	46	178101	106.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.51%
24) Chloroform-d	4.40	84	255032	48.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.98%
26) 1,2-Dichloroethane-d4	5.08	65	163283	51.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.08%
32) Benzene-d6	5.09	84	545959	49.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.42%
36) 1,2-Dichloropropane-d6	6.11	67	173866	50.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.08%
41) Toluene-d8	7.35	98	504274	49.74	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.48%
43) trans-1,3-Dichloropropene-	7.66	79	90210	51.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	102.16%
47) 2-Hexanone-d5	8.13	63	140339	103.23	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.23%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	217636	48.61	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.22%
64) 1,2-Dichlorobenzene-d4	11.67	152	189722	50.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.52%


Target Compounds					Ovalue
13) Acetone	2.19	43	4367	3.061 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020320\
Data File : VV014481.D
Acq On : 03 Feb 2020 11:16
Operator : SY/MD
Sample : VV0203MBL01
Misc : 5.00µL/5.00mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Time: Feb 04 04:55:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 04 04:44:38 2020
Response via : Initial Calibration

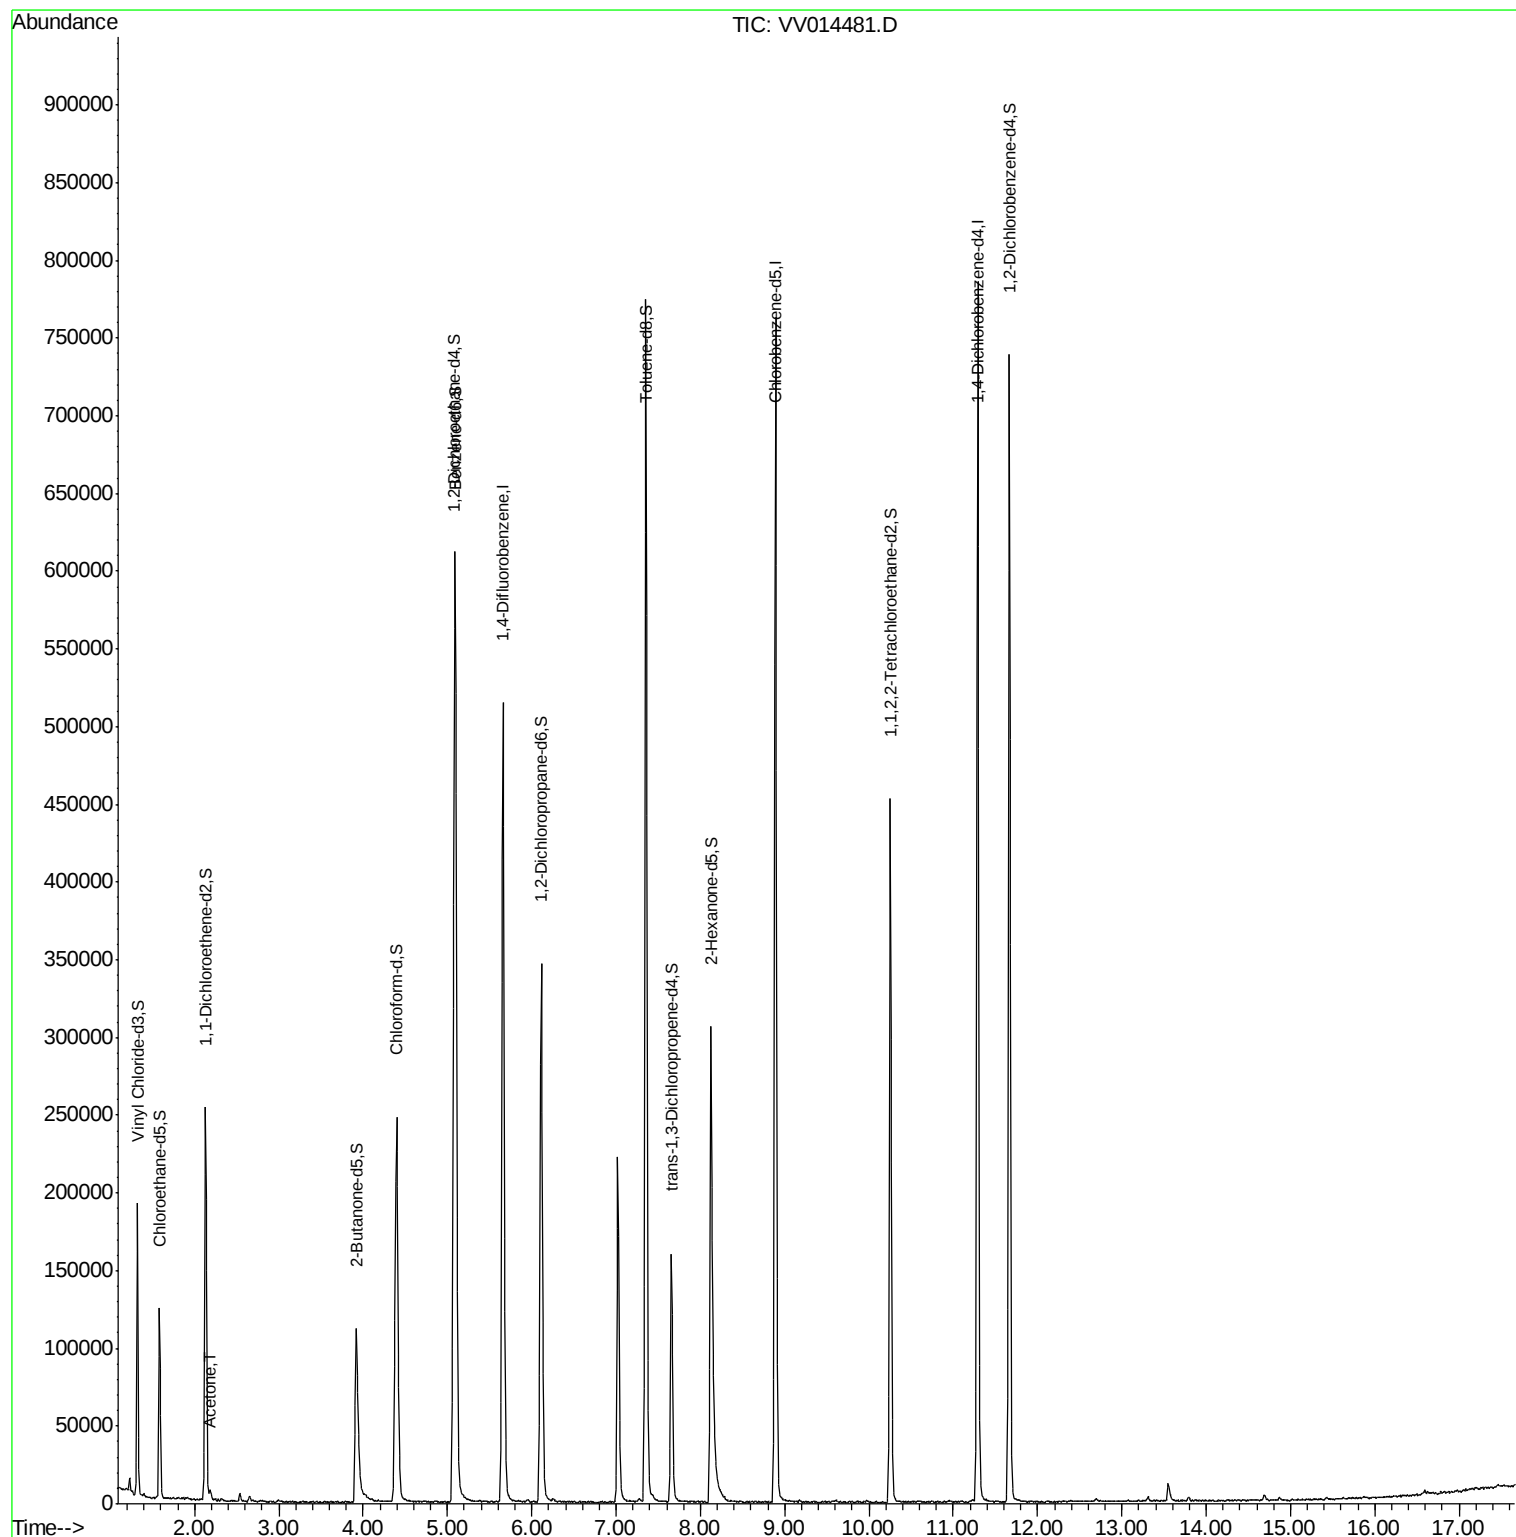

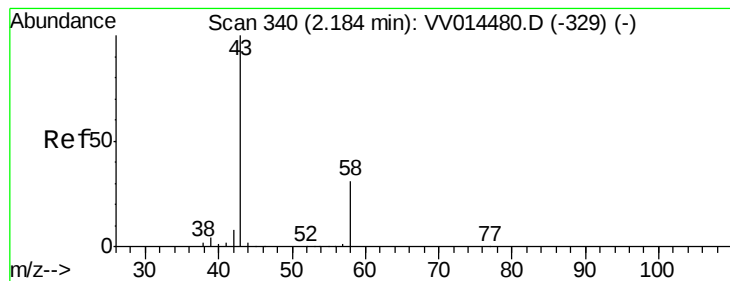

#13

Acetone

Concen: 3.061 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV014481.D

Acq: 03 Feb 2020 11:16

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Tot Ion: 43 Resp: 4367

Ion Ratio Lower Upper

43 100

58 34.0 0.0 61.2

