

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014481.D
 Acq On : 03 Feb 2020 11:16
 Operator : SY/MD
 Sample : VV0203MBL01
 Misc : 5.00µ/5.00mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	85	rVB	187575	188655	12.14%	1.574%
2	1.586	147	154	171	rVB	122585	146695	9.44%	1.224%
3	2.132	314	324	335	rBV	251872	360995	23.22%	3.012%
4	2.476	430	431	432	rBV	794	248	0.02%	0.002%
5	2.595	466	468	473	rVB3	763	415	0.03%	0.003%
6	2.618	473	475	476	rVB	664	241	0.02%	0.002%
7	2.653	476	486	493	rBV5	3344	6396	0.41%	0.053%
8	2.859	548	550	554	rVB4	779	519	0.03%	0.004%
9	2.878	554	556	558	rBV	422	264	0.02%	0.002%
10	2.975	581	586	588	rBV3	749	623	0.04%	0.005%
11	3.058	608	612	616	rBV3	503	495	0.03%	0.004%
12	3.151	637	641	646	rBV6	541	584	0.04%	0.005%
13	3.306	687	689	692	rVB2	544	253	0.02%	0.002%
14	3.331	693	697	701	rVB3	570	478	0.03%	0.004%
15	3.351	701	703	707	rBV2	261	223	0.01%	0.002%
16	3.441	728	731	734	rBV3	513	446	0.03%	0.004%
17	3.540	758	762	764	rVB3	631	432	0.03%	0.004%
18	3.557	764	767	770	rBV2	534	389	0.03%	0.003%
19	3.576	771	773	778	rVB2	576	504	0.03%	0.004%
20	3.608	781	783	784	rBV2	669	249	0.02%	0.002%
21	3.692	806	809	810	rBV2	362	219	0.01%	0.002%
22	3.717	813	817	819	rBV	379	222	0.01%	0.002%
23	3.920	869	880	907	rBV	111742	293252	18.86%	2.447%
24	4.396	1013	1028	1049	rBV	246195	590846	38.01%	4.930%
25	4.553	1073	1077	1080	rBV5	862	718	0.05%	0.006%
26	4.949	1195	1200	1202	rBV2	634	502	0.03%	0.004%
27	5.016	1220	1221	1223	rBV2	498	222	0.01%	0.002%
28	5.090	1226	1244	1273	rBV2	611299	1554543	100.00%	12.972%
29	5.347	1322	1324	1326	rBV3	728	278	0.02%	0.002%
30	5.380	1331	1334	1337	rBV3	1085	845	0.05%	0.007%
31	5.447	1352	1355	1357	rBV3	637	492	0.03%	0.004%
32	5.576	1392	1395	1401	rVB4	754	523	0.03%	0.004%
33	5.601	1401	1403	1405	rBV2	853	478	0.03%	0.004%
34	5.659	1408	1421	1441	rBV	513361	1018794	65.54%	8.501%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014481.D
 Acq On : 03 Feb 2020 11:16
 Operator : SY/MD
 Sample : VV0203MBL01
 Misc : 5.00µ/5.00mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

35	5.839	1475	1477	1482	rVB2	935	551	0.04%	0.005%
36	5.907	1493	1498	1502	rBV6	662	706	0.05%	0.006%
37	5.923	1502	1503	1506	rBV2	783	492	0.03%	0.004%
38	6.045	1539	1541	1543	rVB3	395	219	0.01%	0.002%
39	6.113	1548	1562	1589	rVV	346367	707965	45.54%	5.908%
40	6.470	1669	1673	1676	rVB4	549	503	0.03%	0.004%
41	6.486	1676	1678	1679	rBV4	542	234	0.02%	0.002%
42	6.566	1700	1703	1704	rBV	665	437	0.03%	0.004%
43	6.662	1728	1733	1734	rBV3	573	537	0.03%	0.004%
44	6.695	1739	1743	1746	rVB2	821	623	0.04%	0.005%
45	6.717	1746	1750	1752	rVB3	425	289	0.02%	0.002%
46	6.769	1762	1766	1768	rBV	330	251	0.02%	0.002%
47	6.814	1777	1780	1783	rBV2	558	408	0.03%	0.003%
48	6.868	1794	1797	1801	rVB3	603	441	0.03%	0.004%
49	6.926	1809	1815	1817	rBV3	623	650	0.04%	0.005%
50	6.962	1822	1826	1829	rVB3	539	315	0.02%	0.003%
51	7.023	1831	1845	1872	rBV	222396	399128	25.67%	3.331%
52	7.228	1907	1909	1911	rBV3	484	251	0.02%	0.002%
53	7.354	1935	1948	1967	rBV	772768	1324183	85.18%	11.050%
54	7.656	2030	2042	2061	rBV	159920	272806	17.55%	2.276%
55	7.923	2124	2125	2130	rVB3	516	353	0.02%	0.003%
56	7.949	2131	2133	2135	rBV	514	249	0.02%	0.002%
57	8.006	2149	2151	2153	rBV2	458	282	0.02%	0.002%
58	8.048	2161	2164	2169	rVB4	601	572	0.04%	0.005%
59	8.071	2169	2171	2175	rVB2	363	210	0.01%	0.002%
60	8.125	2175	2188	2234	rBV	306159	702475	45.19%	5.862%
61	8.685	2360	2362	2366	rVB2	593	280	0.02%	0.002%
62	8.704	2366	2368	2374	rVB3	697	655	0.04%	0.005%
63	8.736	2374	2378	2382	rBV3	596	532	0.03%	0.004%
64	8.810	2397	2401	2402	rBV2	500	285	0.02%	0.002%
65	8.891	2412	2426	2444	rBV	762577	1234474	79.41%	10.301%
66	9.122	2496	2498	2501	rBV2	661	509	0.03%	0.004%
67	9.174	2509	2514	2525	rVB4	1318	2296	0.15%	0.019%
68	9.219	2525	2528	2531	rBV2	388	223	0.01%	0.002%
69	9.244	2533	2536	2540	rVB4	417	358	0.02%	0.003%
70	9.267	2540	2543	2546	rVB3	589	325	0.02%	0.003%
71	9.283	2546	2548	2552	rBV2	701	362	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014481.D
 Acq On : 03 Feb 2020 11:16
 Operator : SY/MD
 Sample : VV0203MBL01
 Misc : 5.00µ/5.00mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

72	9.331	2561	2563	2566	rBV3	689	488	0.03%	0.004%
73	9.415	2585	2589	2594	rBV4	501	575	0.04%	0.005%
74	9.437	2594	2596	2597	rBV	475	212	0.01%	0.002%
75	9.656	2659	2664	2668	rBV3	695	779	0.05%	0.007%
76	9.698	2675	2677	2680	rBV2	450	274	0.02%	0.002%
77	9.852	2720	2725	2727	rBV3	725	589	0.04%	0.005%
78	9.865	2727	2729	2732	rVB2	902	488	0.03%	0.004%
79	9.936	2749	2751	2753	rBV2	462	256	0.02%	0.002%
80	9.971	2758	2762	2768	rVV7	910	1260	0.08%	0.011%
81	10.039	2780	2783	2786	rBV	460	286	0.02%	0.002%
82	10.161	2819	2821	2826	rVB2	589	348	0.02%	0.003%
83	10.254	2837	2850	2874	rBV	452819	706371	45.44%	5.894%
84	10.415	2898	2900	2904	rVB	483	216	0.01%	0.002%
85	10.434	2904	2906	2908	rBV2	419	216	0.01%	0.002%
86	10.502	2925	2927	2929	rBV	564	325	0.02%	0.003%
87	10.566	2942	2947	2948	rBV3	734	546	0.04%	0.005%
88	10.682	2981	2983	2988	rBV3	840	575	0.04%	0.005%
89	10.743	2996	3002	3006	rBV3	854	938	0.06%	0.008%
90	10.817	3020	3025	3026	rBV2	452	401	0.03%	0.003%
91	10.881	3042	3045	3048	rBV2	438	374	0.02%	0.003%
92	11.151	3127	3129	3133	rVB3	615	366	0.02%	0.003%
93	11.186	3138	3140	3142	rBV2	584	344	0.02%	0.003%
94	11.289	3160	3172	3190	rBV	784981	1248540	80.32%	10.418%
95	11.498	3235	3237	3239	rBV	558	279	0.02%	0.002%
96	11.601	3266	3269	3270	rBV	729	402	0.03%	0.003%
97	11.665	3276	3289	3306	rBV	738180	1172044	75.39%	9.780%
98	11.846	3341	3345	3347	rBV4	644	523	0.03%	0.004%
99	12.383	3510	3512	3513	rBV	573	262	0.02%	0.002%
100	13.550	3868	3875	3889	rBV2	11076	19239	1.24%	0.161%


Sum of corrected areas: 11983983

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020320\
Data File : VV014481.D
Acq On : 03 Feb 2020 11:16
Operator : SY/MD
Sample : VV0203MBL01
Misc : 5.00µ/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

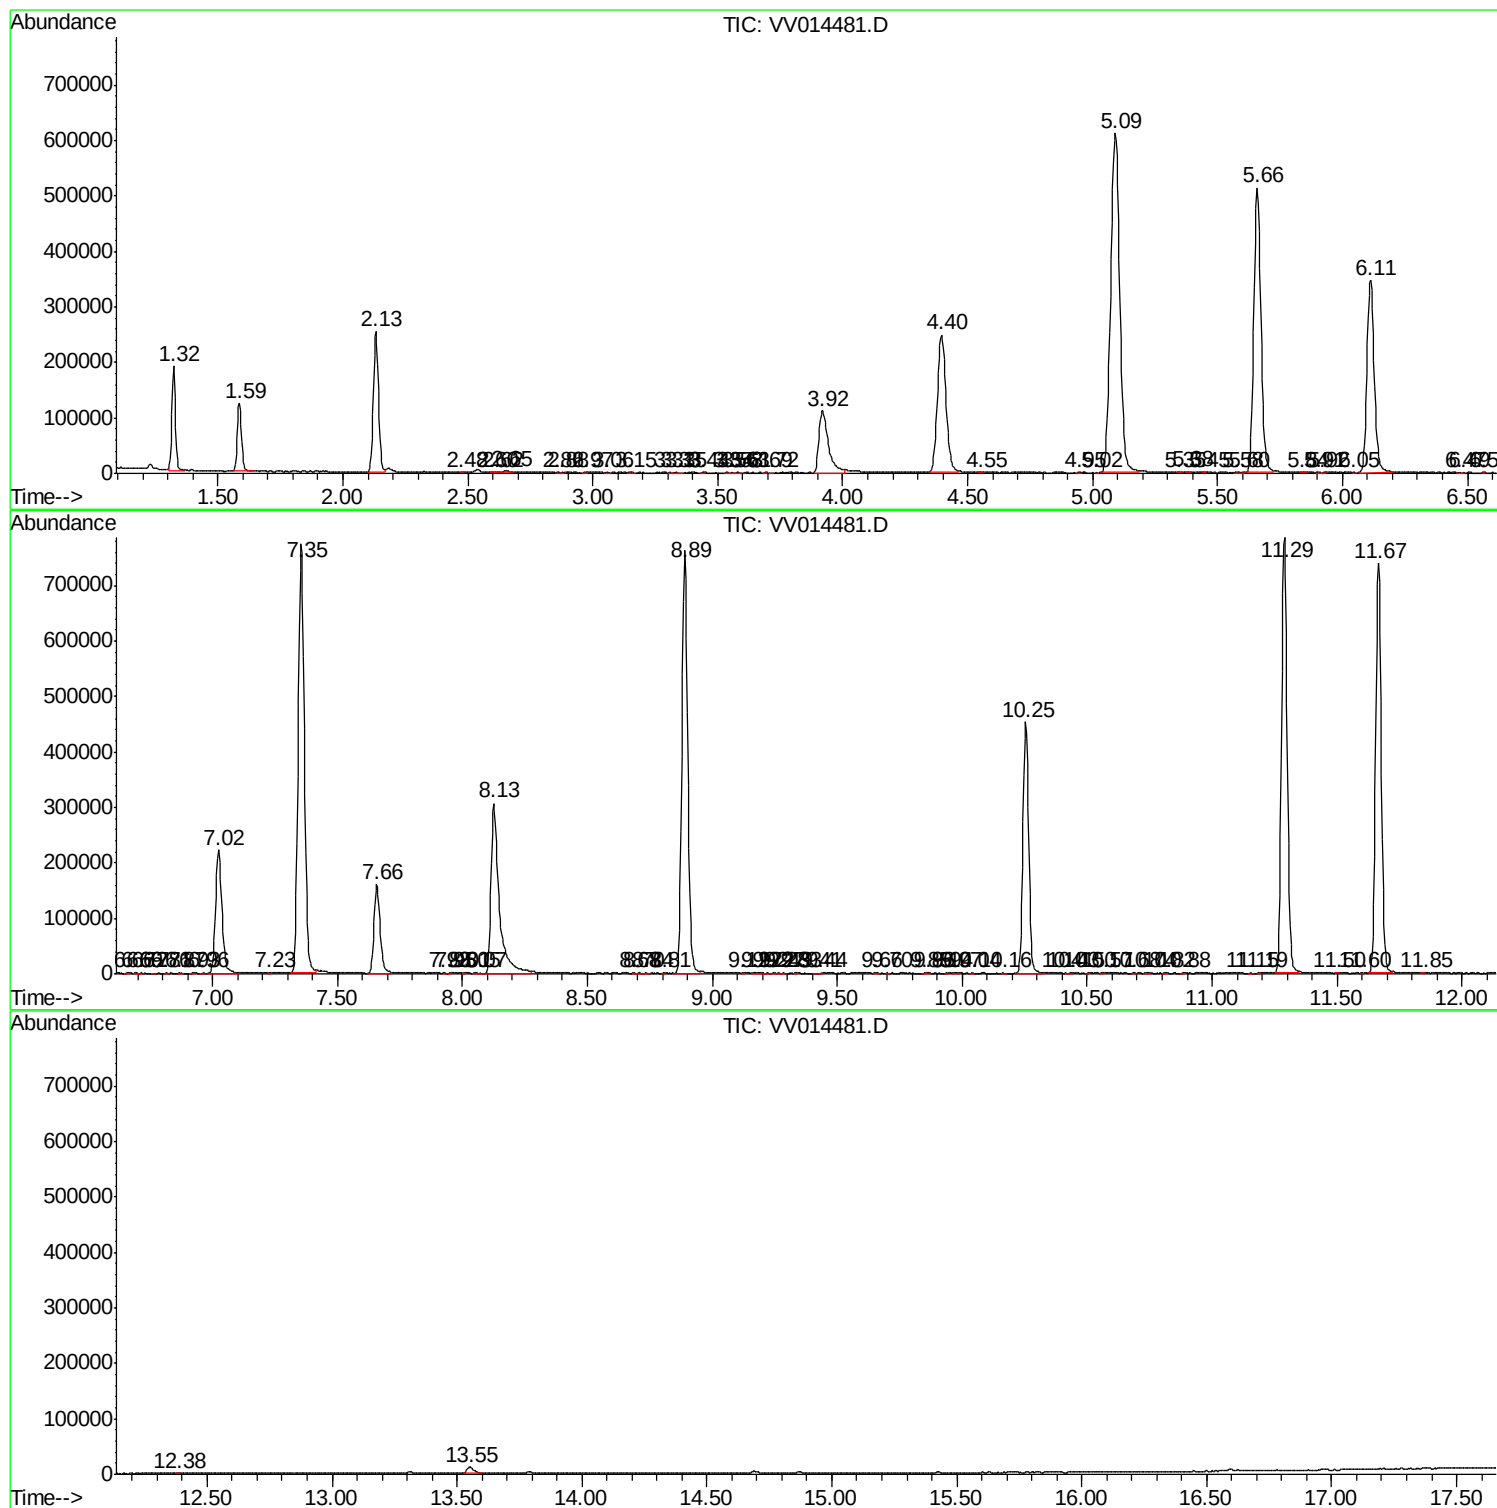

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020320\
Data File : VV014481.D
Acq On : 03 Feb 2020 11:16
Operator : SY/MD
Sample : VV0203MBL01
Misc : 5.00g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020320\
Data File : VV014481.D
Acq On : 03 Feb 2020 11:16
Operator : SY/MD
Sample : VV0203MBL01
Misc : 5.00g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc